

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091724AL\
 Data File : FE050140.D
 Signal(s) : FID1B.ch
 Acq On : 17 Sep 2024 09:41
 Operator : YP\AJ
 Sample : P3989-07DL 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 18 01:26:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 091024.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 17:11:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.875	1982694	13.326 ug/ml
Spiked Amount 50.000		Recovery =	26.65%
12) S 1-chlorooctadecane (S...	13.310	1502062	13.372 ug/ml
Spiked Amount 50.000		Recovery =	26.74%
Target Compounds			
14) T n-Tetracosane (C24)	15.163	50783	0.389 ug/ml
16) T n-Octacosane (C28)	17.131	64798	0.503 ug/ml
17) T n-Tricontane (C30)	18.017	93827	0.702 ug/ml
18) T n-Dotriacontane (C32)	18.849	92500	0.694 ug/ml
19) T n-Tetratriacontane (C34)	19.632	64981	0.526 ug/ml
20) T n-Hexatriacontane (C36)	20.372	70536	0.636 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091724AL\
Data File : FE050140.D
Signal(s) : FID1B.ch
Acq On : 17 Sep 2024 09:41
Operator : YP\AJ
Sample : P3989-07DL 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 18 01:26:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 091024.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 17:11:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

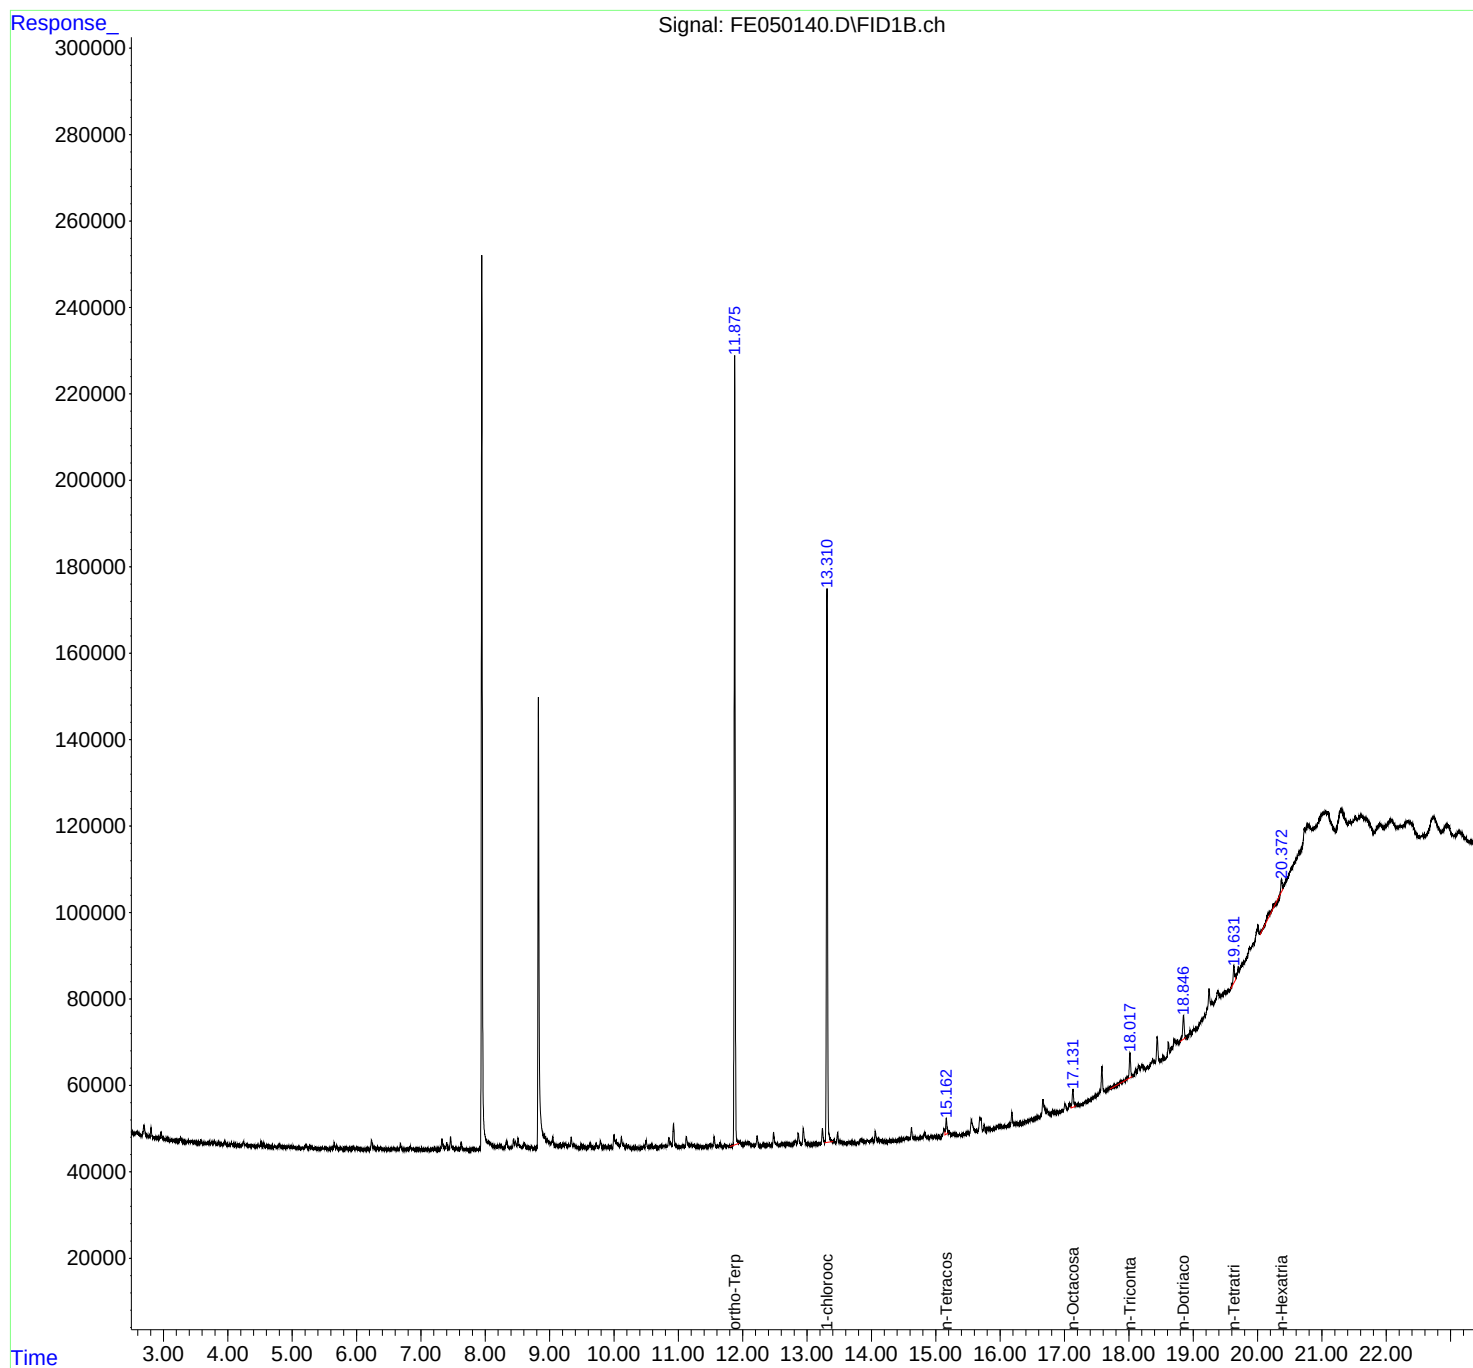


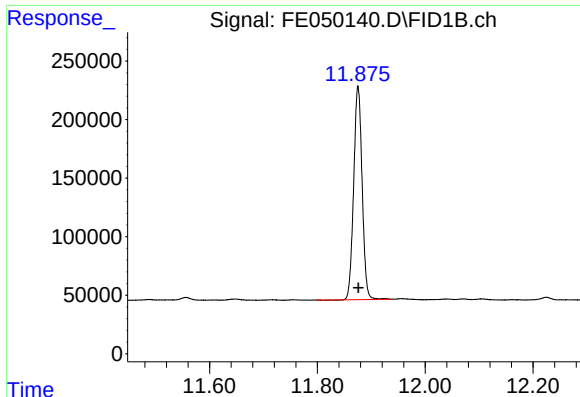

#9 ortho-Terphenyl (SURR)


R.T.: 11.875 min
Delta R.T.: -0.001 min
Response: 1982694
Conc: 13.33 ug/ml

Instrument :
FID_E
ClientSampleId :

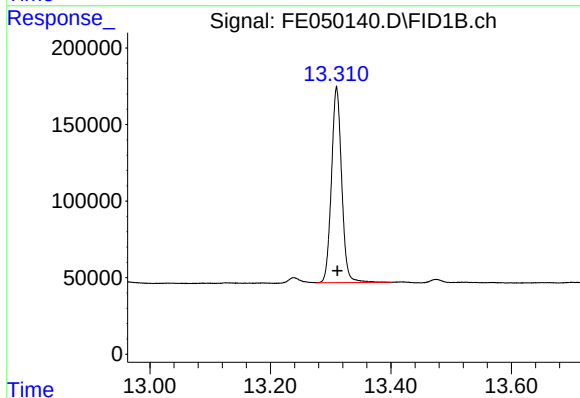


#12 1-chlorooctadecane (SURR)

R.T.: 13.310 min
Delta R.T.: -0.002 min
Response: 1502062
Conc: 13.37 ug/ml

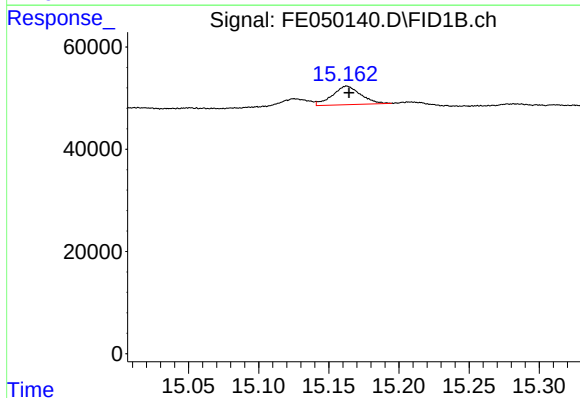


#14 n-Tetracosane (C24)

R.T.: 15.163 min
Delta R.T.: -0.001 min
Response: 50783
Conc: 0.39 ug/ml

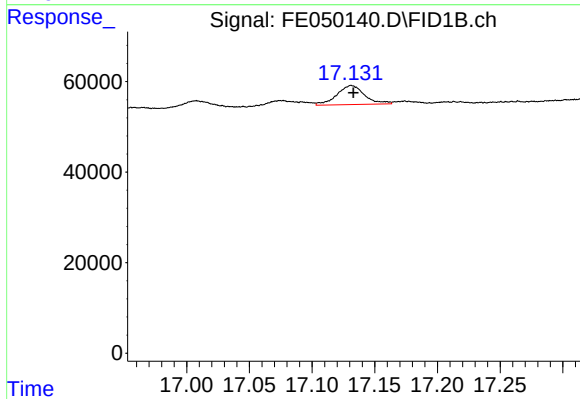

#16 n-Octacosane (C28)


R.T.: 17.131 min
Delta R.T.: -0.002 min
Response: 64798
Conc: 0.50 ug/ml

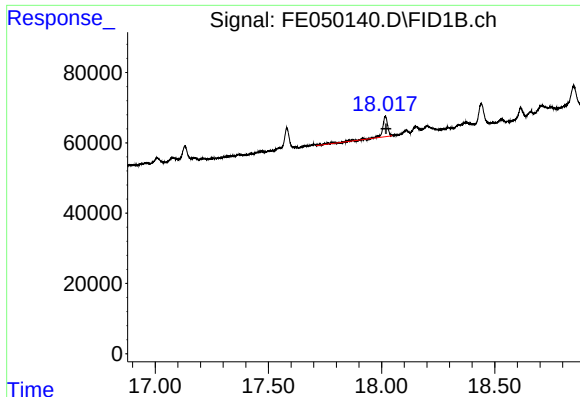

#17 n-Tricontane (C30)


R.T.: 18.017 min
Delta R.T.: -0.003 min
Response: 93827
Conc: 0.70 ug/ml

Instrument :
FID_E
ClientSampleId :

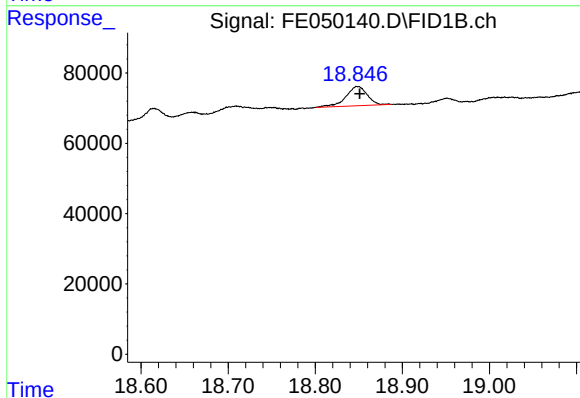


#18 n-Dotriacontane (C32)

R.T.: 18.849 min
Delta R.T.: -0.002 min
Response: 92500
Conc: 0.69 ug/ml

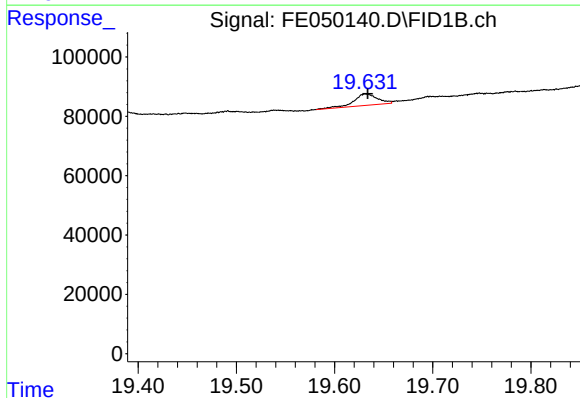

#19 n-Tetratriacontane (C34)

R.T.: 19.632 min
Delta R.T.: -0.002 min
Response: 64981
Conc: 0.53 ug/ml

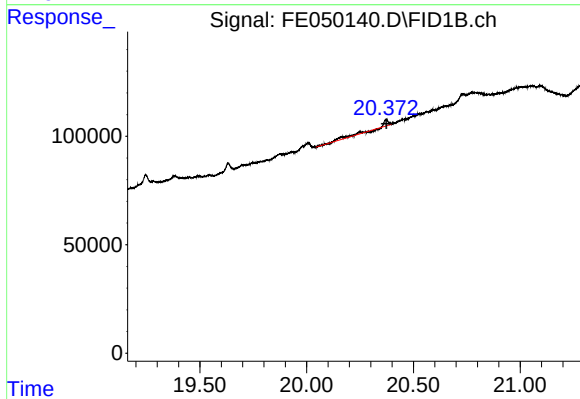

#20 n-Hexatriacontane (C36)

R.T.: 20.372 min
Delta R.T.: -0.001 min
Response: 70536
Conc: 0.64 ug/ml