

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE091724AL\  
 Data File : FE050156.D  
 Signal(s) : FID1B.ch  
 Acq On : 17 Sep 2024 18:15  
 Operator : YP\AJ  
 Sample : P4023-02  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 TP-9-E2

Integration File: autoint1.e  
 Quant Time: Sep 18 01:28:24 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 091024.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Sep 09 17:11:47 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units   |
|--------------------------------|--------|----------|--------------|
| -----                          |        |          |              |
| System Monitoring Compounds    |        |          |              |
| 9) S ortho-Terphenyl (SURR)    | 11.875 | 5433794  | 36.522 ug/ml |
| Spiked Amount                  | 50.000 | Recovery | = 73.04%     |
| 12) S 1-chlorooctadecane (S... | 13.309 | 4318379  | 38.445 ug/ml |
| Spiked Amount                  | 50.000 | Recovery | = 76.89%     |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE091724AL\  
Data File : FE050156.D  
Signal(s) : FID1B.ch  
Acq On : 17 Sep 2024 18:15  
Operator : YP\AJ  
Sample : P4023-02  
Misc :  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
TP-9-E2

Integration File: autoint1.e  
Quant Time: Sep 18 01:28:24 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 091024.M  
Quant Title : GC Extractables  
QLast Update : Mon Sep 09 17:11:47 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

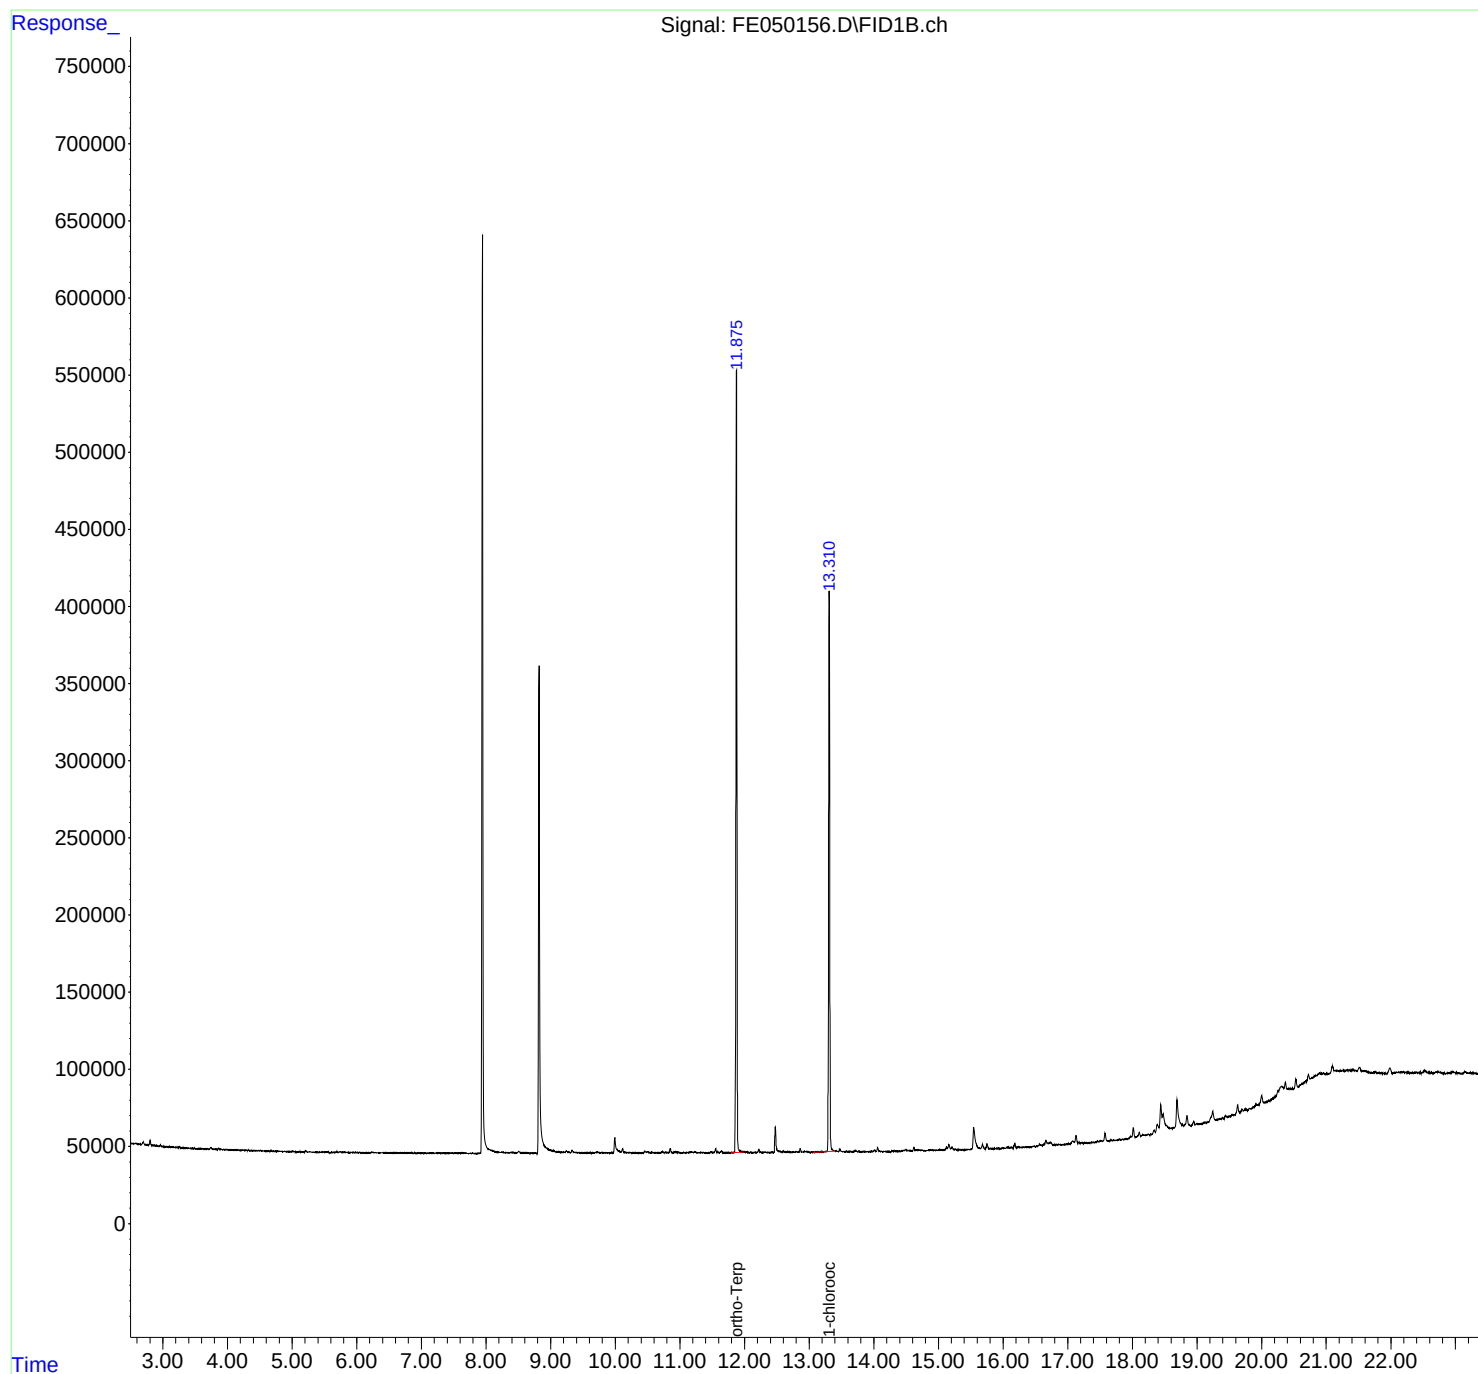


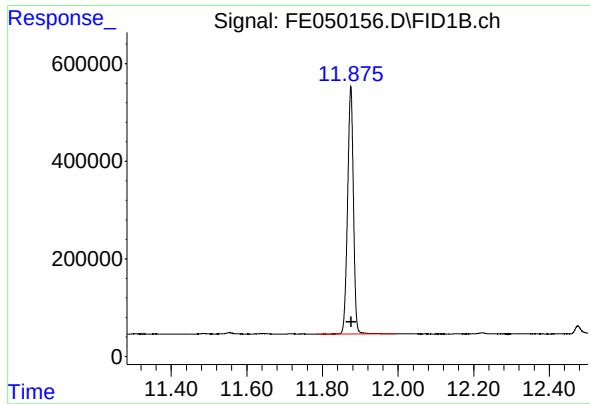

#9 ortho-Terphenyl (SURR)

R.T.: 11.875 min  
Delta R.T.: -0.002 min  
Response: 5433794  
Conc: 36.52 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
TP-9-E2

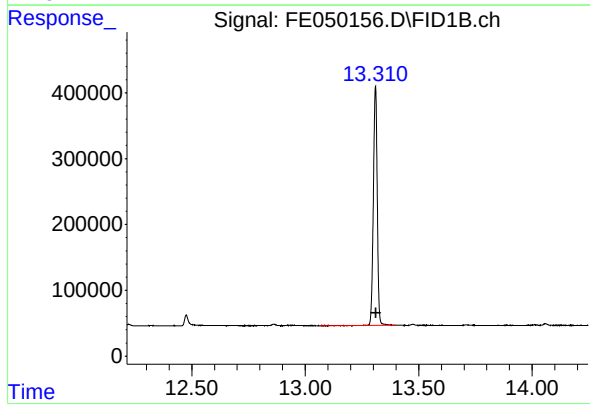

#12 1-chlorooctadecane (SURR)

R.T.: 13.309 min  
Delta R.T.: -0.002 min  
Response: 4318379  
Conc: 38.44 ug/ml