

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091725\
 Data File : FB032201.D
 Signal(s) : FID2B.CH
 Acq On : 17 Sep 2025 13:13
 Operator : YP/AJ
 Sample : BSF0917S2
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 BSF0917S2

Integration File: Calibration.e
 Quant Time: Sep 18 04:07:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082125.M
 Quant Title :
 QLast Update : Thu Aug 21 10:58:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	356692	20.726 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	746874	32.623 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	835376	32.633 ng/ml
3) t n-Heptane	7.756	267353	10.862 ng/ml
4) t Benzene	7.895	321380	10.098 ng/ml
6) t Toluene	10.626	988799	30.147 ng/ml
7) t Ethylbenzene	13.062	288282	9.928 ng/ml
8) t m-Xylene	13.194	601277	20.083 ng/ml
9) t O-Xylene	13.922	576163	20.155 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	495846	19.075 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091725\
Data File : FB032201.D
Signal(s) : FID2B.CH
Acq On : 17 Sep 2025 13:13
Operator : YP/AJ
Sample : BSF0917S2
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
BSF0917S2

Integration File: Calibration.e
Quant Time: Sep 18 04:07:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082125.M
Quant Title :
QLast Update : Thu Aug 21 10:58:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

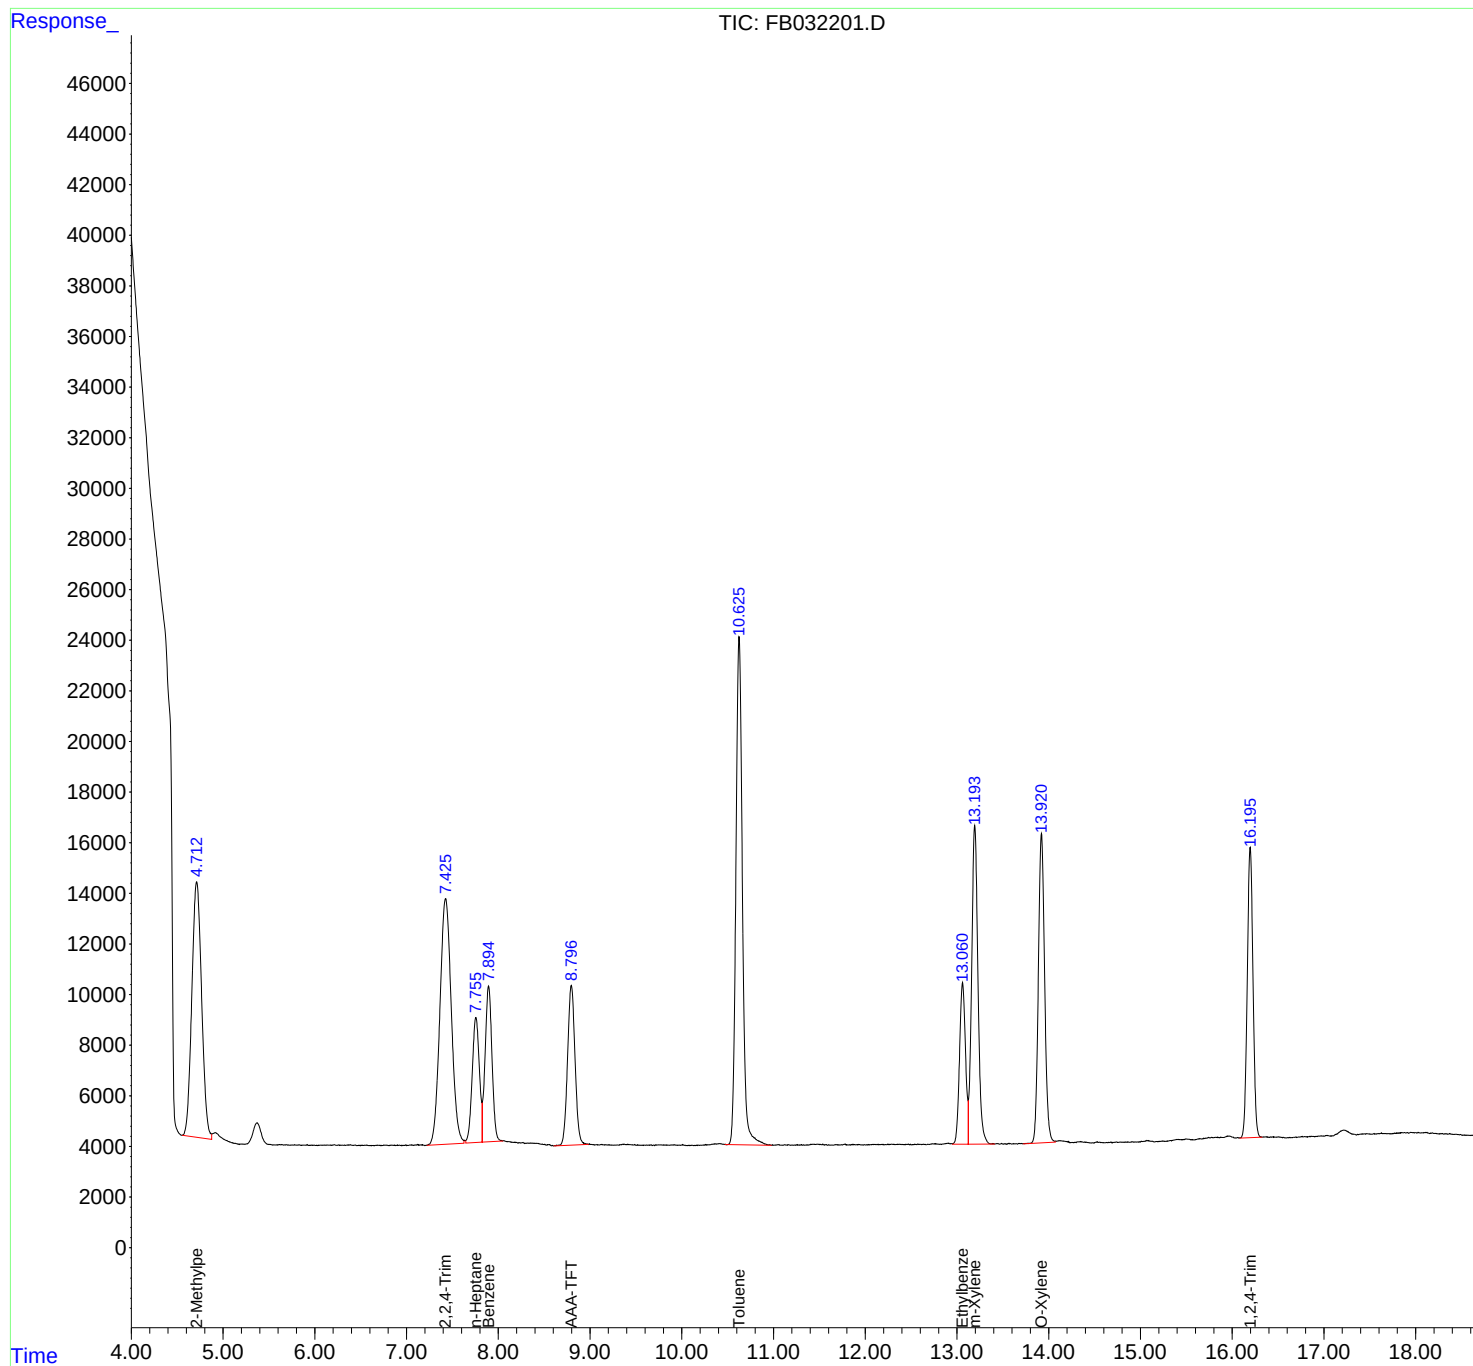


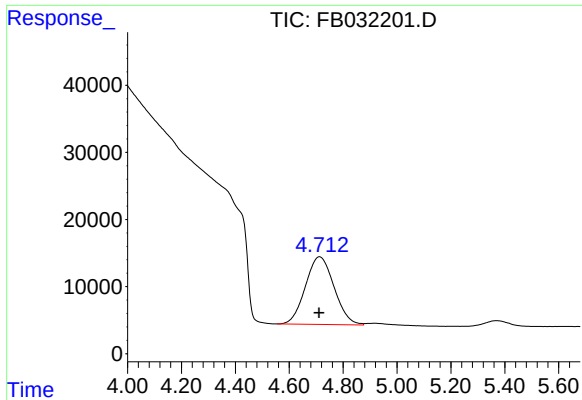

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.002 min
Response: 746874
Conc: 32.62 ng/ml

Instrument :
FID_E
ClientSampleId :
BSF0917S2

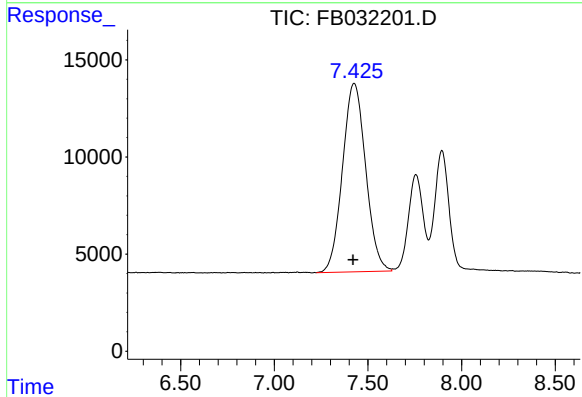


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: 0.005 min
Response: 835376
Conc: 32.63 ng/ml

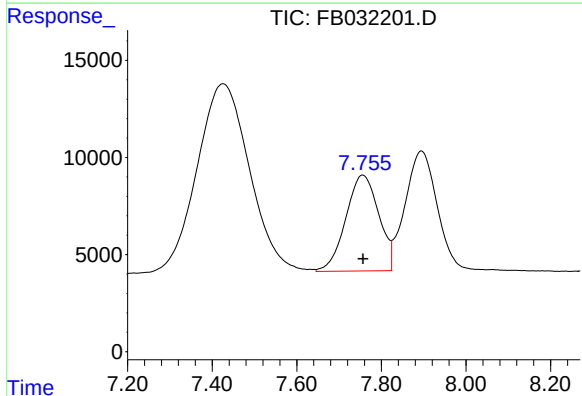


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 267353
Conc: 10.86 ng/ml

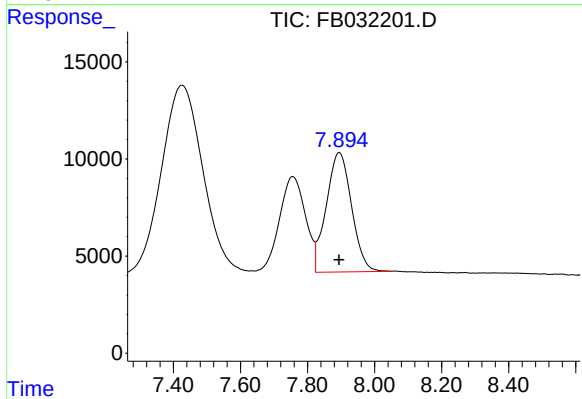

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 321380
Conc: 10.10 ng/ml

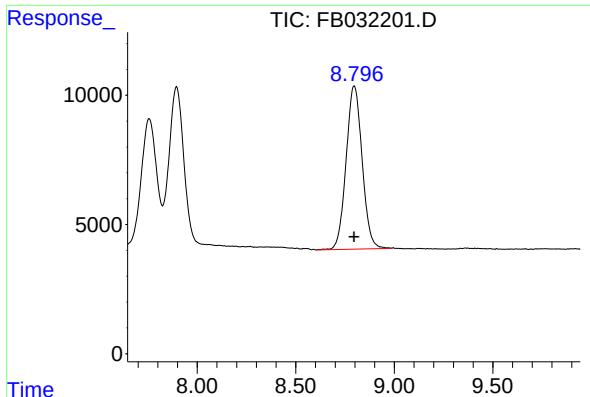

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 356692
Conc: 20.73 ng/ml

Instrument :
FID_E
ClientSampleId :
BSF0917S2

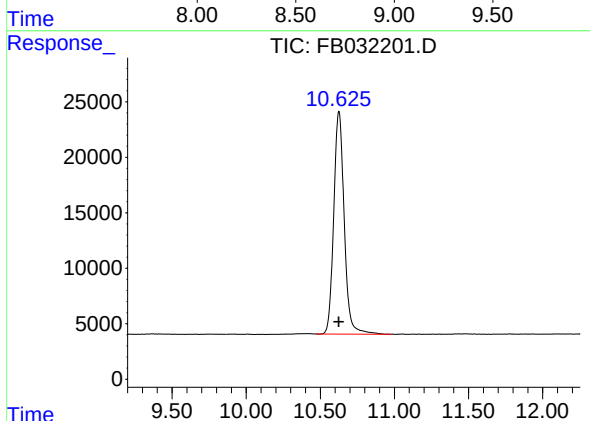


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.001 min
Response: 988799
Conc: 30.15 ng/ml

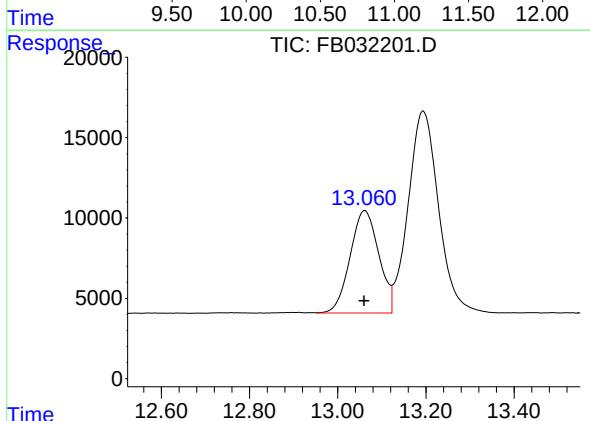


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.002 min
Response: 288282
Conc: 9.93 ng/ml

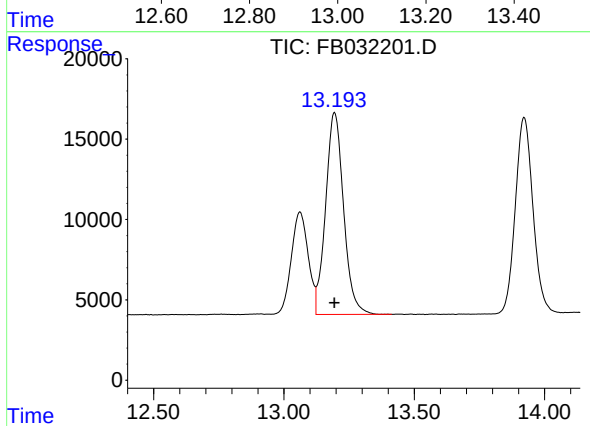

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.000 min
Response: 601277
Conc: 20.08 ng/ml

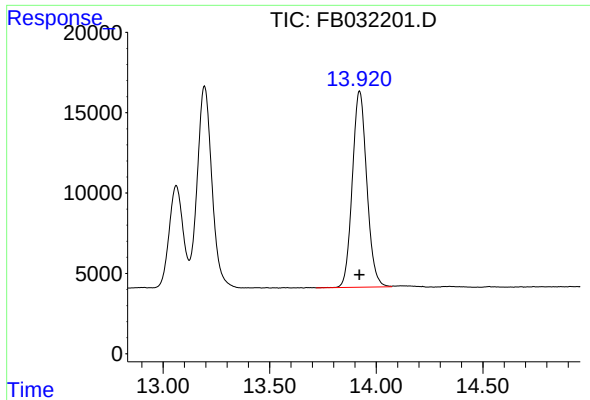

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.001 min
Response: 576163
Conc: 20.15 ng/ml

Instrument :
FID_E
ClientSampleId :
BSF0917S2

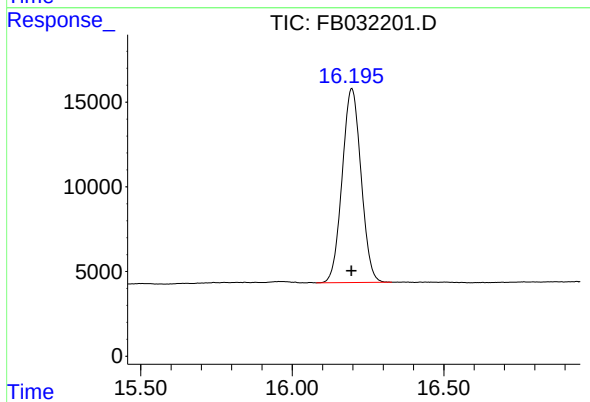

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.001 min
Response: 495846
Conc: 19.08 ng/ml