

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091818\
Data File : FE028672.D
Signal(s) : FID1B.CH
Acq On : 18 Sep 2018 10:20
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 19 03:24:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
Quant Title :
QLast Update : Tue Aug 21 14:35:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
5)	N-DODECANE	6.677	4068035	26.996 ug/ml
11)	N-OCTACOSANE	17.151	3850813	17.323 ug/ml
12)	N-DOTRIACONTANE	18.872	293564	1.601 ug/ml
14)	N-HEXATRIACONTANE	20.402	146245	1.110 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091818\
Data File : FE028672.D
Signal(s) : FID1B.CH
Acq On : 18 Sep 2018 10:20
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 19 03:24:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
Quant Title :
QLast Update : Tue Aug 21 14:35:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

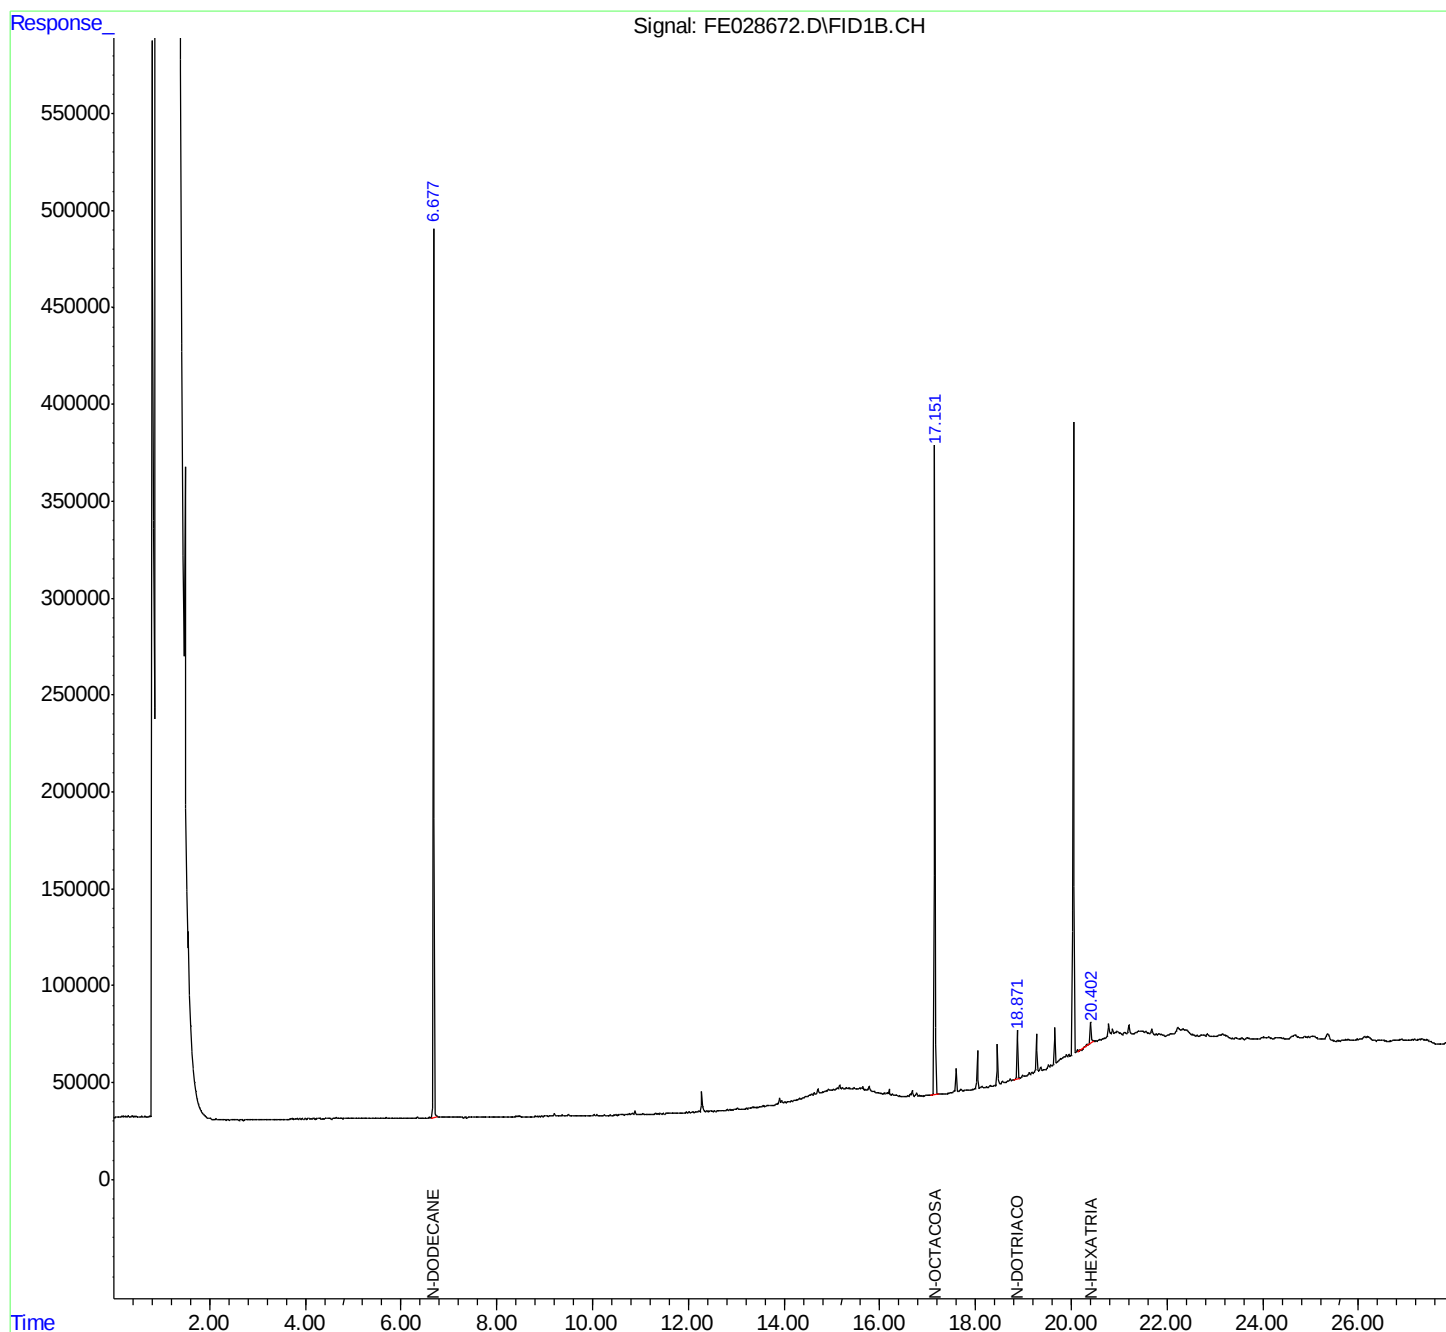

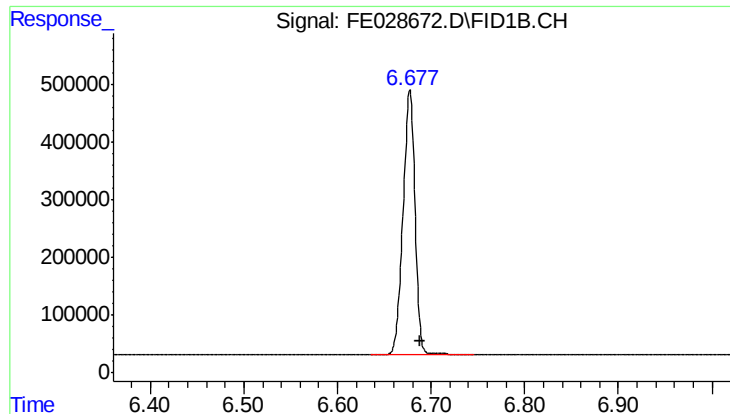


#5 N-DODECANE

R.T.: 6.677 min
Delta R.T.: -0.011 min
Response: 4068035
Conc: 27.00 ug/ml

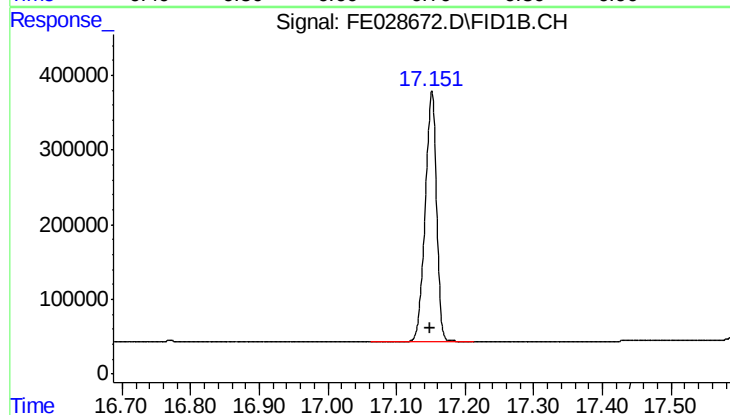


#11 N-OCTACOSANE

R.T.: 17.151 min
Delta R.T.: 0.003 min
Response: 3850813
Conc: 17.32 ug/ml

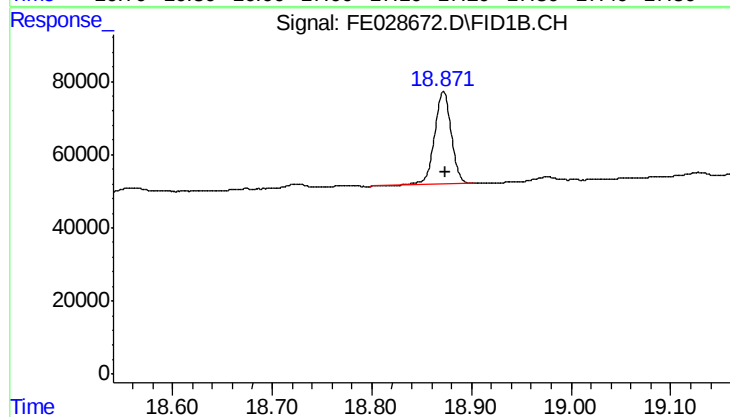


#12 N-DOTRIACONTANE

R.T.: 18.872 min
Delta R.T.: -0.002 min
Response: 293564
Conc: 1.60 ug/ml

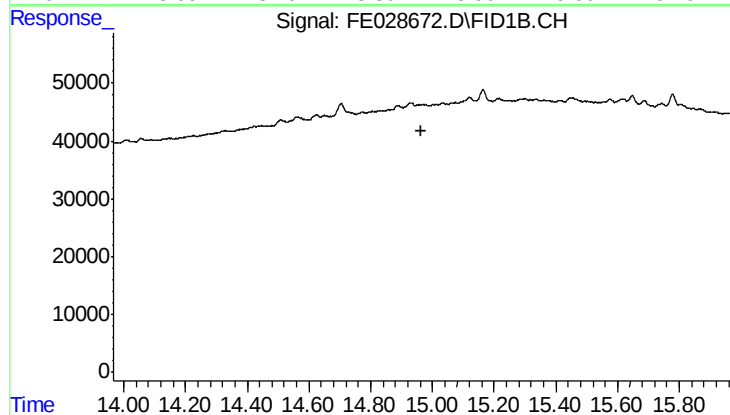

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.966 min
Response: 0
Conc: N.D.

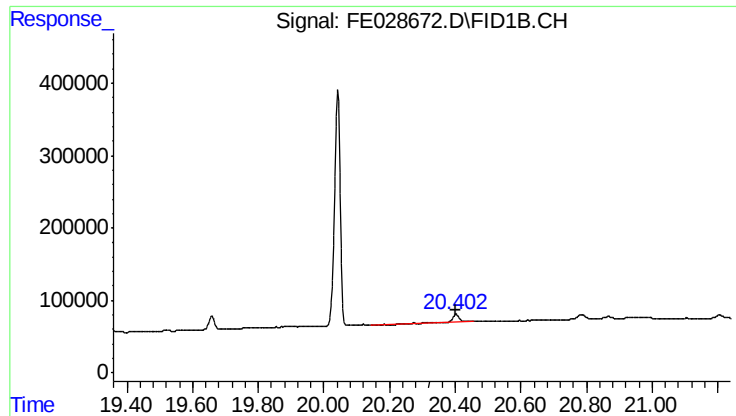

#14 N-HEXATRIACONTANE

R.T.: 20.402 min
Delta R.T.: 0.000 min
Response: 146245
Conc: 1.11 ug/ml