

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091923AL\
 Data File : FE044336.D
 Signal(s) : FID1B.ch
 Acq On : 19 Sep 2023 08:46
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 20 01:39:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 083023.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 31 03:37:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	13.521	364176	2.251 ug/ml
13) T n-Docosane (C22)	14.114	313508	1.962 ug/ml
14) T n-Tetracosane (C24)	15.226	217156	1.389 ug/ml
15) T n-Hexacosane (C26)	16.249	185319	1.229 ug/ml
16) T n-Octacosane (C28)	17.201	163773	1.135 ug/ml
17) T n-Tricontane (C30)	18.091	194198	1.337 ug/ml
18) T n-Dotriacontane (C32)	18.928	201777	1.417 ug/ml
19) T n-Tetratriacontane (C34)	19.711	213234	1.524 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091923AL\
Data File : FE044336.D
Signal(s) : FID1B.ch
Acq On : 19 Sep 2023 08:46
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 20 01:39:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 083023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 31 03:37:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

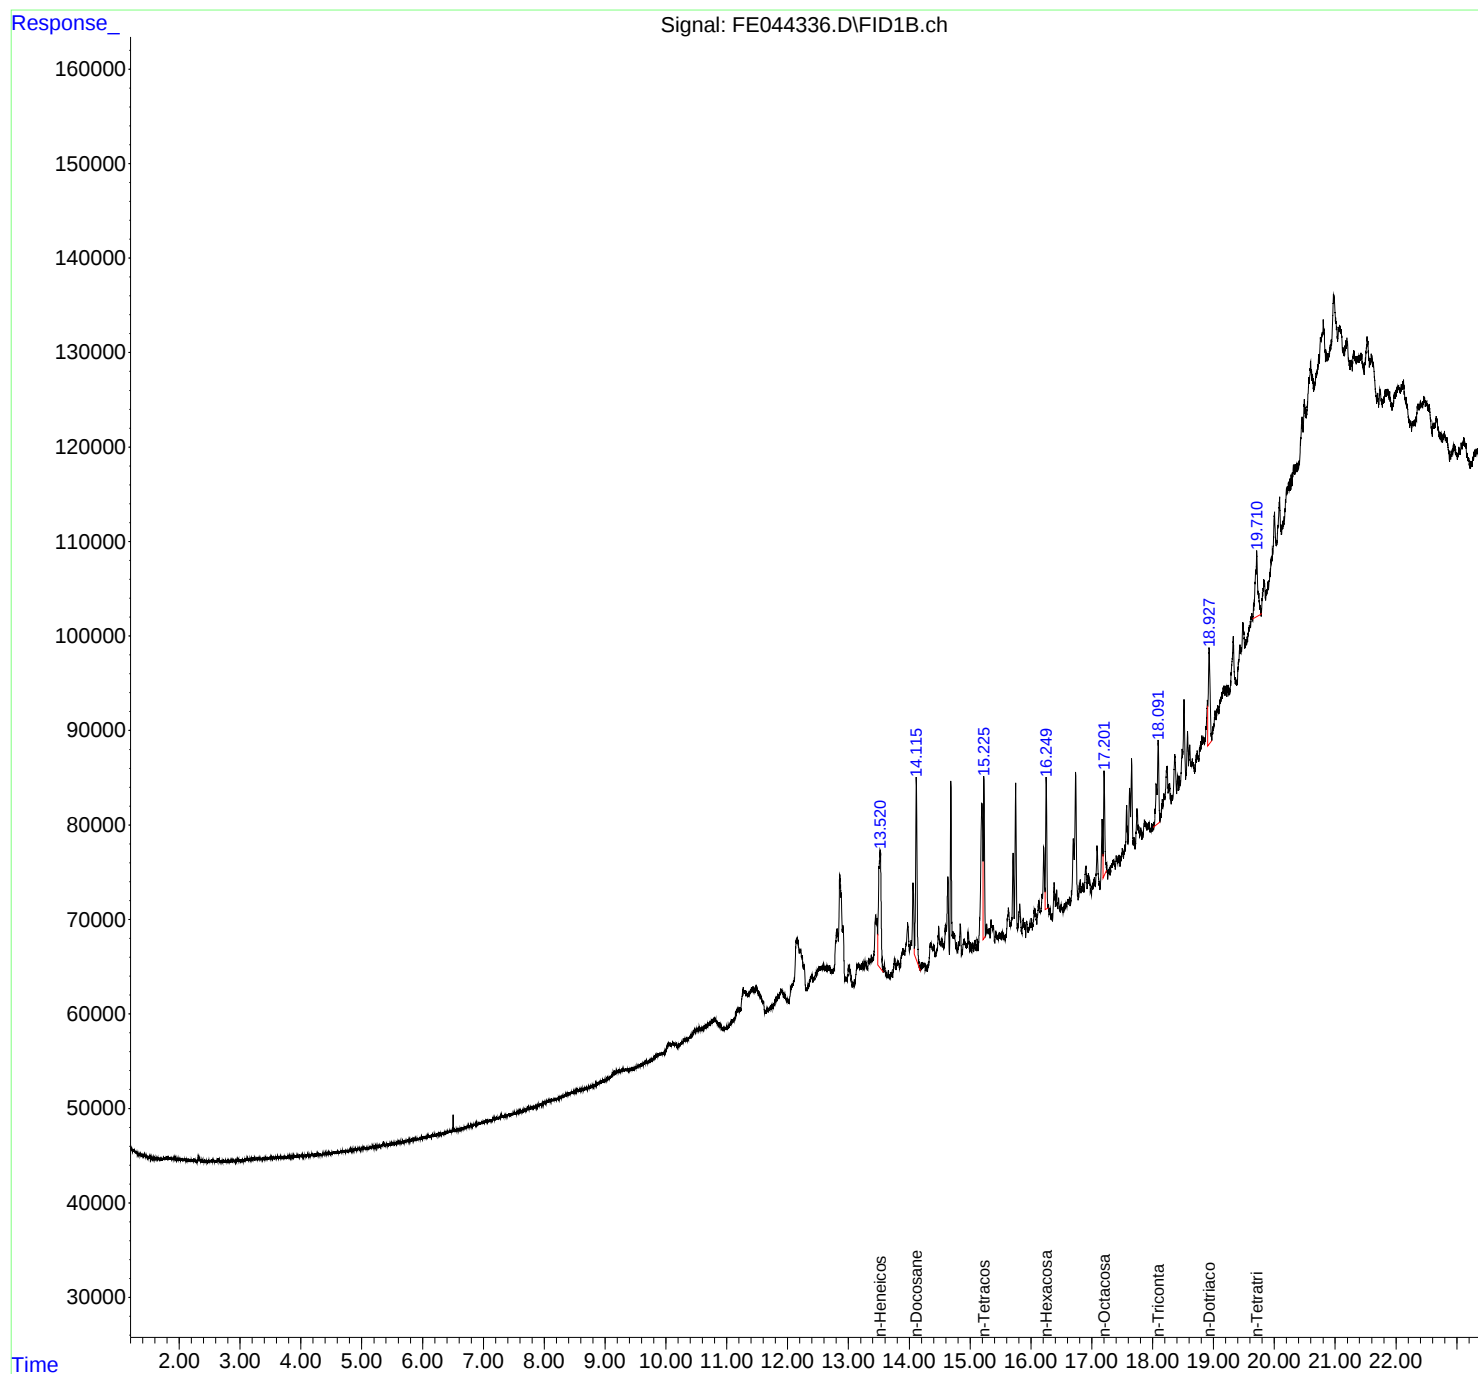


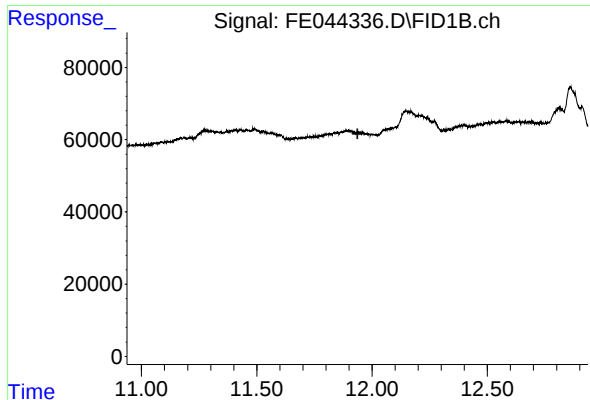

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.937 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

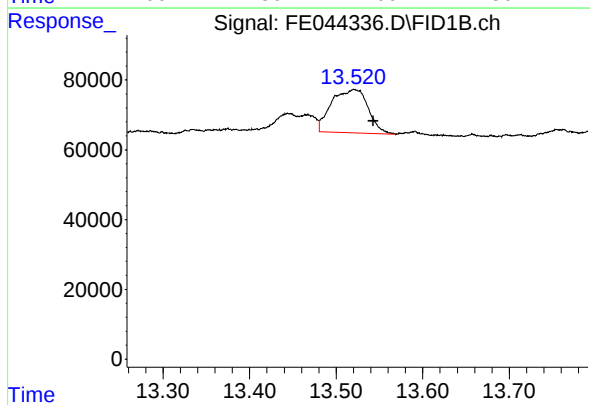


#11 n-Heneicosane (C21)

R.T.: 13.521 min
Delta R.T.: -0.022 min
Response: 364176
Conc: 2.25 ug/ml

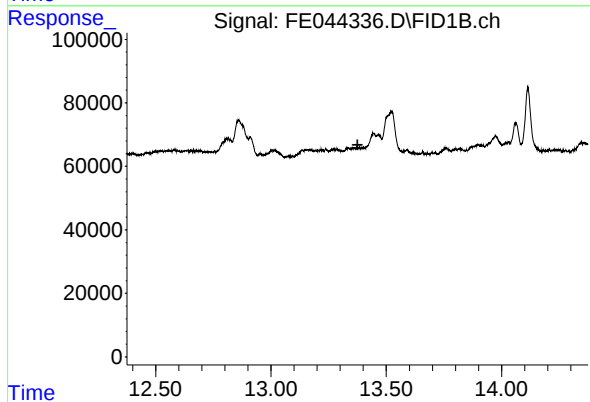


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.375 min
Response: 0
Conc: N.D.

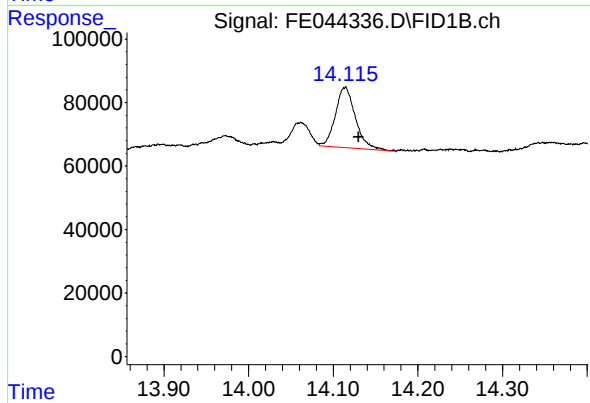

#13 n-Docosane (C22)


R.T.: 14.114 min
Delta R.T.: -0.016 min
Response: 313508
Conc: 1.96 ug/ml

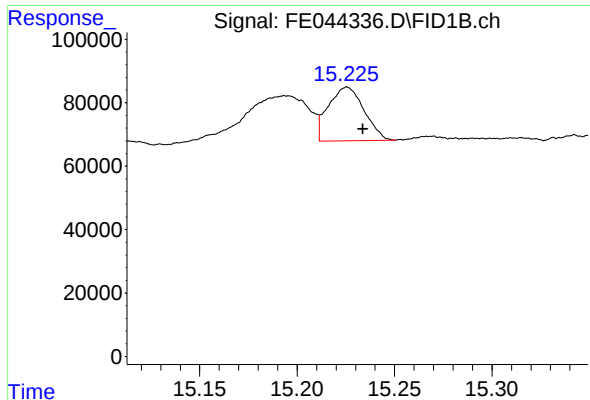

#14 n-Tetracosane (C24)


R.T.: 15.226 min
Delta R.T.: -0.008 min
Response: 217156
Conc: 1.39 ug/ml

Instrument :
FID_E
ClientSampleId :

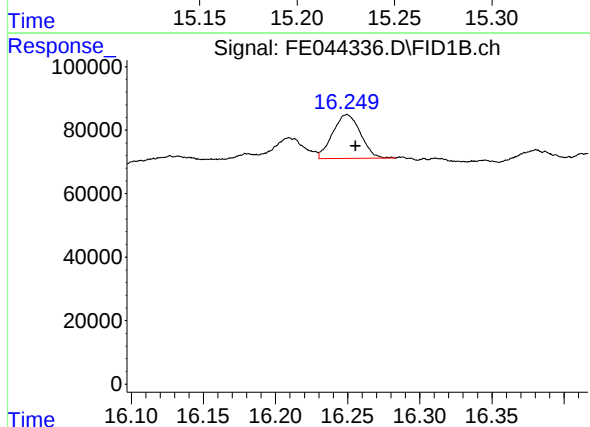


#15 n-Hexacosane (C26)

R.T.: 16.249 min
Delta R.T.: -0.006 min
Response: 185319
Conc: 1.23 ug/ml

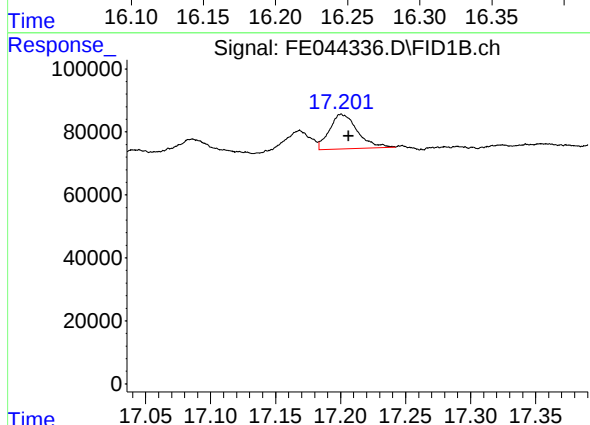


#16 n-Octacosane (C28)

R.T.: 17.201 min
Delta R.T.: -0.005 min
Response: 163773
Conc: 1.13 ug/ml

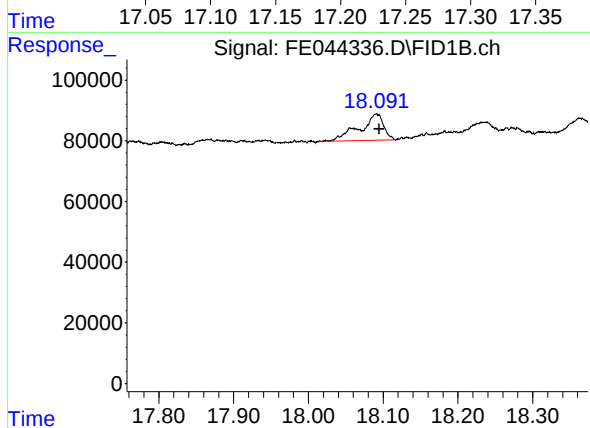

#17 n-Tricontane (C30)


R.T.: 18.091 min
Delta R.T.: -0.004 min
Response: 194198
Conc: 1.34 ug/ml

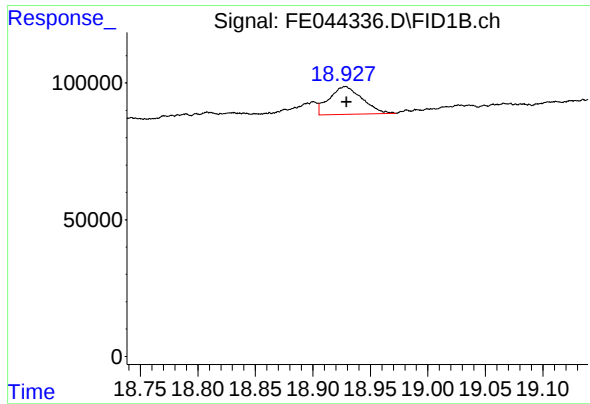

#18 n-Dotriacontane (C32)

R.T.: 18.928 min
Delta R.T.: -0.001 min
Response: 201777
Conc: 1.42 ug/ml

Instrument :
FID_E
ClientSampleId :

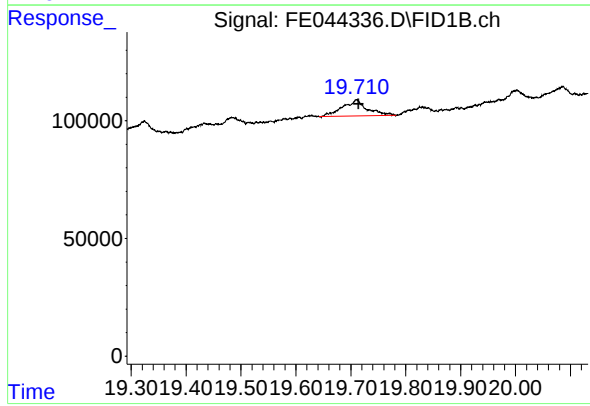

#19 n-Tetratriacontane (C34)

R.T.: 19.711 min
Delta R.T.: -0.004 min
Response: 213234
Conc: 1.52 ug/ml