

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092024AL\
Data File : FE050278.D
Signal(s) : FID1B.ch
Acq On : 21 Sep 2024 11:02
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 23 00:44:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 091024.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 17:11:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.840	41363	0.310 ug/ml
20) T	n-Hexatriacontane (C36)	20.364	143718	1.295 ug/ml
21) T	n-Octatriacontane (C38)	21.141	22433	0.203 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092024AL\
Data File : FE050278.D
Signal(s) : FID1B.ch
Acq On : 21 Sep 2024 11:02
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 23 00:44:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 091024.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 17:11:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

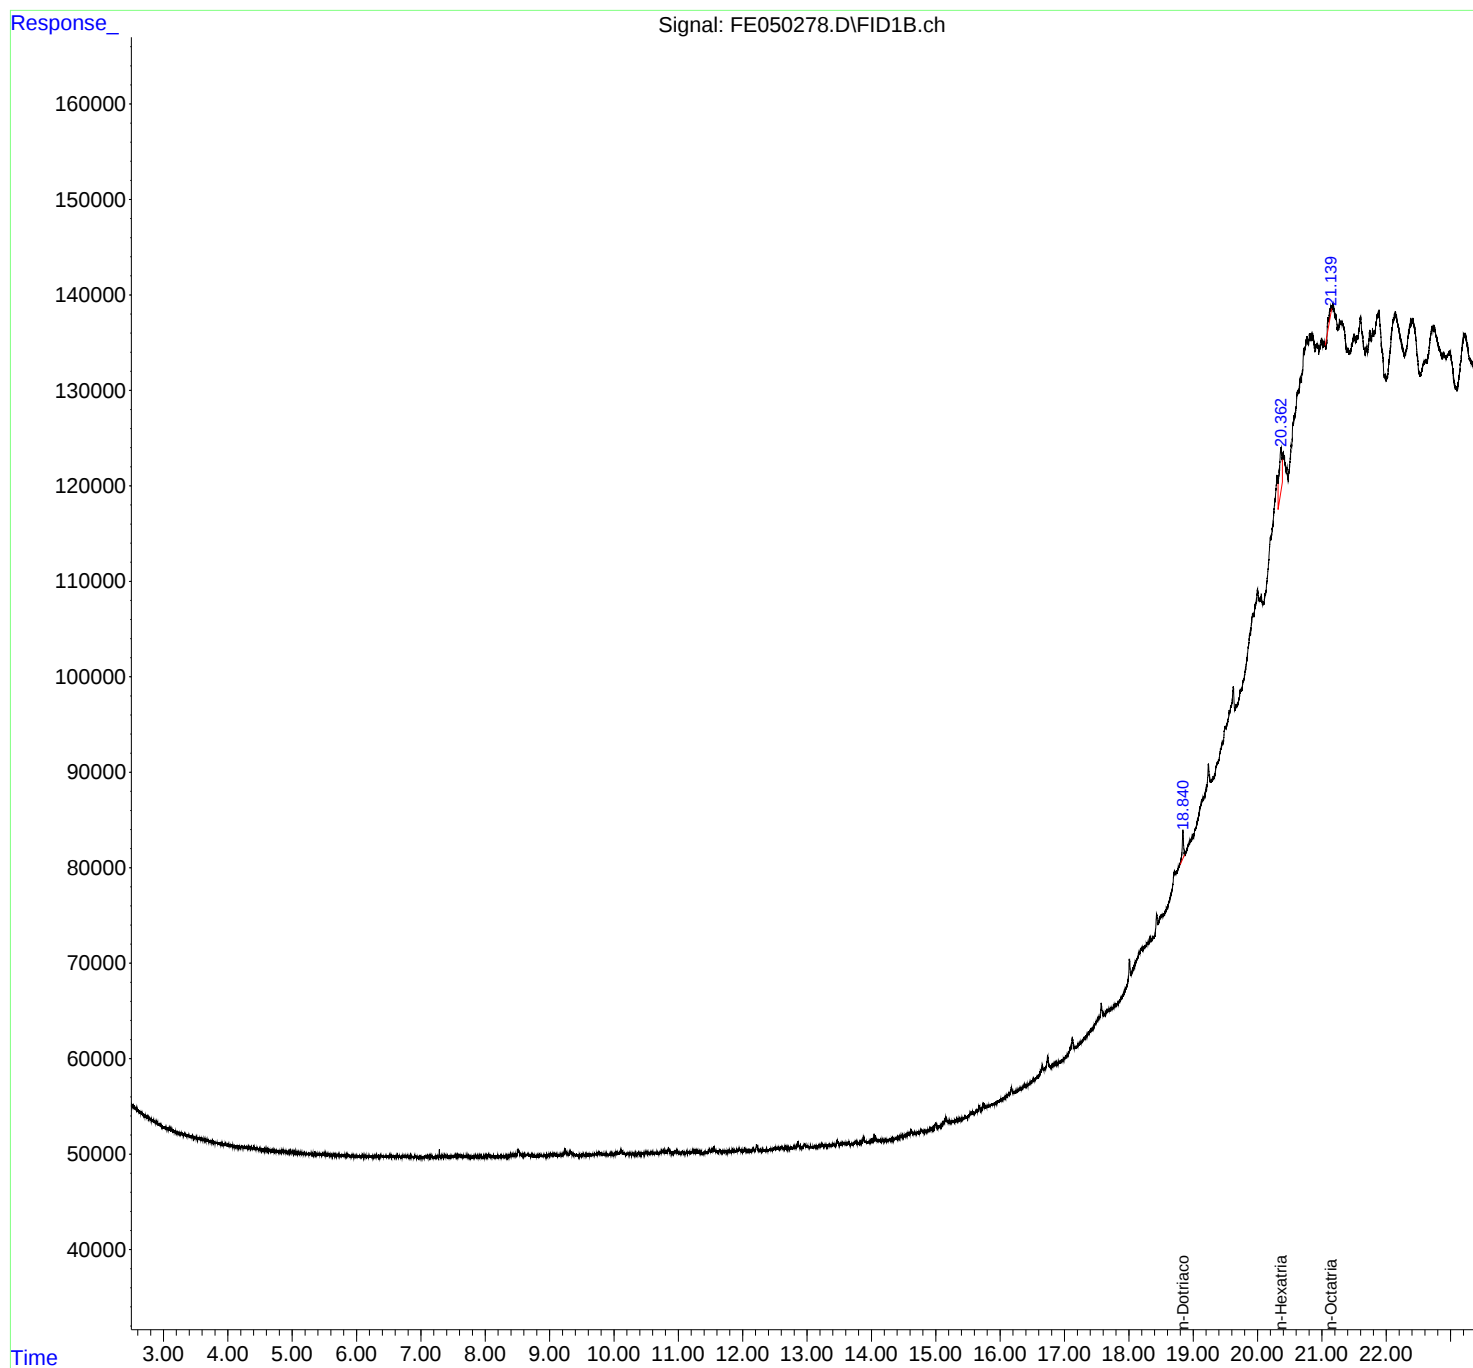


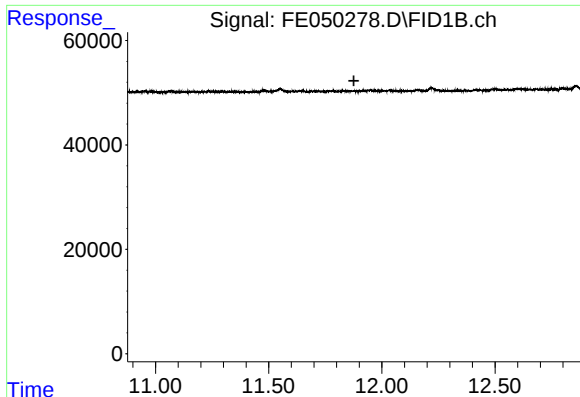

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.876 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

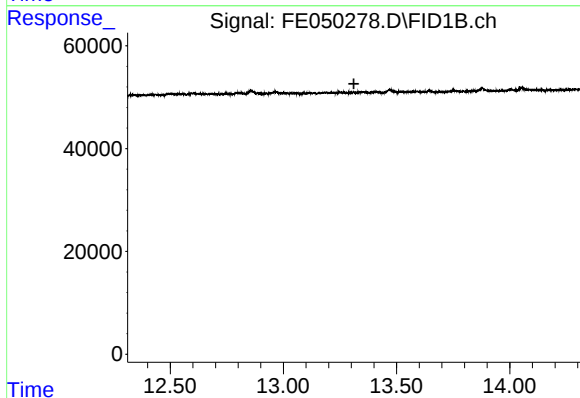


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.312 min
Response: 0
Conc: N.D.

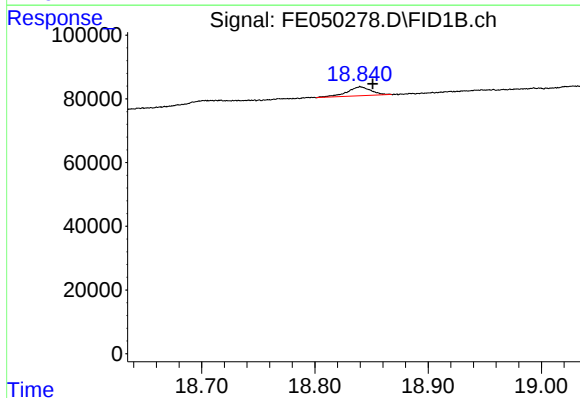


#18 n-Dotriacontane (C32)

R.T.: 18.840 min
Delta R.T.: -0.011 min
Response: 41363
Conc: 0.31 ug/ml

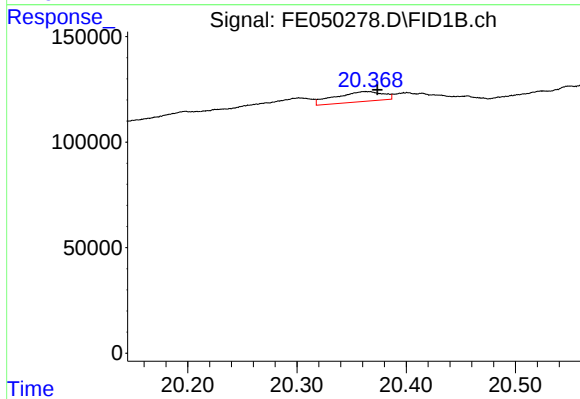

#20 n-Hexatriacontane (C36)

R.T.: 20.364 min
Delta R.T.: -0.010 min
Response: 143718
Conc: 1.30 ug/ml

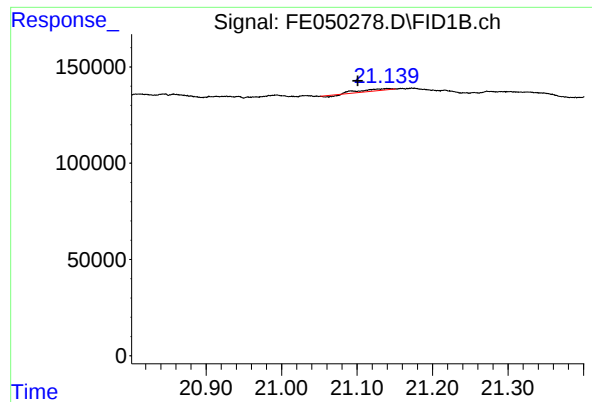

#21 n-Octatriacontane (C38)

R.T.: 21.141 min
Delta R.T.: 0.041 min
Response: 22433
Conc: 0.20 ug/ml

Instrument :

FID_E

ClientSampleId :