

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092118\
 Data File : FE028710.D
 Signal(s) : FID1B.CH
 Acq On : 20 Sep 2018 20:38
 Operator : AJ\SJ
 Sample : 4400 TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 21 07:19:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE092118.M
 Quant Title :
 QLast Update : Fri Sep 21 07:17:13 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.958	9891522	50.000 ug/ml
Target Compounds				
1)	N-OCTANE	2.554	40541159	400.000 ug/ml
2)	N-NONANE	3.587	42308712	400.000 ug/ml
3)	N-DECANE	4.674	65801380	400.000 ug/ml
4)	N-UNDECANE	5.718	72667151	600.000 ug/ml
5)	N-DODECANE	6.707	75325930	600.000 ug/ml
6)	N-TETRADECANE	8.517	81805558	600.000 ug/ml
7)	N-HEXADECANE	10.126	75541612	500.000 ug/ml
8)	N-OCTADECANE	11.559	40566708	250.000 ug/ml
9)	N-EICOSANE	12.859	17045121	100.000 ug/ml
10)	N-TETRACOSANE	15.172	16714698	100.000 ug/ml
11)	N-OCTACOSANE	17.138	7223936	50.000 ug/ml
12)	N-DOTRIACONTANE	18.864	6030219	50.000 ug/ml
14)	N-HEXATRIACONTANE	20.390	4908540	50.000 ug/ml
15)	N-TETRACONTANE	22.200	3449286	50.000 ug/ml
16)	N-TETRTETRACOOCTANE	25.302	2190372	50.000 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092118\
Data File : FE028710.D
Signal(s) : FID1B.CH
Acq On : 20 Sep 2018 20:38
Operator : AJ\SJ
Sample : 4400 TRPH STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 21 07:19:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE092118.M
Quant Title :
QLast Update : Fri Sep 21 07:17:13 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

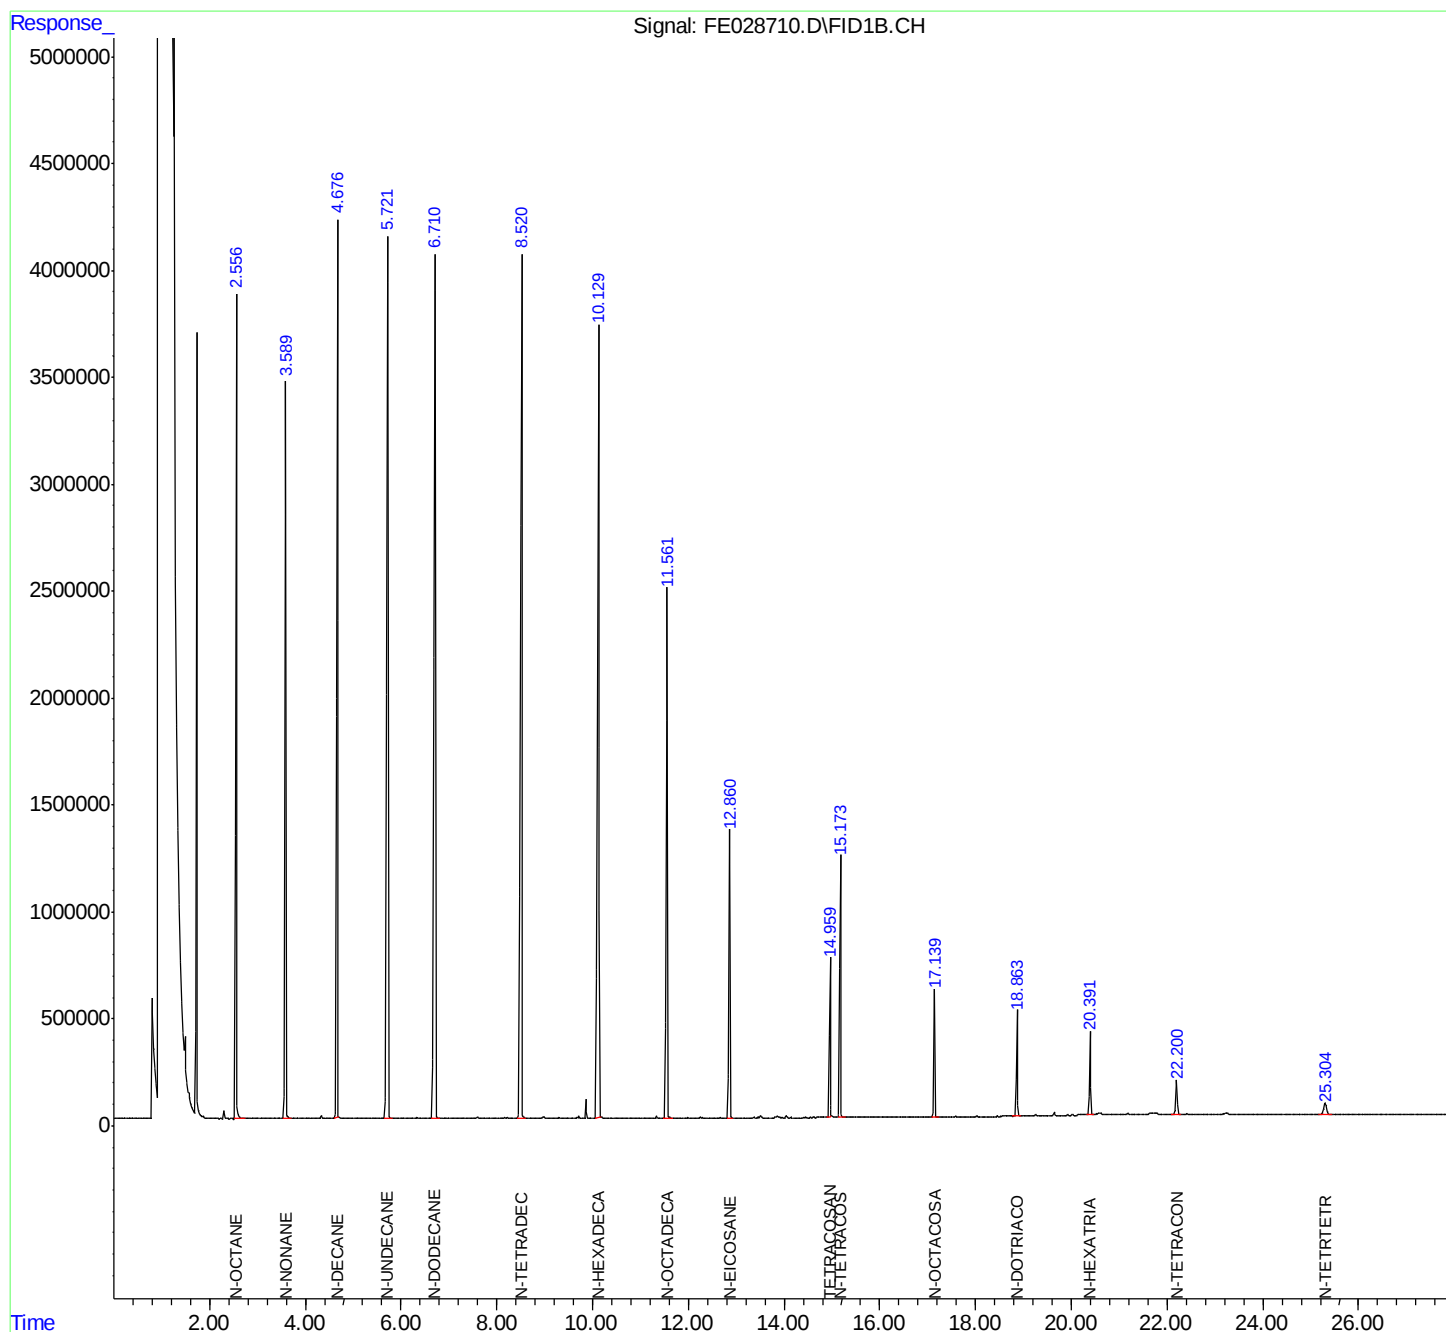

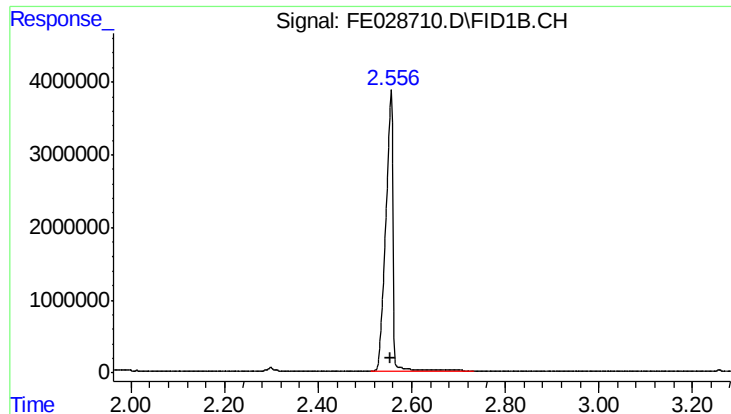


#1 N-OCTANE

R.T.: 2.554 min
Delta R.T.: 0.000 min
Response: 40541159
Conc: 400.00 ug/ml

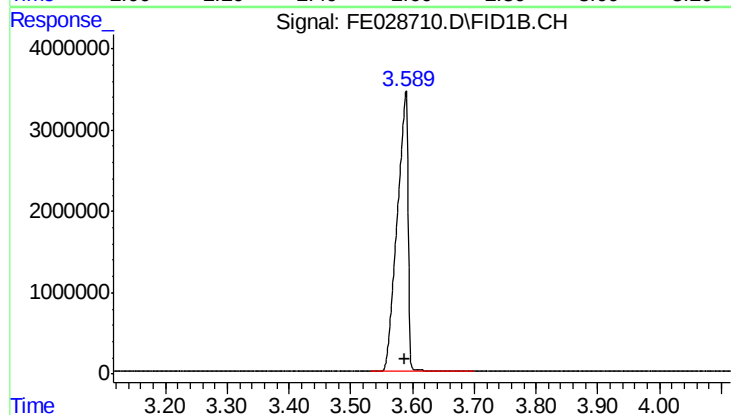


#2 N-NONANE

R.T.: 3.587 min
Delta R.T.: 0.000 min
Response: 42308712
Conc: 400.00 ug/ml

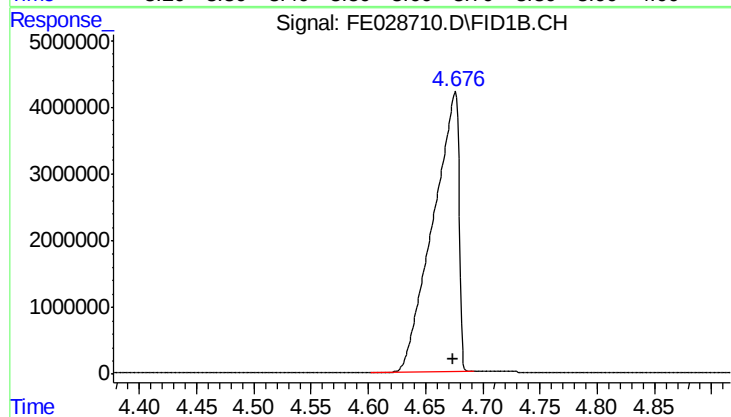


#3 N-DECANE

R.T.: 4.674 min
Delta R.T.: 0.000 min
Response: 65801380
Conc: 400.00 ug/ml

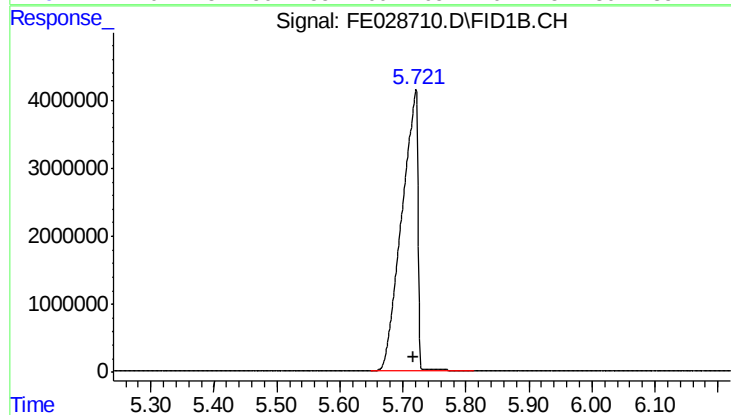


#4 N-UNDECANE

R.T.: 5.718 min
Delta R.T.: 0.000 min
Response: 72667151
Conc: 600.00 ug/ml

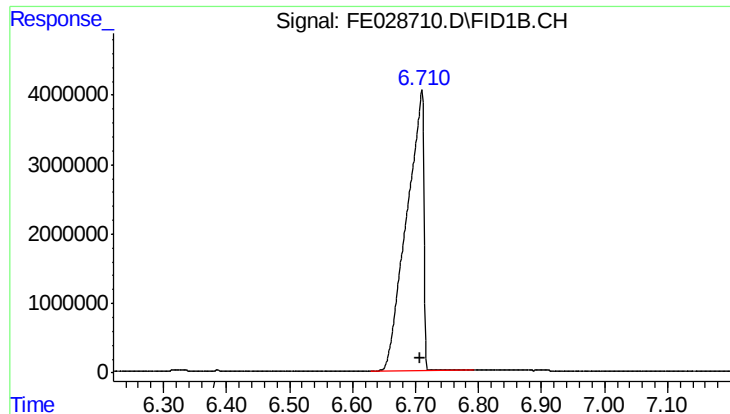


#5 N-DODECANE

R.T.: 6.707 min
Delta R.T.: 0.000 min
Response: 75325930
Conc: 600.00 ug/ml

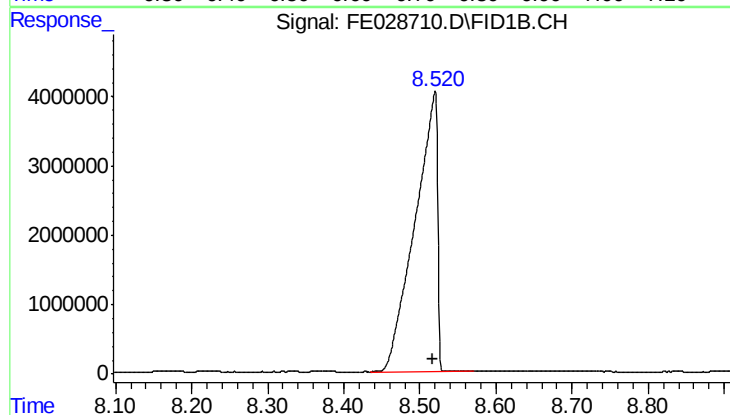


#6 N-TETRADECANE

R.T.: 8.517 min
Delta R.T.: 0.000 min
Response: 81805558
Conc: 600.00 ug/ml

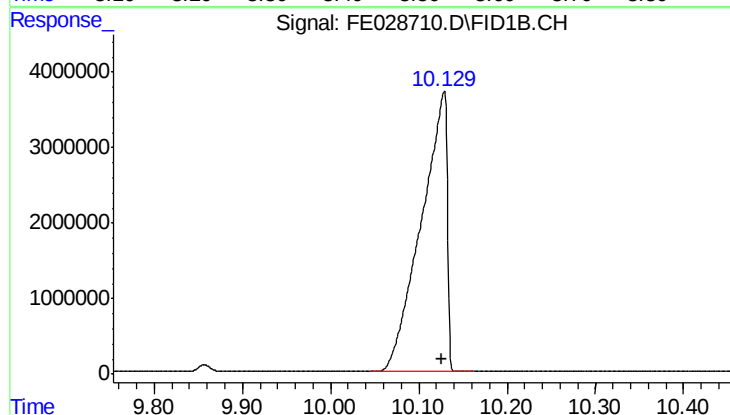


#7 N-HEXADECANE

R.T.: 10.126 min
Delta R.T.: 0.000 min
Response: 75541612
Conc: 500.00 ug/ml

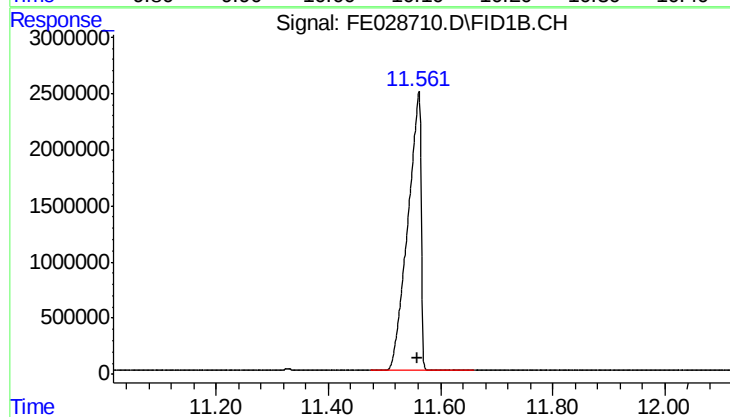


#8 N-OCTADECANE

R.T.: 11.559 min
Delta R.T.: 0.000 min
Response: 40566708
Conc: 250.00 ug/ml

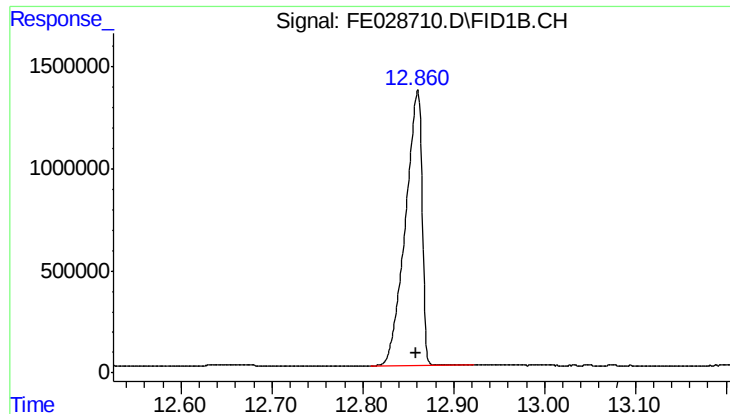


#9 N-EICOSANE

R.T.: 12.859 min
Delta R.T.: 0.000 min
Response: 17045121
Conc: 100.00 ug/ml

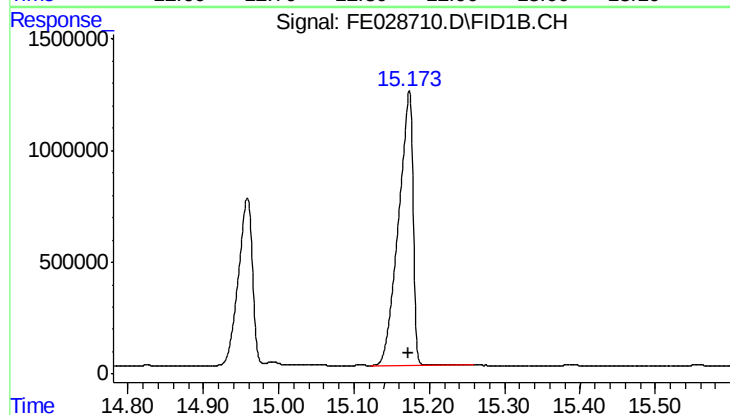


#10 N-TETRACOSANE

R.T.: 15.172 min
Delta R.T.: 0.000 min
Response: 16714698
Conc: 100.00 ug/ml

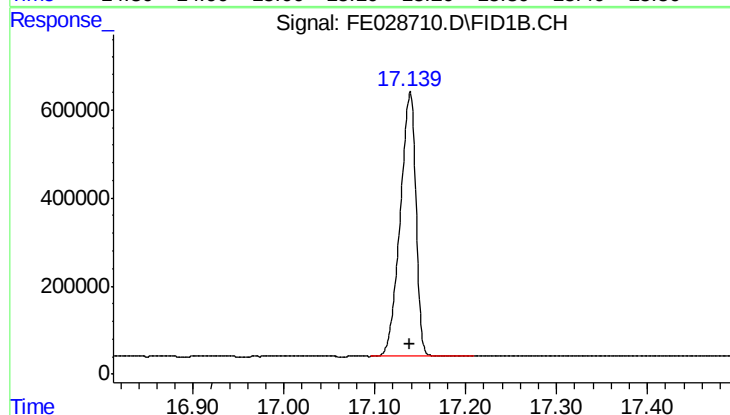


#11 N-OCTACOSANE

R.T.: 17.138 min
Delta R.T.: 0.000 min
Response: 7223936
Conc: 50.00 ug/ml

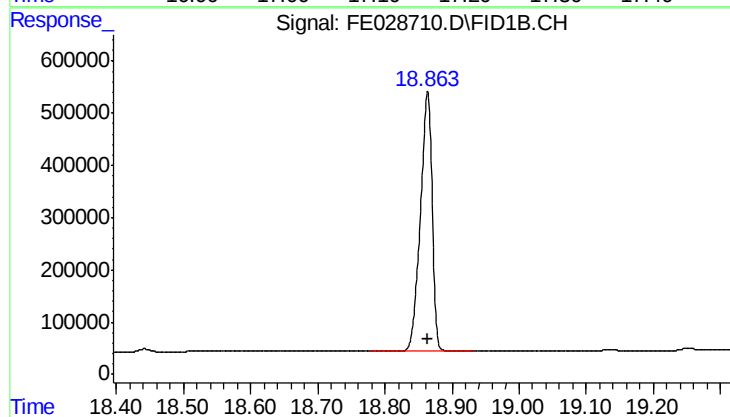


#12 N-DOTRIACONTANE

R.T.: 18.864 min
Delta R.T.: 0.000 min
Response: 6030219
Conc: 50.00 ug/ml

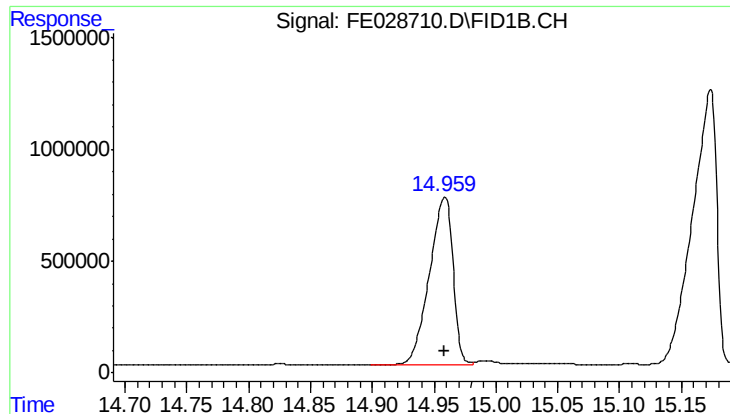


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.958 min
Delta R.T.: 0.000 min
Response: 9891522
Conc: 50.00 ug/ml

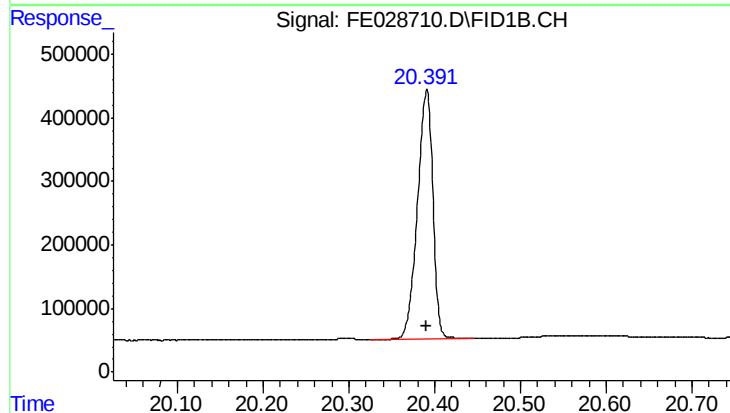


#14 N-HEXATRIACONTANE

R.T.: 20.390 min
Delta R.T.: 0.000 min
Response: 4908540
Conc: 50.00 ug/ml

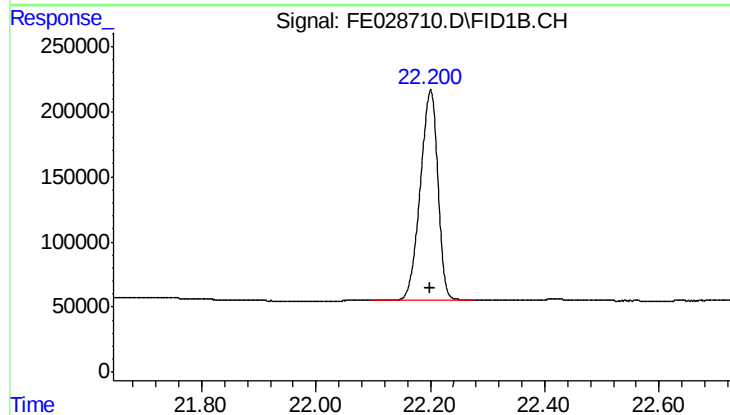

#15 N-TETRACONTANE

R.T.: 22.200 min
Delta R.T.: 0.000 min
Response: 3449286
Conc: 50.00 ug/ml

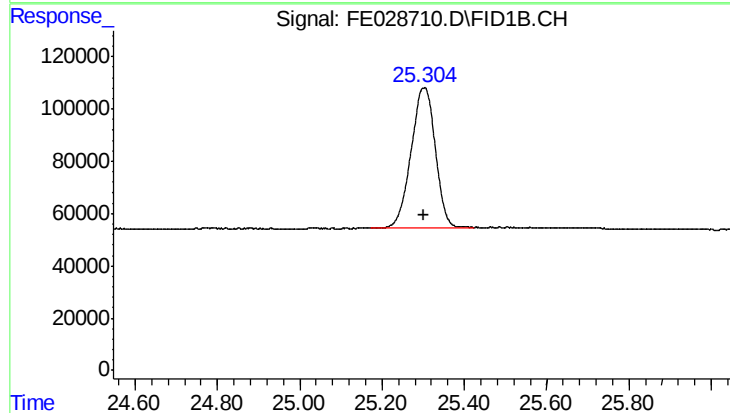

#16 N-TETRTETRACOOCTANE

R.T.: 25.302 min
Delta R.T.: 0.000 min
Response: 2190372
Conc: 50.00 ug/ml