

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE092324AL\  
Data File : FE050288.D  
Signal(s) : FID1B.ch  
Acq On : 23 Sep 2024 13:11  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Sep 24 01:26:02 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 091024.M  
Quant Title : GC Extractables  
QLast Update : Mon Sep 09 17:11:47 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                    |                          | R.T.   | Response | Conc Units  |
|-----------------------------|--------------------------|--------|----------|-------------|
| -----                       |                          |        |          |             |
| System Monitoring Compounds |                          |        |          |             |
| Target Compounds            |                          |        |          |             |
| 17) T                       | n-Tricontane (C30)       | 18.011 | 58332    | 0.436 ug/ml |
| 18) T                       | n-Dotriacontane (C32)    | 18.842 | 98956    | 0.743 ug/ml |
| 19) T                       | n-Tetratriacontane (C34) | 19.623 | 97090    | 0.786 ug/ml |
| 20) T                       | n-Hexatriacontane (C36)  | 20.363 | 180585   | 1.628 ug/ml |
| -----                       |                          |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE092324AL\  
Data File : FE050288.D  
Signal(s) : FID1B.ch  
Acq On : 23 Sep 2024 13:11  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Sep 24 01:26:02 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 091024.M  
Quant Title : GC Extractables  
QLast Update : Mon Sep 09 17:11:47 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

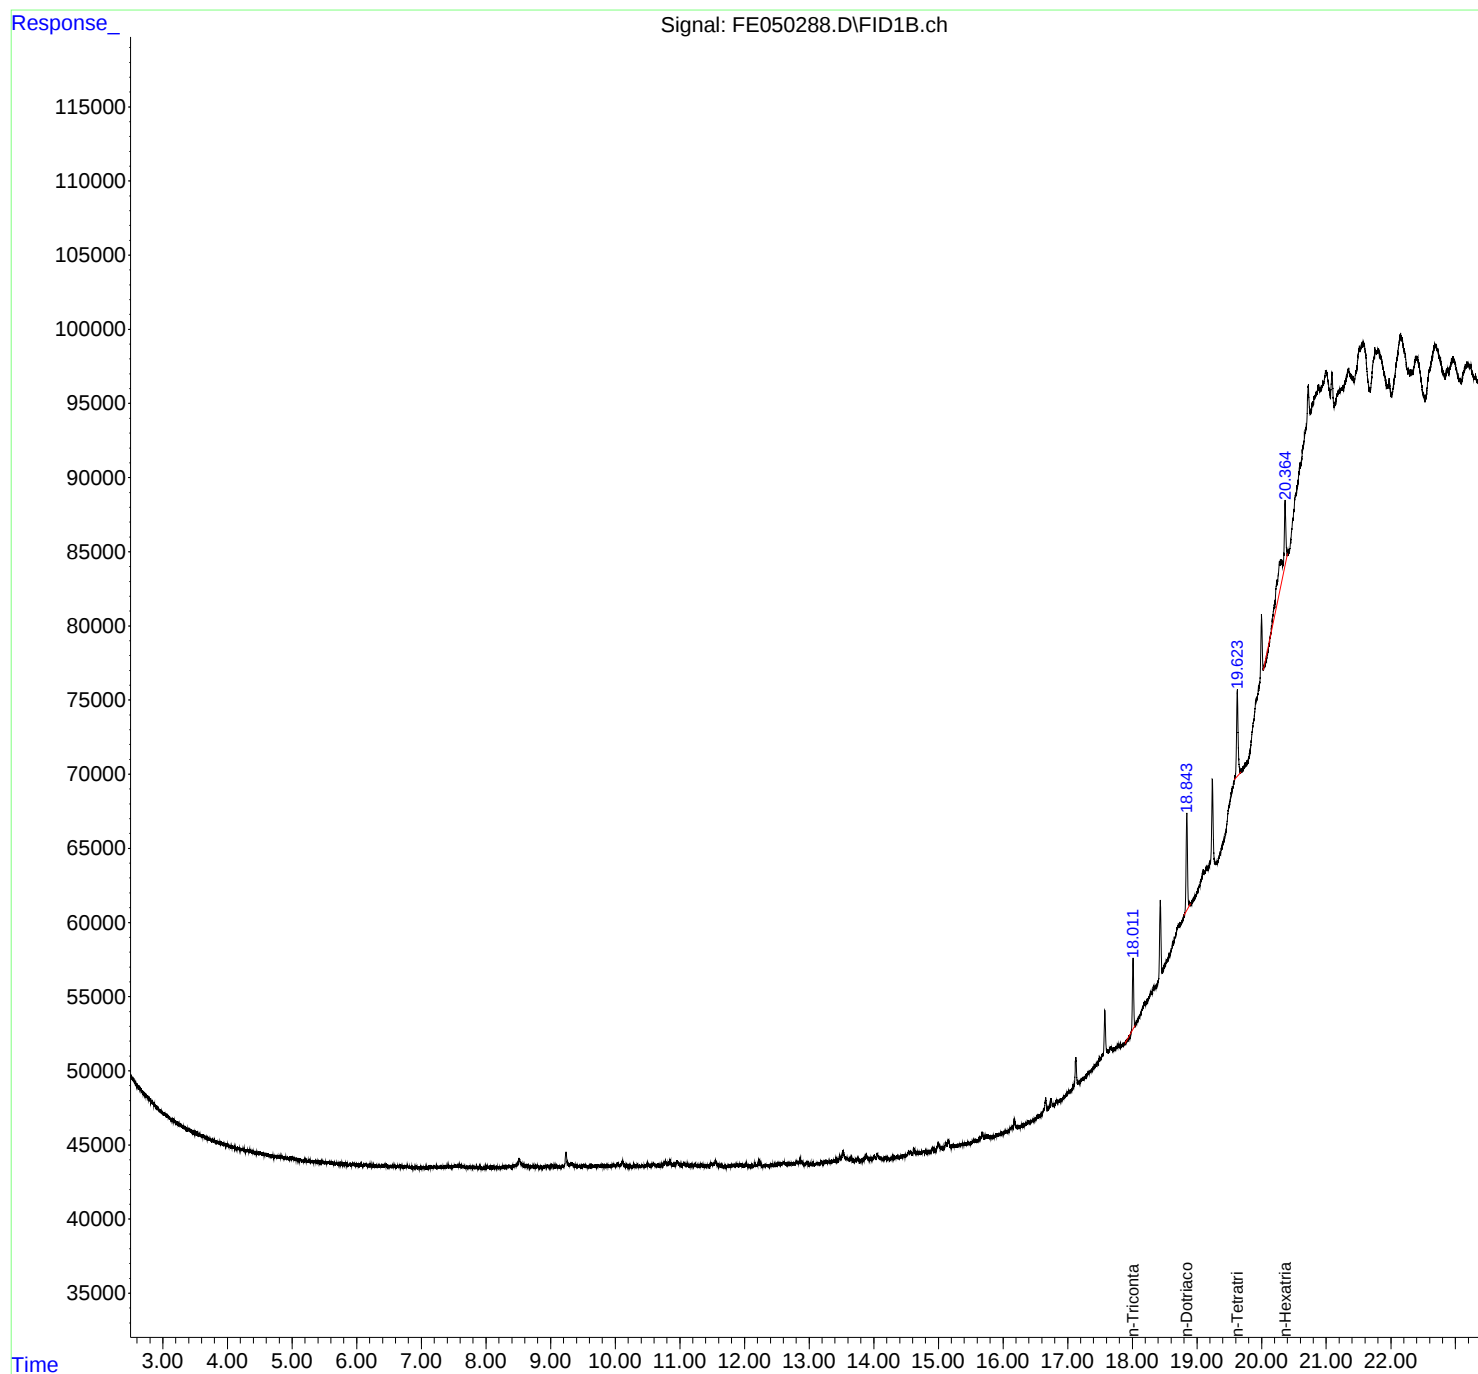


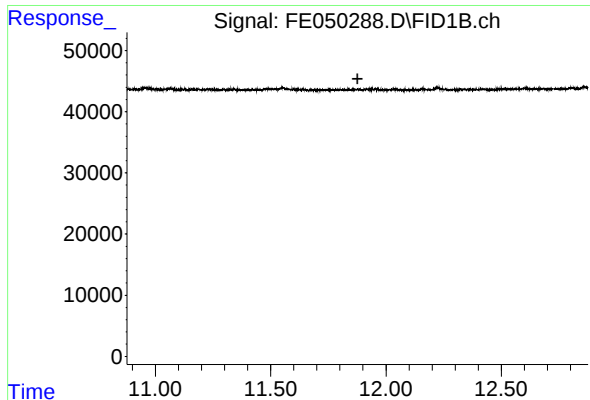

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min  
Exp R.T.: 11.876 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :

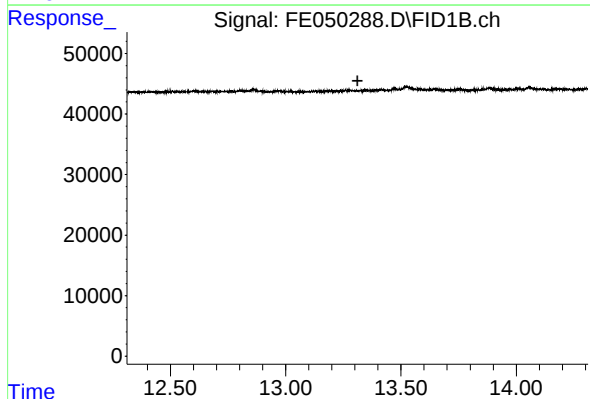


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min  
Exp R.T.: 13.312 min  
Response: 0  
Conc: N.D.

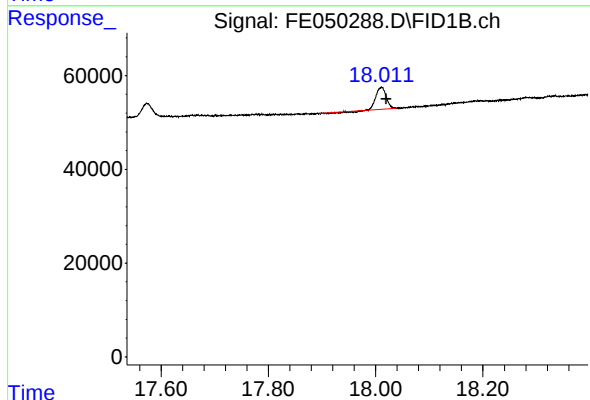


#17 n-Tricontane (C30)

R.T.: 18.011 min  
Delta R.T.: -0.009 min  
Response: 58332  
Conc: 0.44 ug/ml

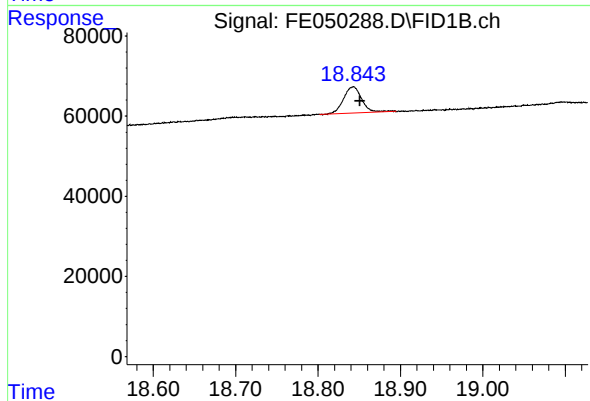

#18 n-Dotriacontane (C32)


R.T.: 18.842 min  
Delta R.T.: -0.009 min  
Response: 98956  
Conc: 0.74 ug/ml

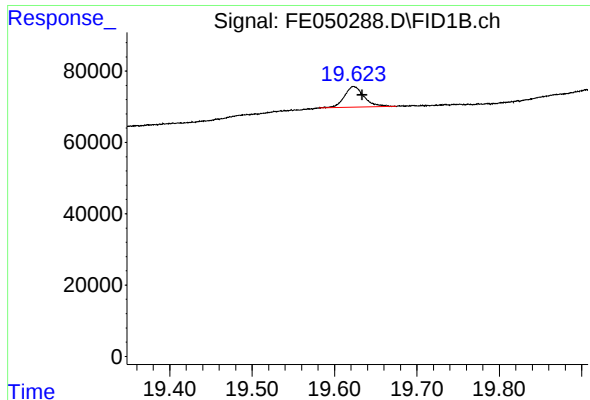

#19 n-Tetratriacontane (C34)

R.T.: 19.623 min  
Delta R.T.: -0.010 min  
Response: 97090  
Conc: 0.79 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

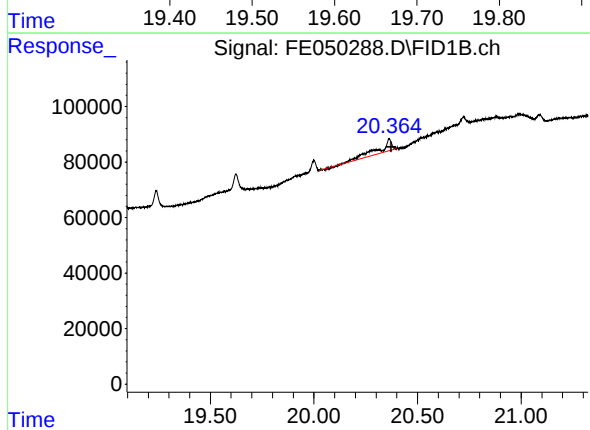

#20 n-Hexatriacontane (C36)

R.T.: 20.363 min  
Delta R.T.: -0.011 min  
Response: 180585  
Conc: 1.63 ug/ml