

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE092324AL\  
Data File : FE050292.D  
Signal(s) : FID1B.ch  
Acq On : 23 Sep 2024 15:42  
Operator : YP\AJ  
Sample : P4104-24DL 10X  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
WC-22A-EPH-4DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 09/24/2024  
Supervised By :Ankita Jodhani 09/24/2024

Integration File: autoint1.e  
Quant Time: Sep 24 01:26:47 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 091024.M  
Quant Title : GC Extractables  
QLast Update : Mon Sep 09 17:11:47 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 13.302 | 318469     | 2.835 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery = | 5.67%        |

Target Compounds

-----

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE092324AL\  
Data File : FE050292.D  
Signal(s) : FID1B.ch  
Acq On : 23 Sep 2024 15:42  
Operator : YP\AJ  
Sample : P4104-24DL 10X  
Misc :  
ALS Vial : 14 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
WC-22A-EPH-4DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 09/24/2024  
Supervised By :Ankita Jodhani 09/24/2024

Integration File: autoint1.e  
Quant Time: Sep 24 01:26:47 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 091024.  
Quant Title : GC Extractables  
QLast Update : Mon Sep 09 17:11:47 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

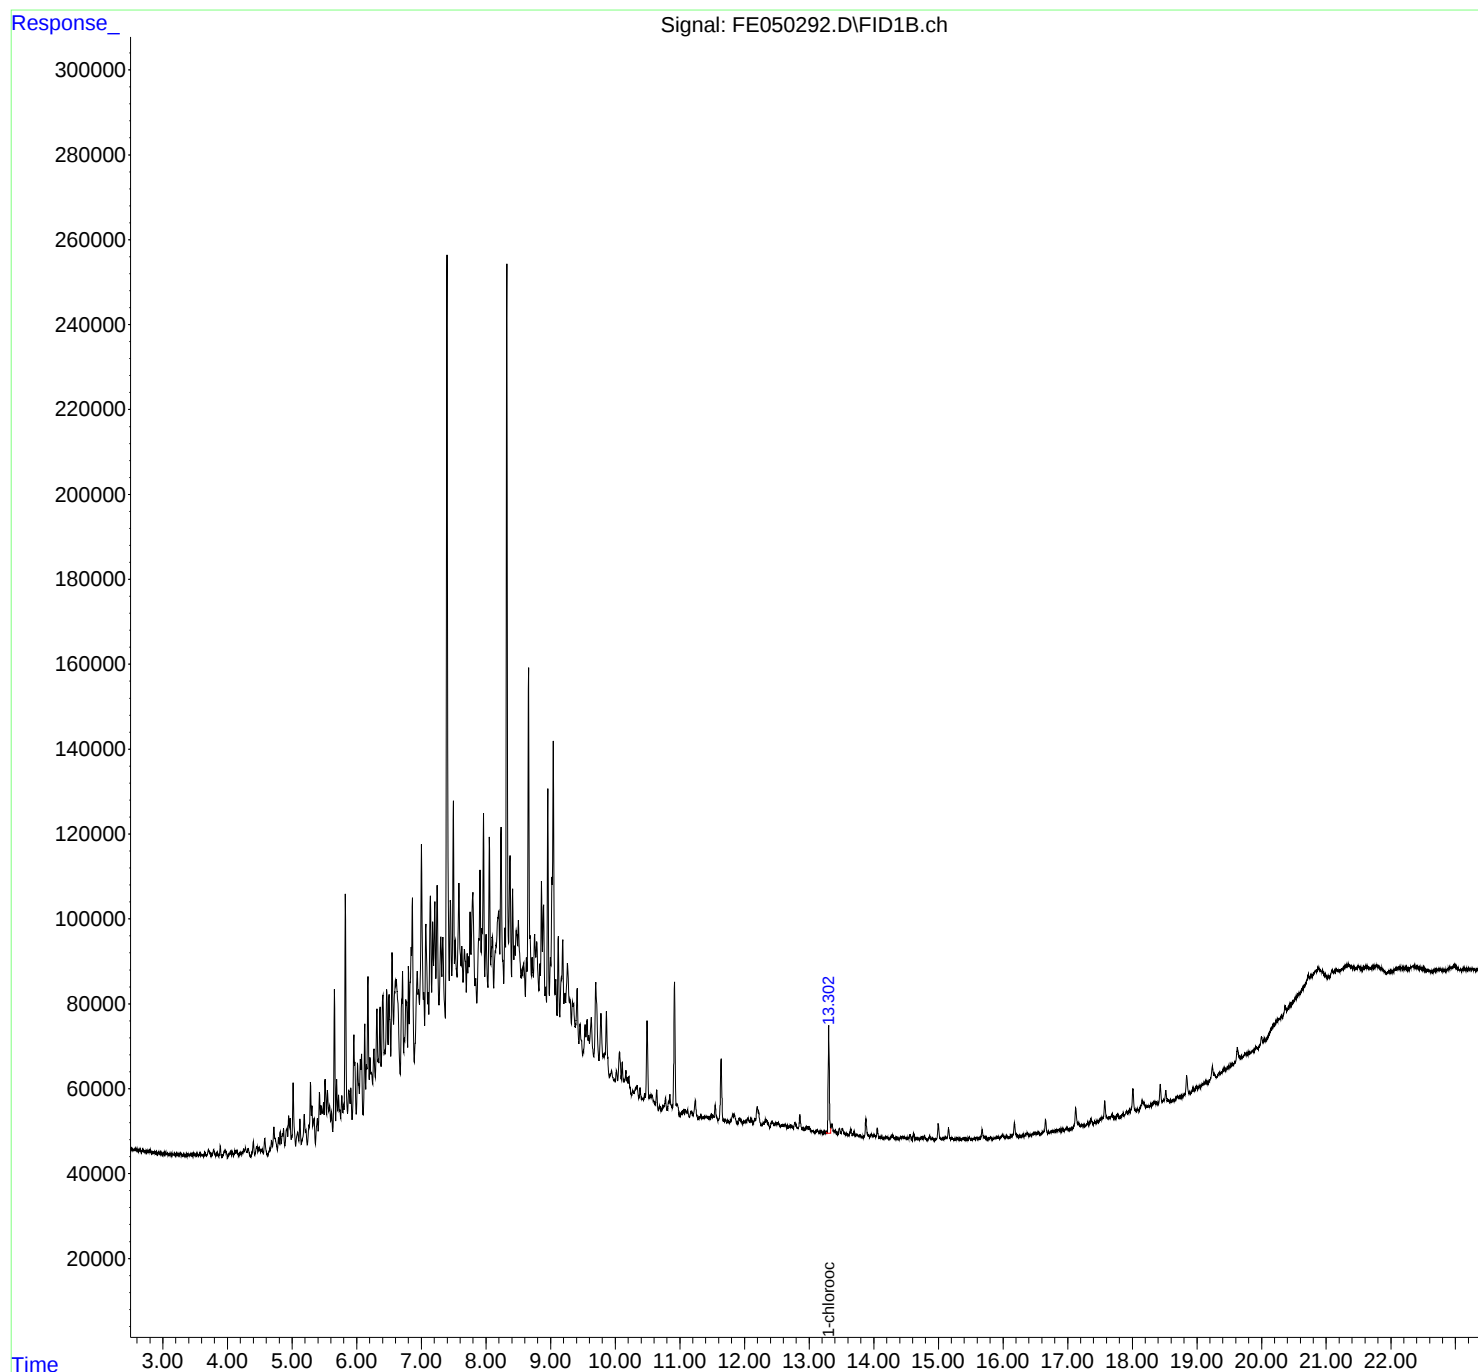

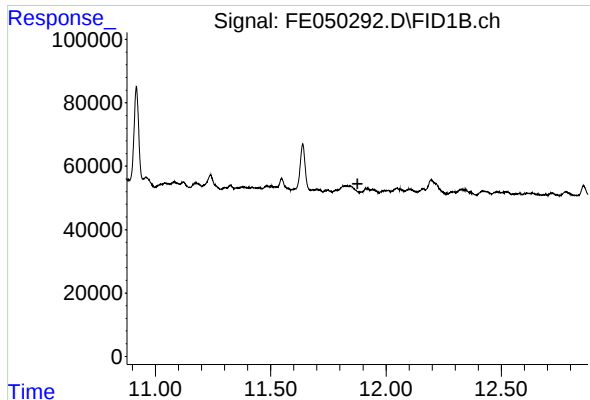


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 11.876 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :  
WC-22A-EPH-4DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 09/24/2024  
Supervised By :Ankita Jodhani 09/24/2024

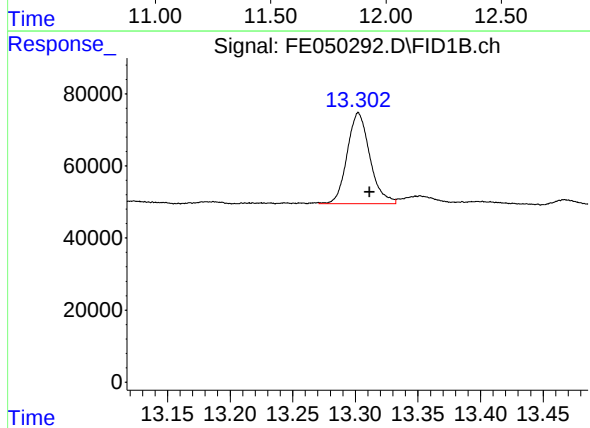

#12 1-chlorooctadecane (SURR)

R.T.: 13.302 min  
Delta R.T.: -0.009 min  
Response: 318469  
Conc: 2.84 ug/ml m