

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE092324AL\  
 Data File : FE050293.D  
 Signal(s) : FID1B.ch  
 Acq On : 23 Sep 2024 16:13  
 Operator : YP\AJ  
 Sample : P4104-24DL2 50X  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 WC-22A-EPH-4DL2

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 09/24/2024  
 Supervised By :Ankita Jodhani 09/24/2024

Integration File: autoint1.e  
 Quant Time: Sep 24 01:27:03 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 091024.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Sep 09 17:11:47 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 13.303 | 65025      | 0.579 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery = | 1.16%        |
| Target Compounds               |        |            |              |
| -----                          |        |            |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE092324AL\  
Data File : FE050293.D  
Signal(s) : FID1B.ch  
Acq On : 23 Sep 2024 16:13  
Operator : YP\AJ  
Sample : P4104-24DL2 50X  
Misc :  
ALS Vial : 15 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
WC-22A-EPH-4DL2


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 09/24/2024  
Supervised By :Ankita Jodhani 09/24/2024

Integration File: autoint1.e  
Quant Time: Sep 24 01:27:03 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 091024.  
Quant Title : GC Extractables  
QLast Update : Mon Sep 09 17:11:47 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

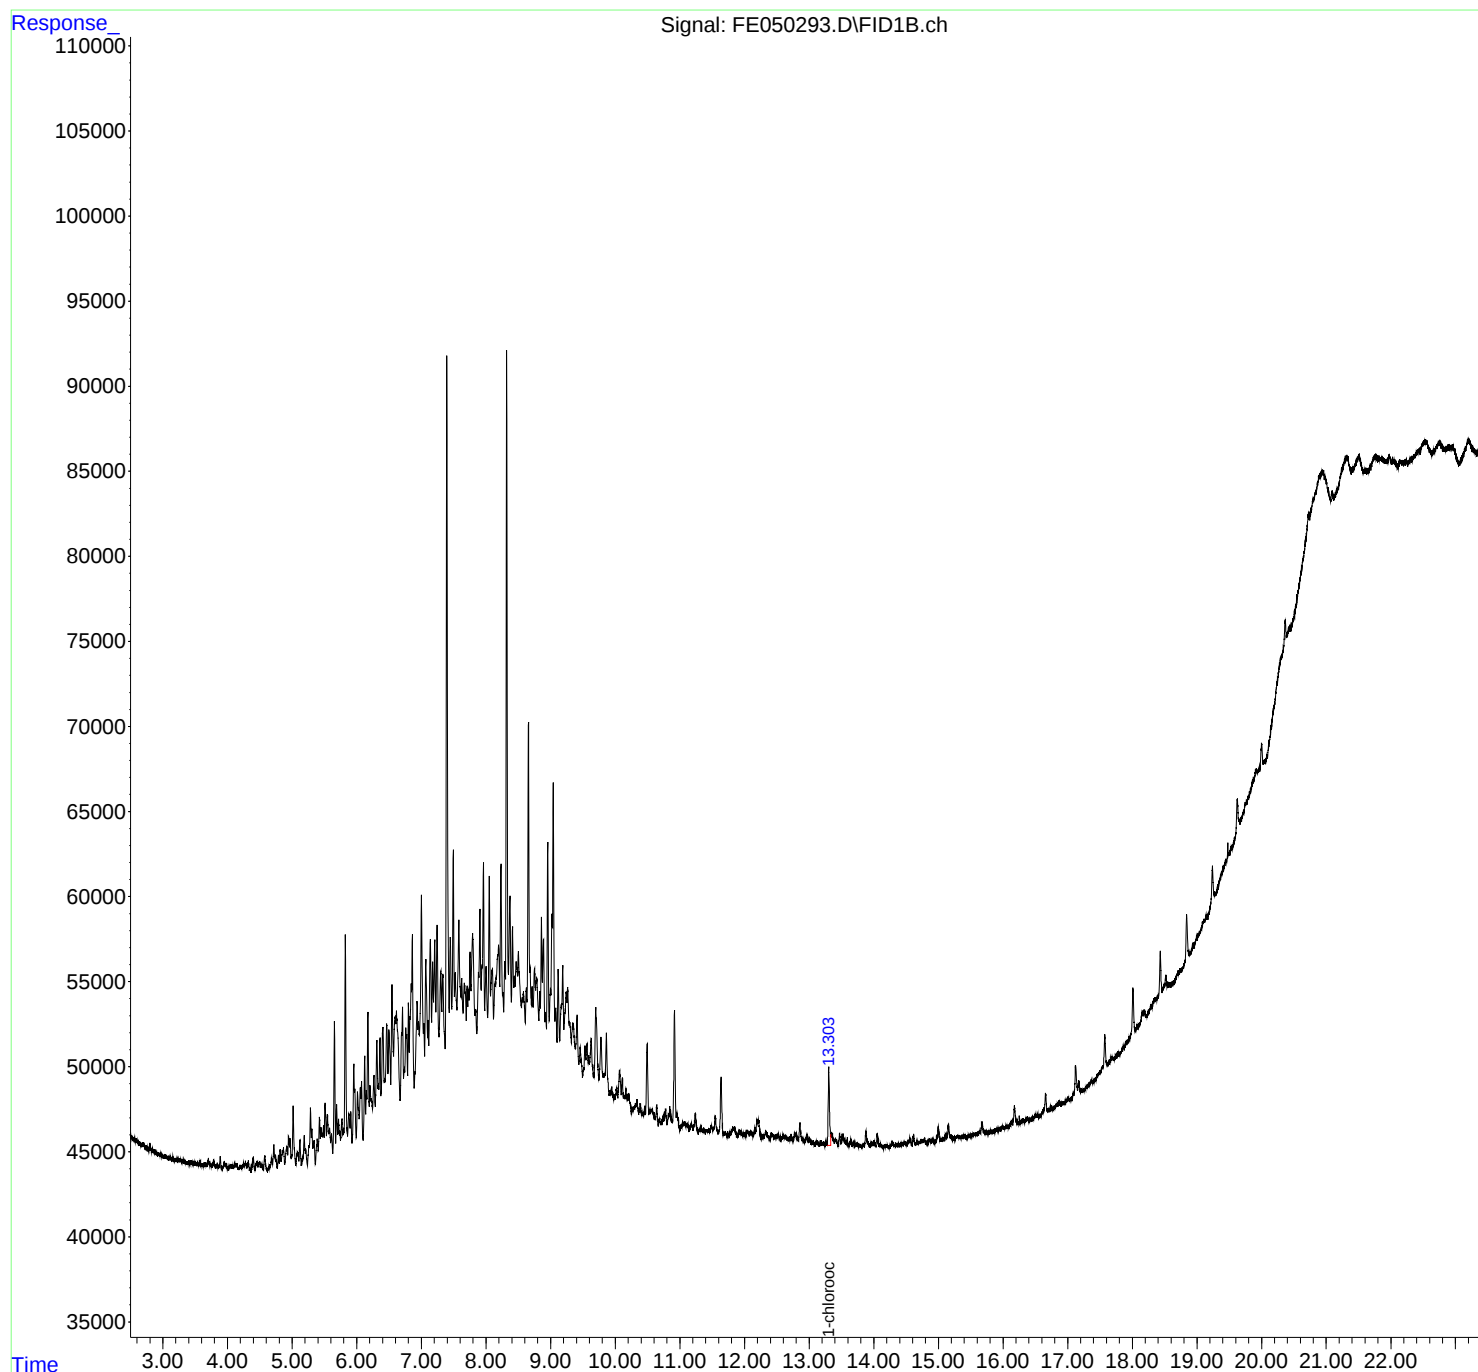

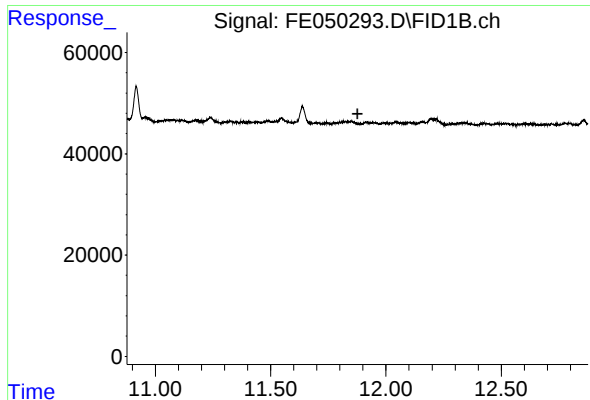

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 11.876 min  
Response: 0  
Conc: N.D.

Instrument :

FID\_E


ClientSampleId :

WC-22A-EPH-4DL2

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 09/24/2024  
Supervised By :Ankita Jodhani 09/24/2024

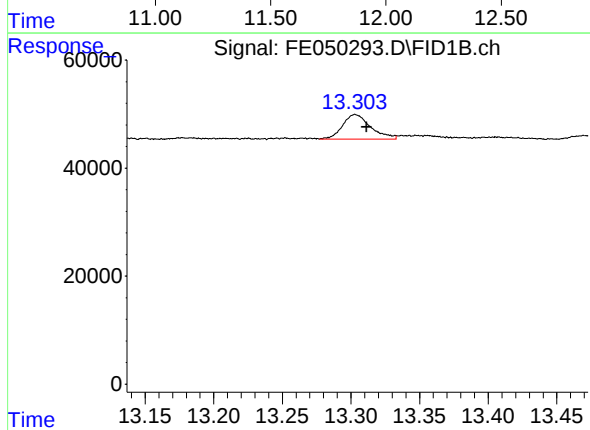

#12 1-chlorooctadecane (SURR)

R.T.: 13.303 min  
Delta R.T.: -0.009 min  
Response: 65025  
Conc: 0.58 ug/ml m