

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE092524AL\  
 Data File : FE050344.D  
 Signal(s) : FID1B.ch  
 Acq On : 25 Sep 2024 10:29  
 Operator : YP\AJ  
 Sample : P4150-02DL 5X  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 OK-02-09132024-E2DL

Integration File: autoint1.e  
 Quant Time: Sep 26 01:16:53 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 091024.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Sep 09 17:11:47 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units  |
|--------------------------------|--------|----------|-------------|
| -----                          |        |          |             |
| System Monitoring Compounds    |        |          |             |
| 9) S ortho-Terphenyl (SURR)    | 11.866 | 704822   | 4.737 ug/ml |
| Spiked Amount                  | 50.000 | Recovery | = 9.47%     |
| 12) S 1-chlorooctadecane (S... | 13.300 | 605612   | 5.391 ug/ml |
| Spiked Amount                  | 50.000 | Recovery | = 10.78%    |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE092524AL\  
Data File : FE050344.D  
Signal(s) : FID1B.ch  
Acq On : 25 Sep 2024 10:29  
Operator : YP\AJ  
Sample : P4150-02DL 5X  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
OK-02-09132024-E2DL

Integration File: autoint1.e  
Quant Time: Sep 26 01:16:53 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 091024.M  
Quant Title : GC Extractables  
QLast Update : Mon Sep 09 17:11:47 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

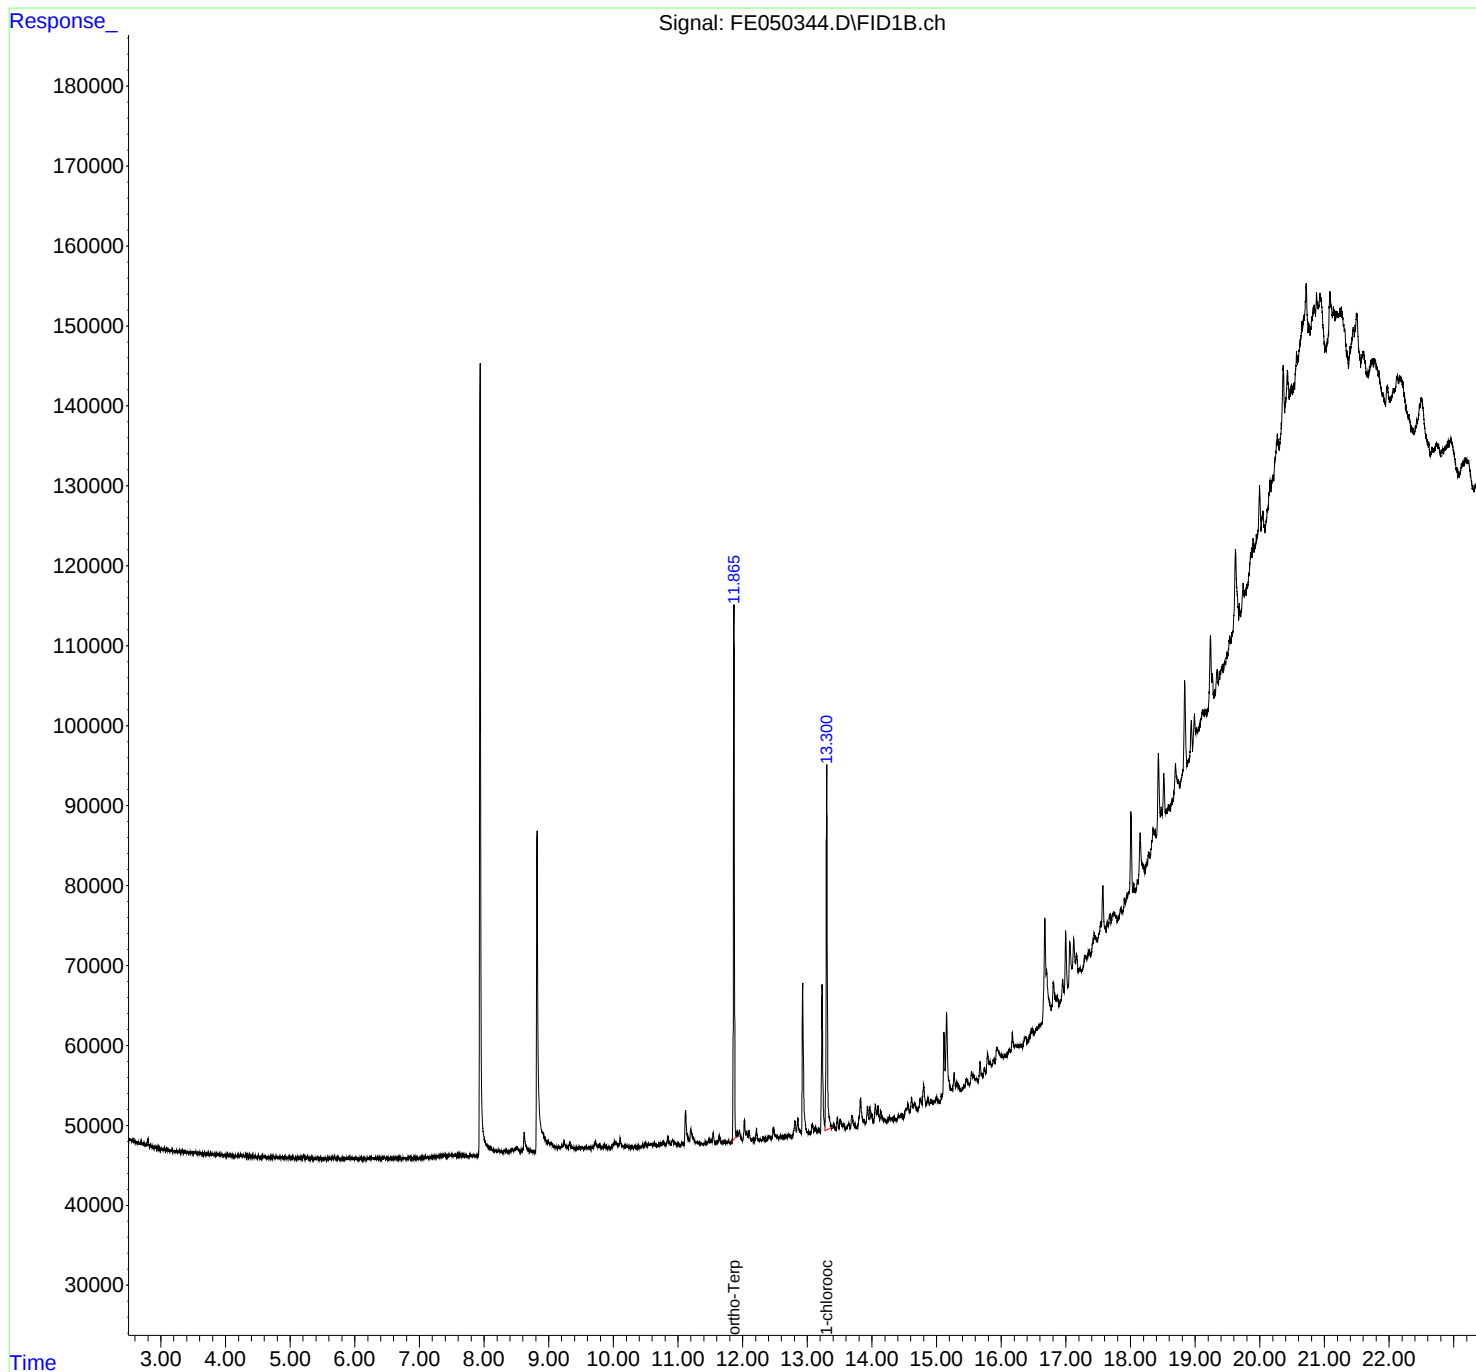


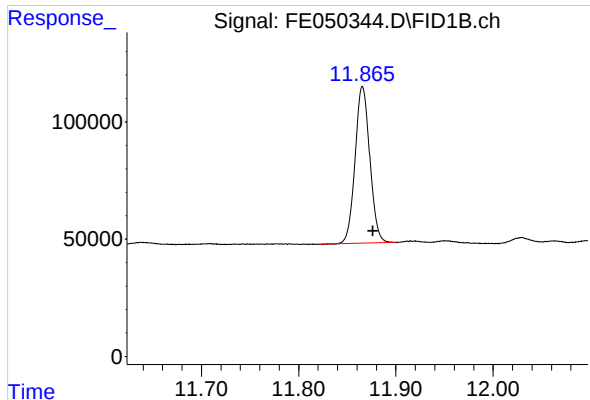

#9 ortho-Terphenyl (SURR)

R.T.: 11.866 min  
Delta R.T.: -0.011 min  
Response: 704822  
Conc: 4.74 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
OK-02-09132024-E2DL

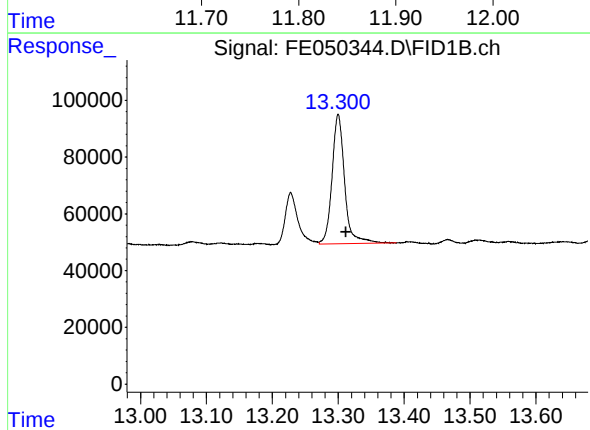

#12 1-chlorooctadecane (SURR)

R.T.: 13.300 min  
Delta R.T.: -0.012 min  
Response: 605612  
Conc: 5.39 ug/ml