

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092525AL\
Data File : FC069834.D
Signal(s) : FID1A.ch
Acq On : 25 Sep 2025 14:36
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 26 02:49:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092325.M
Quant Title : GC Extractables
QLast Update : Tue Sep 23 14:56:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.812	57163	0.327 ug/ml
18) T	n-Dotriacontane (C32)	18.645	95573	0.591 ug/ml
19) T	n-Tetratriacontane (C34)	19.429	69879	0.500 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092525AL\
Data File : FC069834.D
Signal(s) : FID1A.ch
Acq On : 25 Sep 2025 14:36
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 26 02:49:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092325.M
Quant Title : GC Extractables
QLast Update : Tue Sep 23 14:56:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

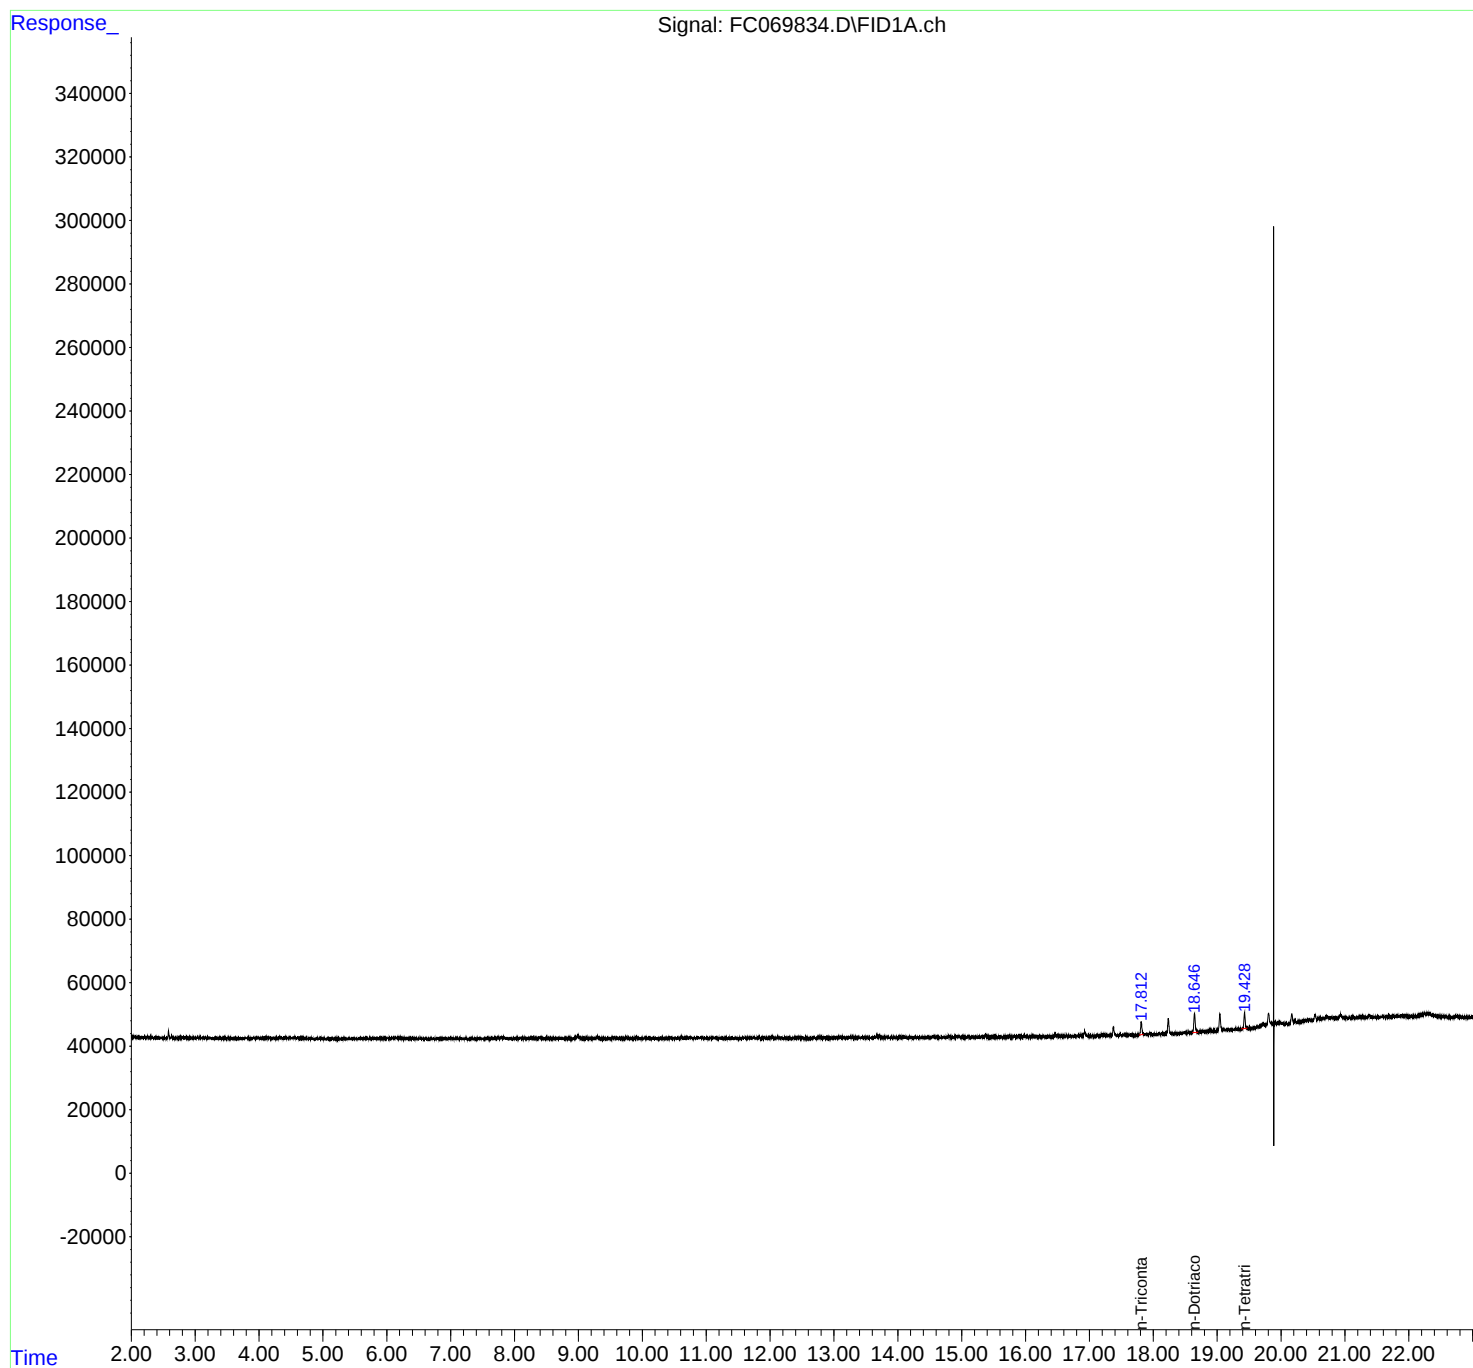


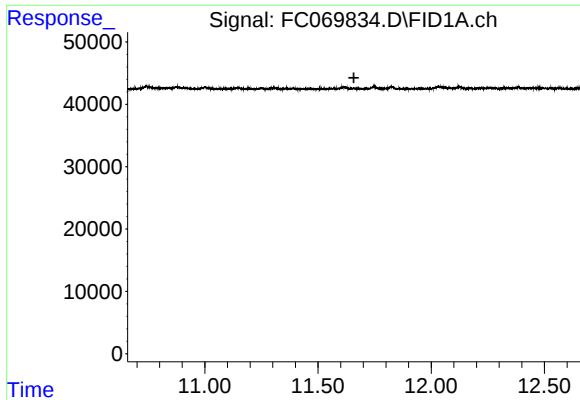

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.658 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

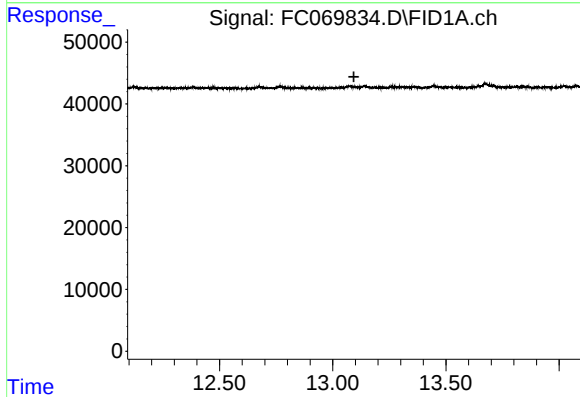


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.094 min
Response: 0
Conc: N.D.

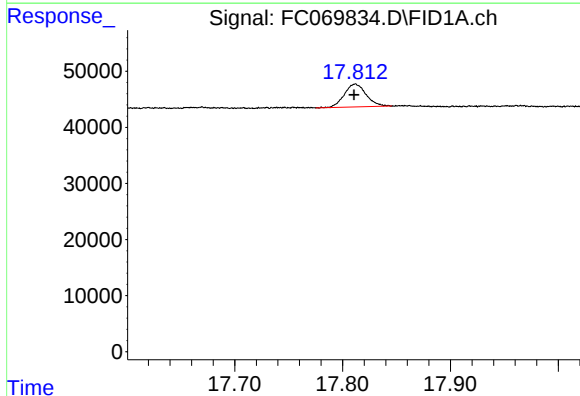


#17 n-Tricontane (C30)

R.T.: 17.812 min
Delta R.T.: 0.000 min
Response: 57163
Conc: 0.33 ug/ml

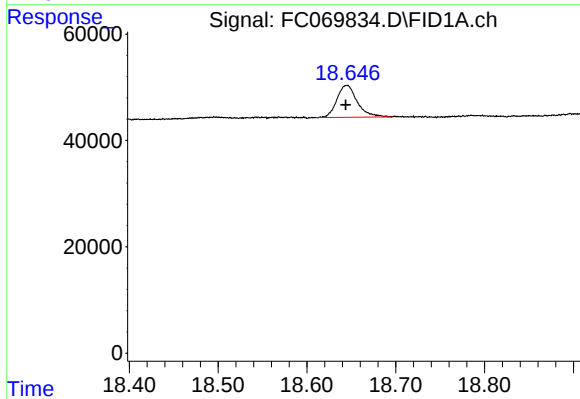

#18 n-Dotriacontane (C32)

R.T.: 18.645 min
Delta R.T.: 0.001 min
Response: 95573
Conc: 0.59 ug/ml

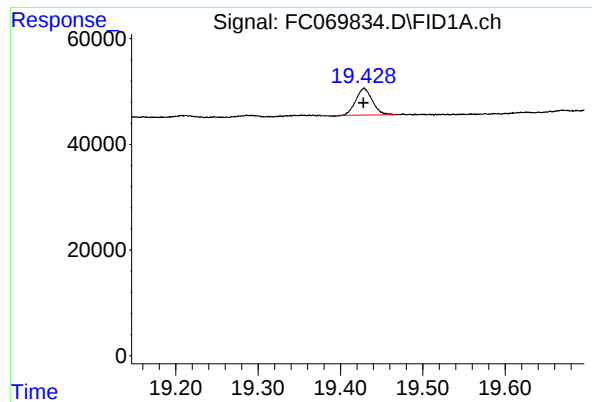

#19 n-Tetratriacontane (C34)

R.T.: 19.429 min
Delta R.T.: 0.000 min
Response: 69879
Conc: 0.50 ug/ml

Instrument :

FID_E

ClientSampleId :