

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092525AL\
Data File : FE055992.D
Signal(s) : FID1B.ch
Acq On : 25 Sep 2025 13:04
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 26 01:25:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092425.M
Quant Title : GC Extractables
QLast Update : Wed Sep 24 12:55:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.233	151881	1.025 ug/ml
18) T	n-Dotriacontane (C32)	19.069	176815	1.185 ug/ml
19) T	n-Tetratriacontane (C34)	19.853	114070	0.806 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092525AL\
Data File : FE055992.D
Signal(s) : FID1B.ch
Acq On : 25 Sep 2025 13:04
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 26 01:25:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092425.M
Quant Title : GC Extractables
QLast Update : Wed Sep 24 12:55:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

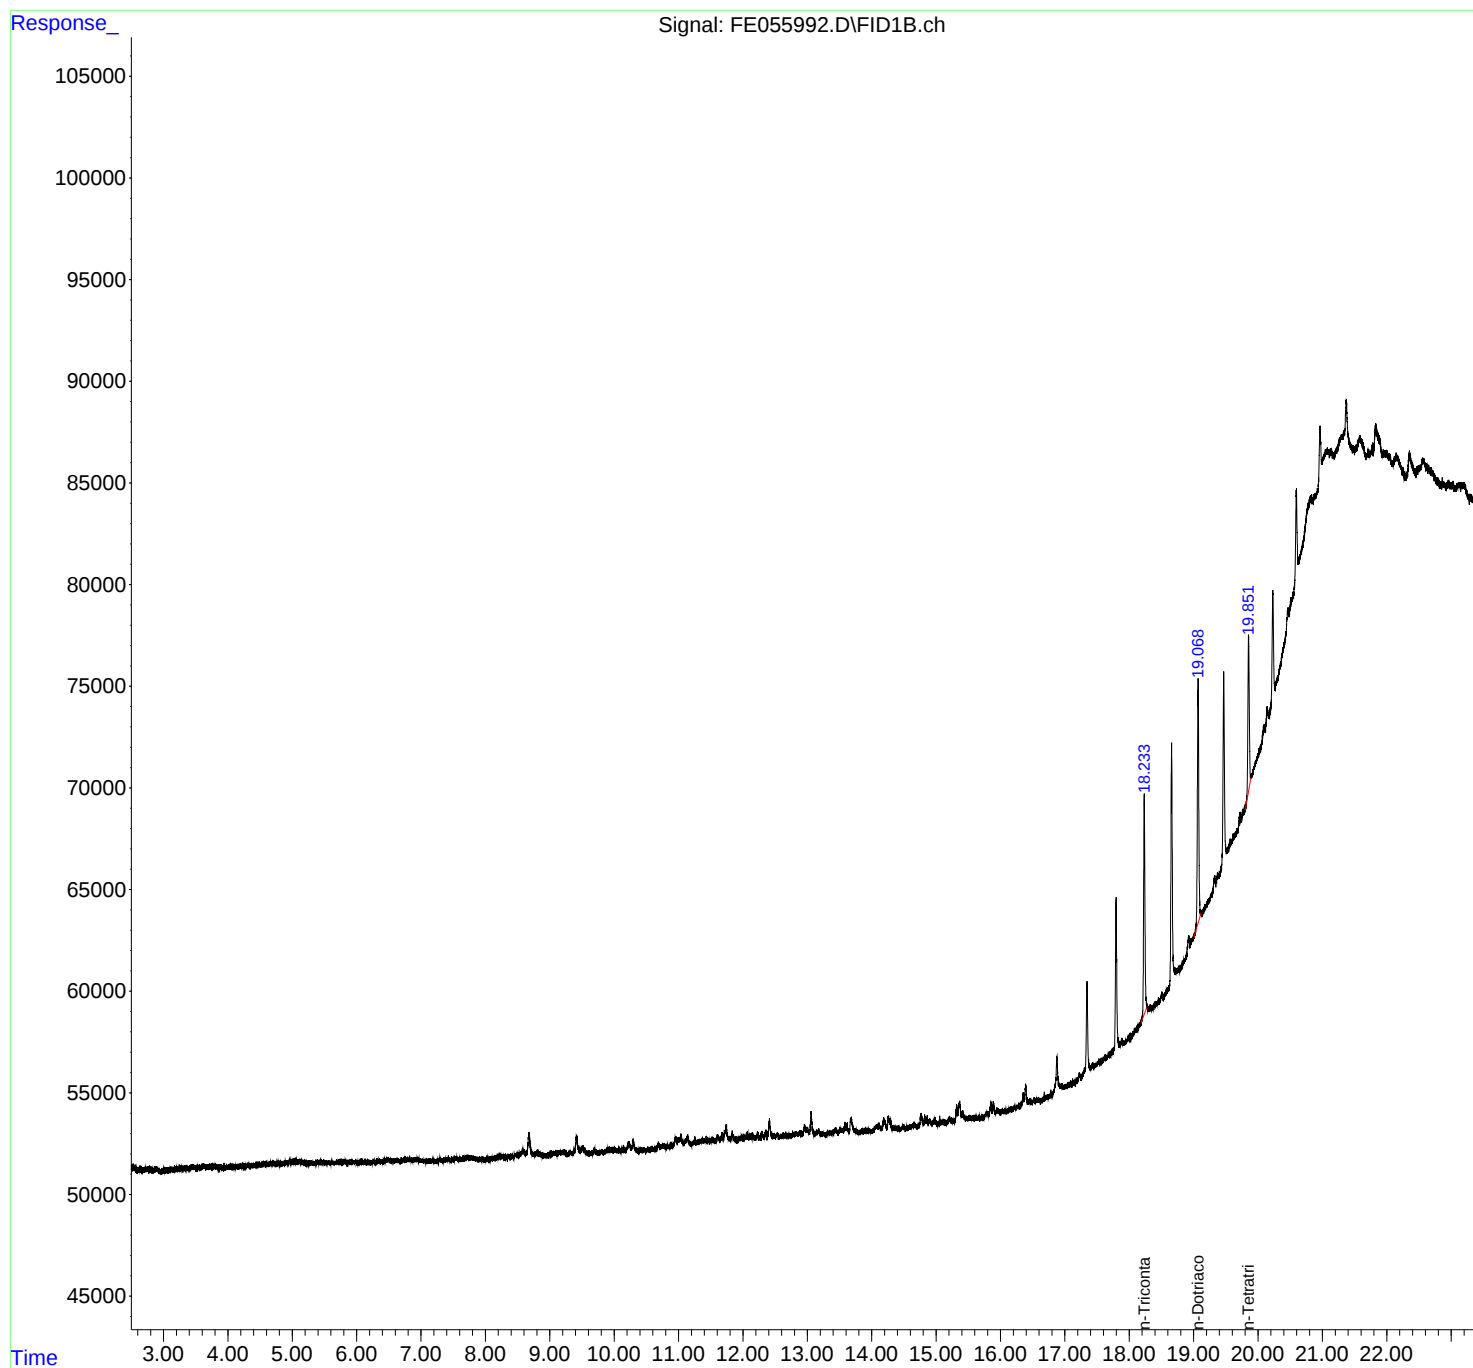


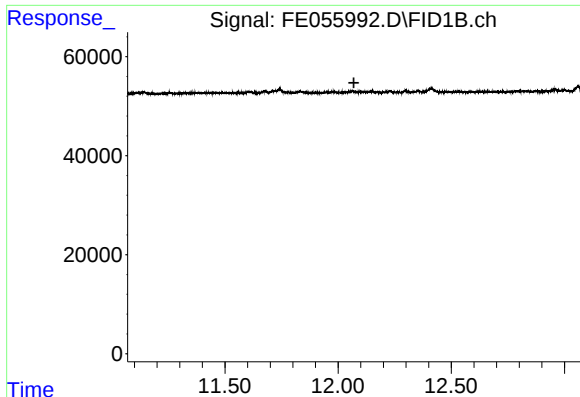

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 12.070 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
I.BLK

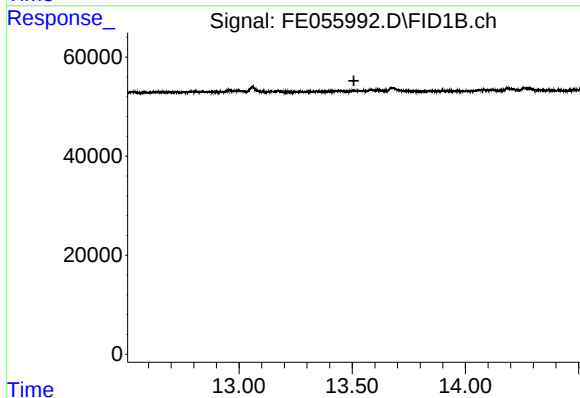


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.507 min
Response: 0
Conc: N.D.

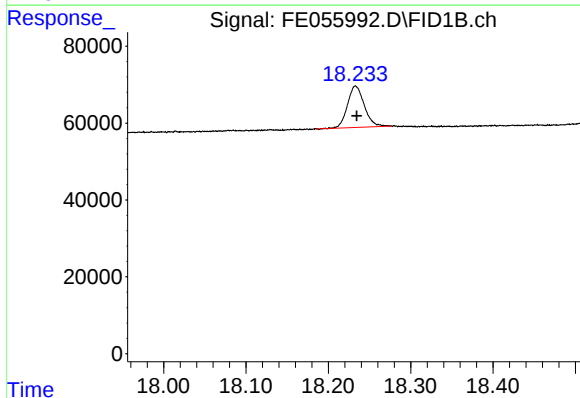


#17 n-Tricontane (C30)

R.T.: 18.233 min
Delta R.T.: -0.001 min
Response: 151881
Conc: 1.02 ug/ml

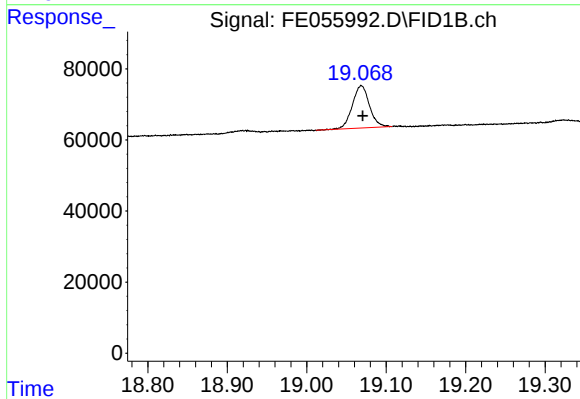

#18 n-Dotriacontane (C32)

R.T.: 19.069 min
Delta R.T.: -0.002 min
Response: 176815
Conc: 1.19 ug/ml

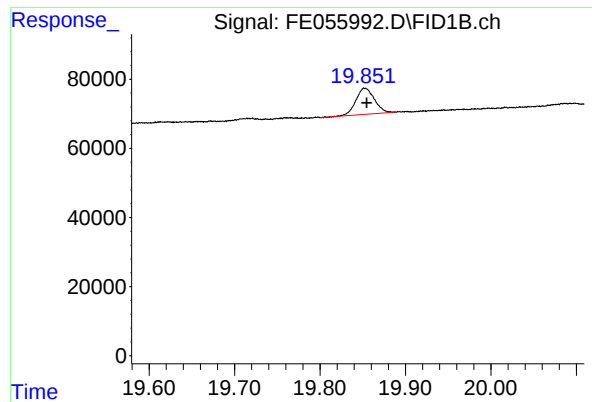

#19 n-Tetratriacontane (C34)

R.T.: 19.853 min
Delta R.T.: -0.002 min
Response: 114070
Conc: 0.81 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK