

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092619\
 Data File : FE030576.D
 Signal(s) : FID1B.CH
 Acq On : 26 Sep 2019 16:42
 Operator : DD\AJ
 Sample : K5020-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 27 00:40:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE092619.M
 Quant Title :
 QLast Update : Thu Sep 26 13:30:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.676	4670508	15.228 ug/ml
Target Compounds			
6) N-TETRADECANE	8.282	1643993	5.170 ug/ml
7) N-HEXADECANE	9.837	102843	0.328 ug/ml
9) N-EICOSANE	12.637	65381	0.214 ug/ml
10) N-TETRACOSANE	14.676	4670508	30.456 ug/ml
11) N-OCTACOSANE	16.846	288067	0.994 ug/ml
12) N-DOTRIACONTANE	18.563	381849	1.369 ug/ml
14) N-HEXATRIACONTANE	20.092	88925	0.349 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092619\
Data File : FE030576.D
Signal(s) : FID1B.CH
Acq On : 26 Sep 2019 16:42
Operator : DD\AJ
Sample : K5020-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 27 00:40:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE092619.M
Quant Title :
QLast Update : Thu Sep 26 13:30:16 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

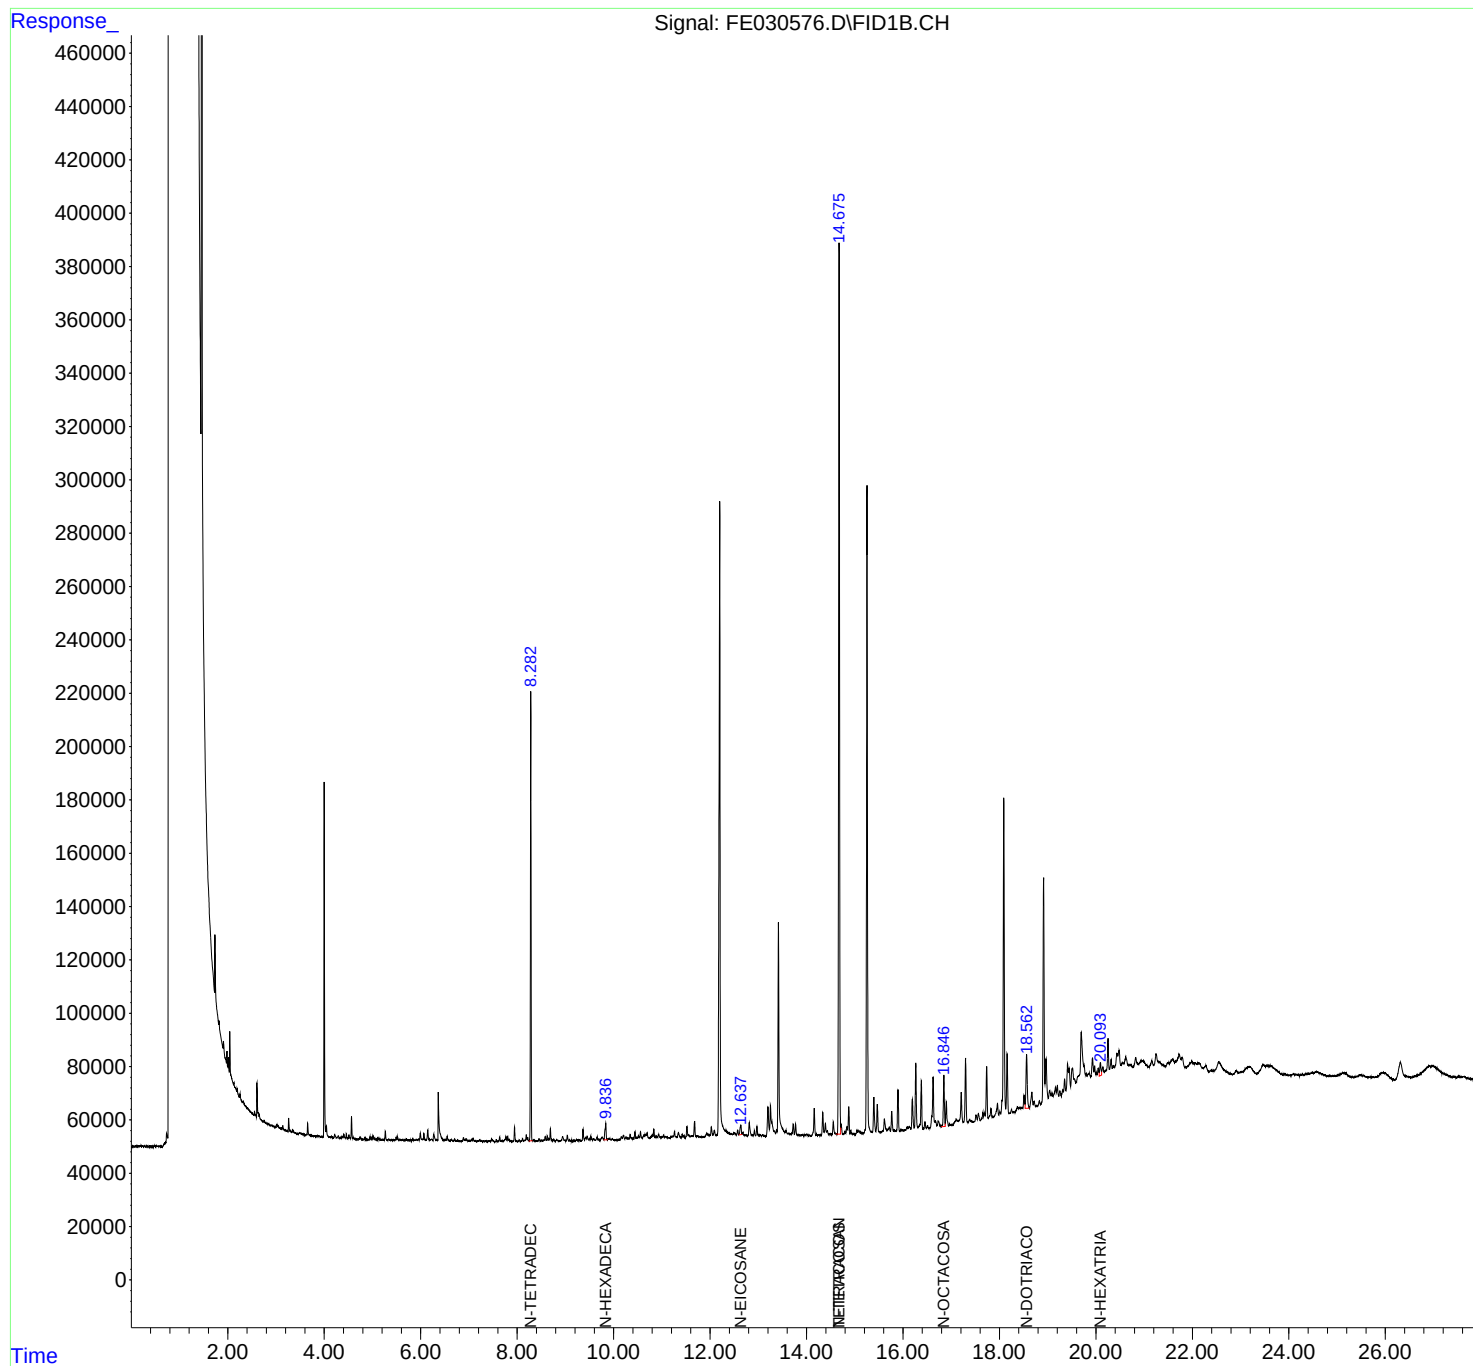

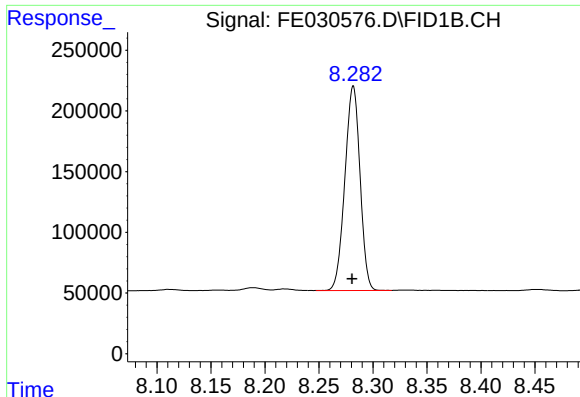


#6 N-TETRADECANE

R.T.: 8.282 min
Delta R.T.: 0.001 min
Response: 1643993
Conc: 5.17 ug/ml

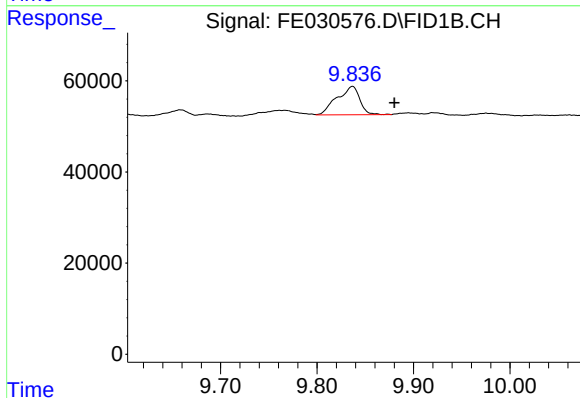


#7 N-HEXADECANE

R.T.: 9.837 min
Delta R.T.: -0.044 min
Response: 102843
Conc: 0.33 ug/ml

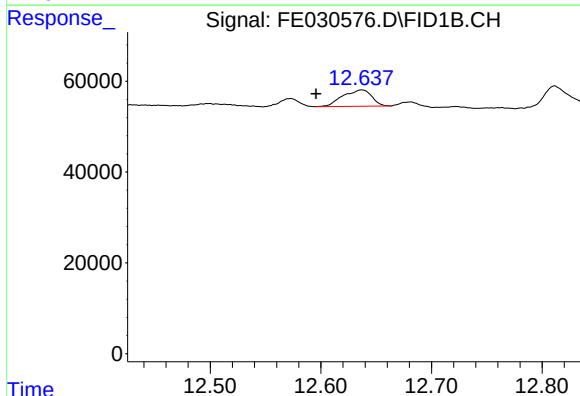


#9 N-EICOSANE

R.T.: 12.637 min
Delta R.T.: 0.041 min
Response: 65381
Conc: 0.21 ug/ml

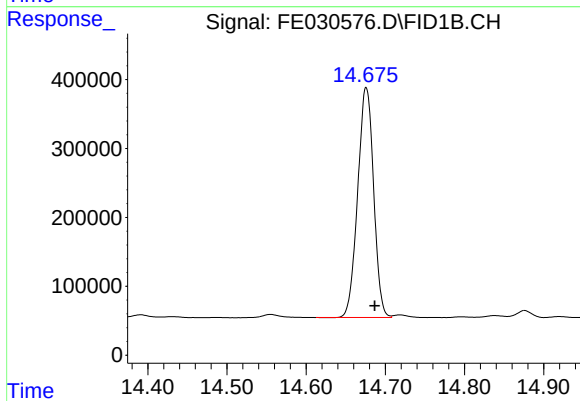


#10 N-TETRACOSANE

R.T.: 14.676 min
Delta R.T.: -0.011 min
Response: 4670508
Conc: 30.46 ug/ml

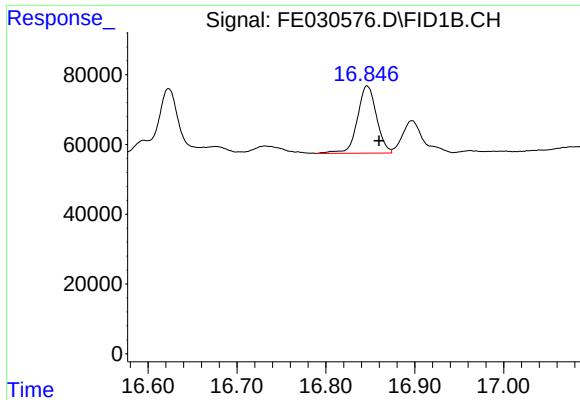


#11 N-OCTACOSANE

R.T.: 16.846 min
Delta R.T.: -0.014 min
Response: 288067
Conc: 0.99 ug/ml

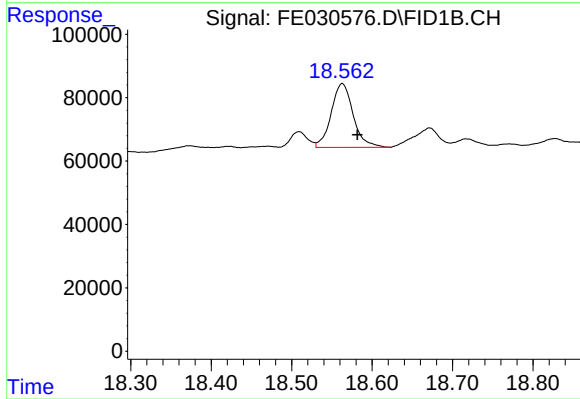


#12 N-DOTRIACONTANE

R.T.: 18.563 min
Delta R.T.: -0.019 min
Response: 381849
Conc: 1.37 ug/ml

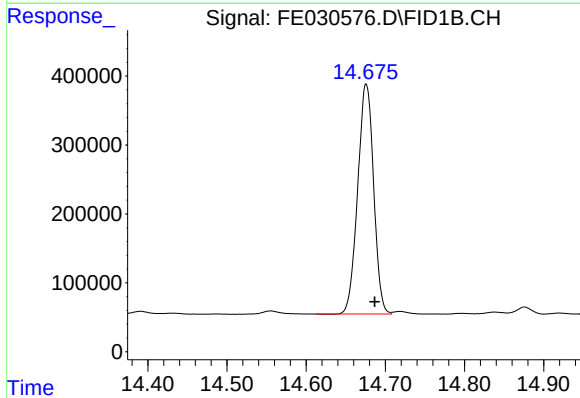

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.676 min
Delta R.T.: -0.011 min
Response: 4670508
Conc: 15.23 ug/ml

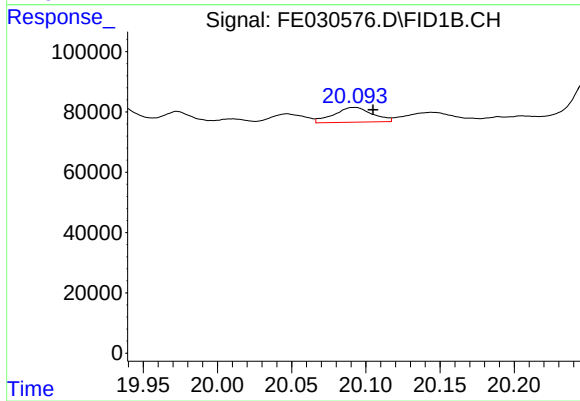

#14 N-HEXATRIACONTANE

R.T.: 20.092 min
Delta R.T.: -0.013 min
Response: 88925
Conc: 0.35 ug/ml