

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092622\
 Data File : FB028447.D
 Signal(s) : FID2B.CH
 Acq On : 26 Sep 2022 12:01
 Operator : AJ/MA
 Sample : BSF0926S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 27 02:10:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	240933	20.130 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.717	654462	32.324 ng/ml
2) t	2,2,4-Trimethylpentane	7.434	687268	32.671 ng/ml
3) t	n-Heptane	7.759	225548	10.492 ng/ml
4) t	Benzene	7.894	264342	10.745 ng/ml
6) t	Toluene	10.628	777043	33.376 ng/ml
7) t	Ethylbenzene	13.065	240258	10.804 ng/ml
8) t	m-Xylene	13.198	475844	21.805 ng/ml
9) t	O-Xylene	13.925	456114	21.770 ng/ml
10) t	1,2,4-Trimethylbenzene	16.199	438045	21.786 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092622\
Data File : FB028447.D
Signal(s) : FID2B.CH
Acq On : 26 Sep 2022 12:01
Operator : AJ/MA
Sample : BSF0926S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 27 02:10:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

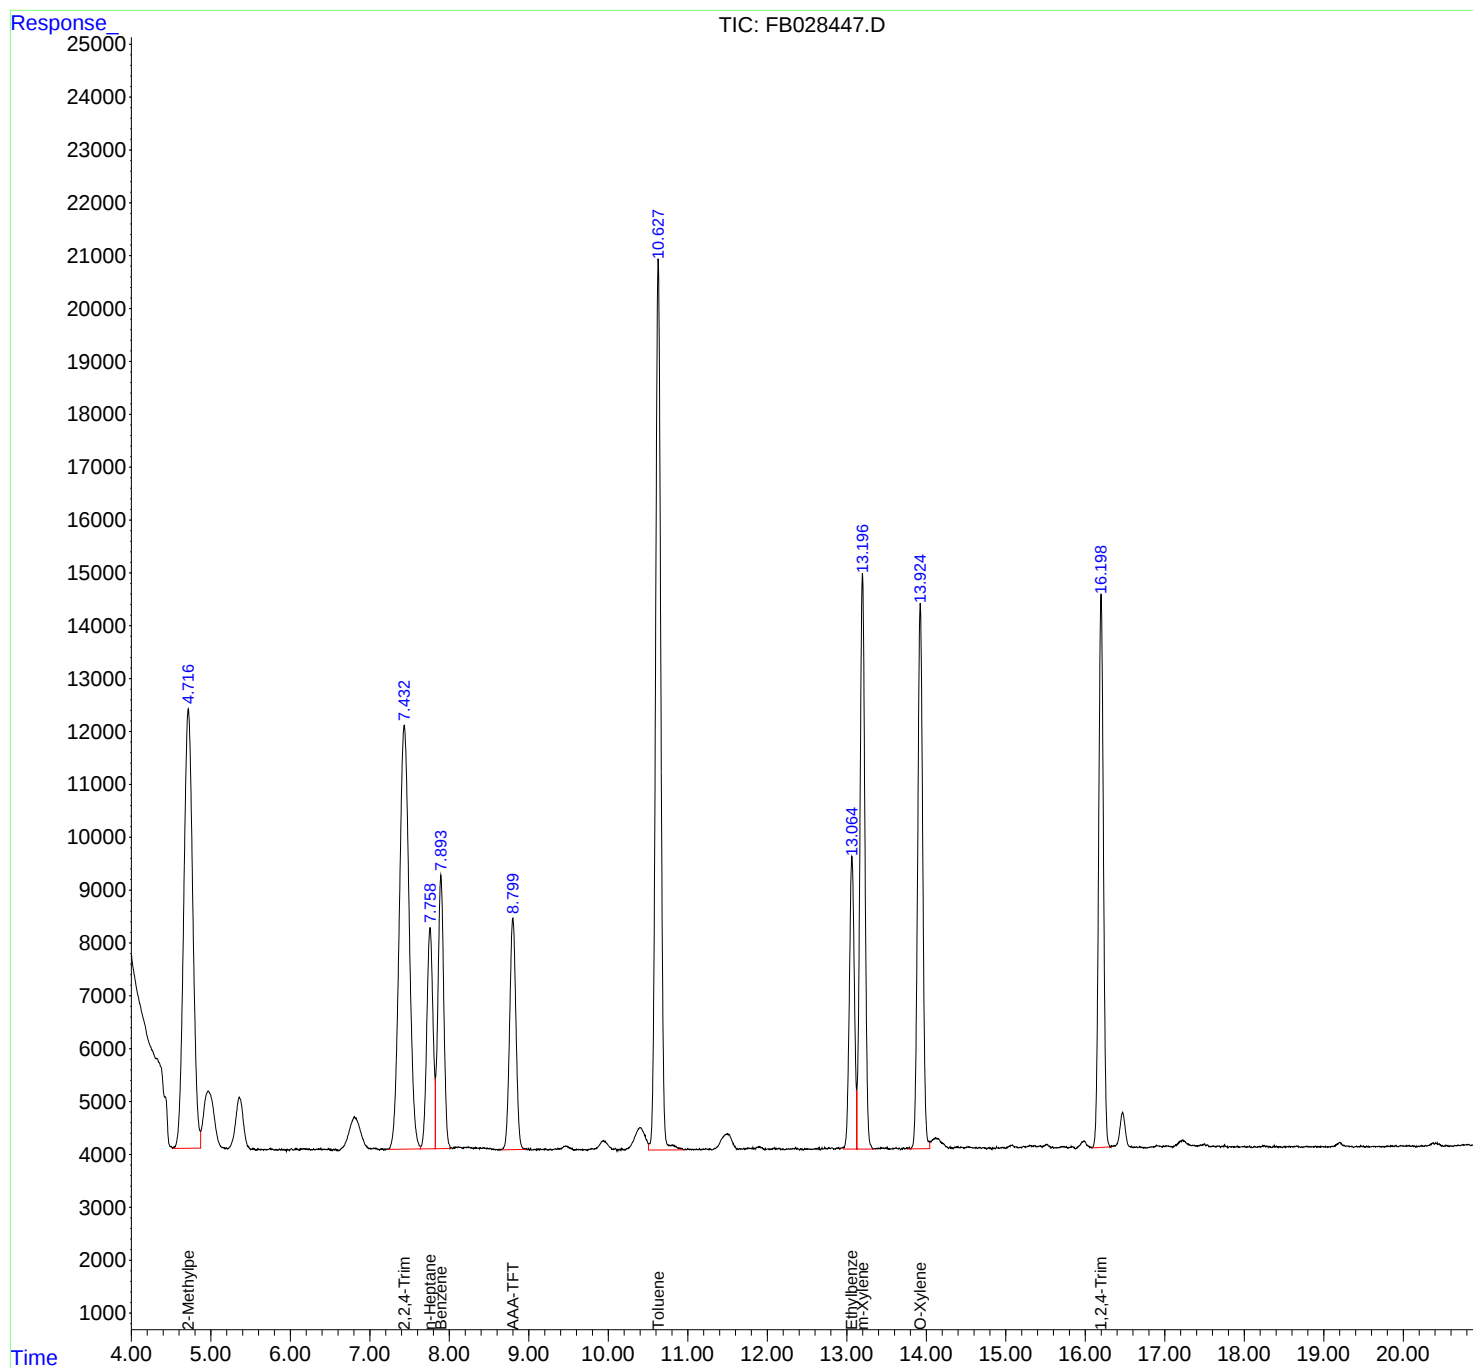


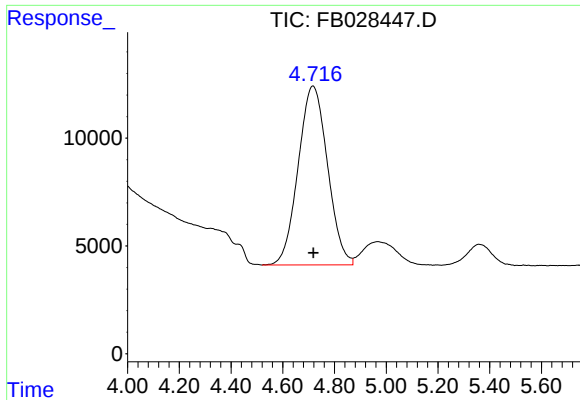

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.000 min
Response: 654462
Conc: 32.32 ng/ml

Instrument :
FID_E
ClientSampleId :

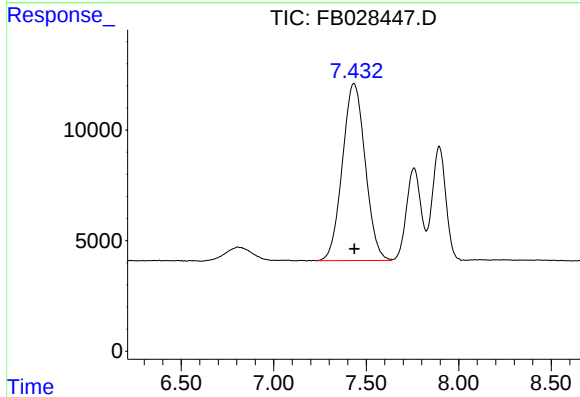


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: -0.003 min
Response: 687268
Conc: 32.67 ng/ml

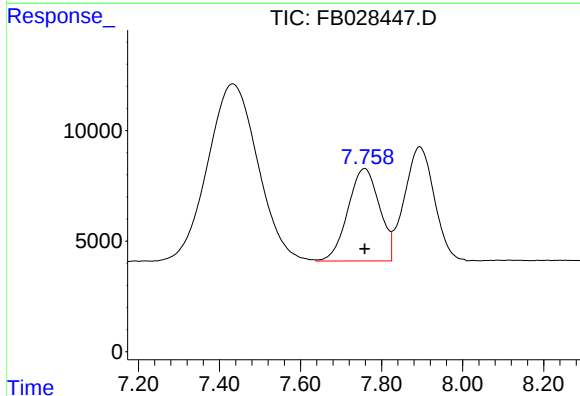


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 225548
Conc: 10.49 ng/ml

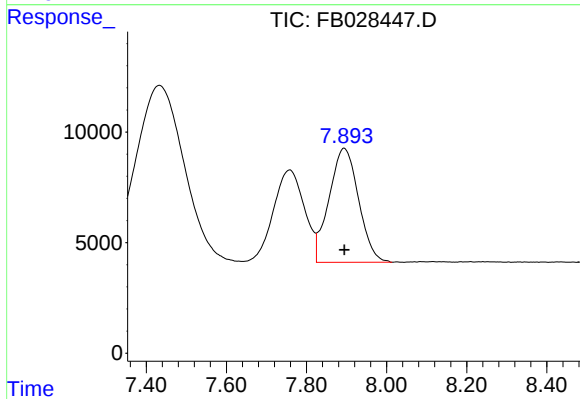

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 264342
Conc: 10.75 ng/ml

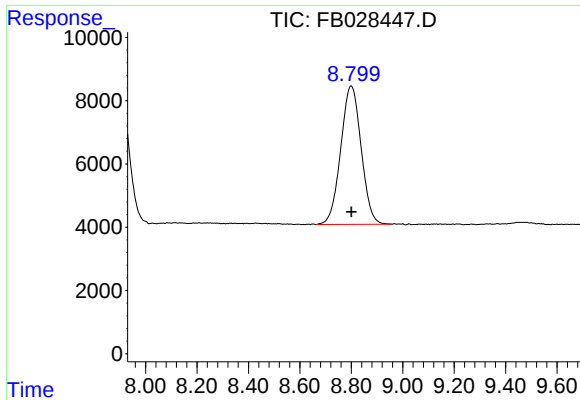

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 240933
Conc: 20.13 ng/ml

Instrument :
FID_E
ClientSampleId :

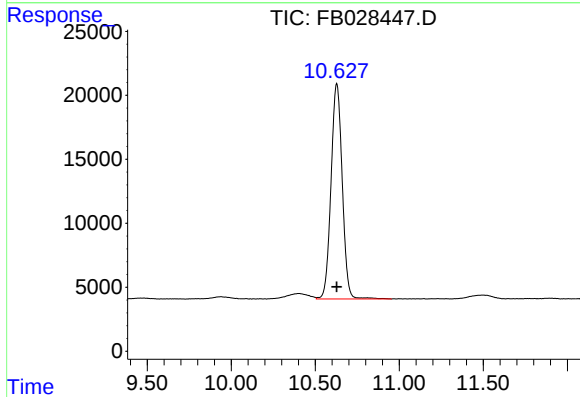


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 777043
Conc: 33.38 ng/ml

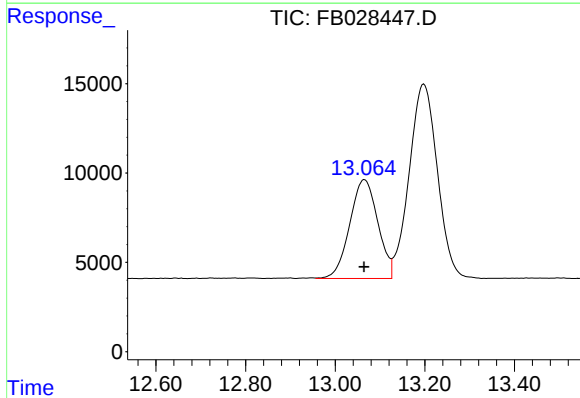


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.000 min
Response: 240258
Conc: 10.80 ng/ml

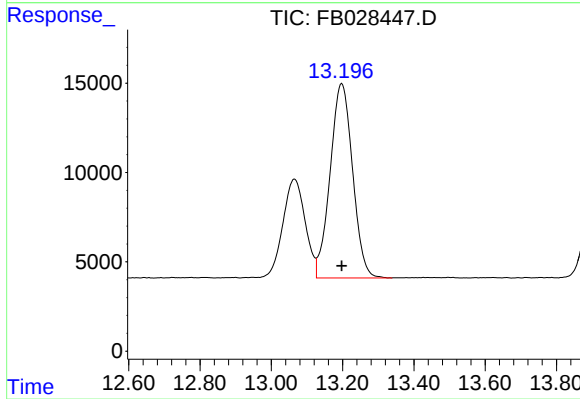

#8 m-Xylene


R.T.: 13.198 min
Delta R.T.: 0.000 min
Response: 475844
Conc: 21.81 ng/ml

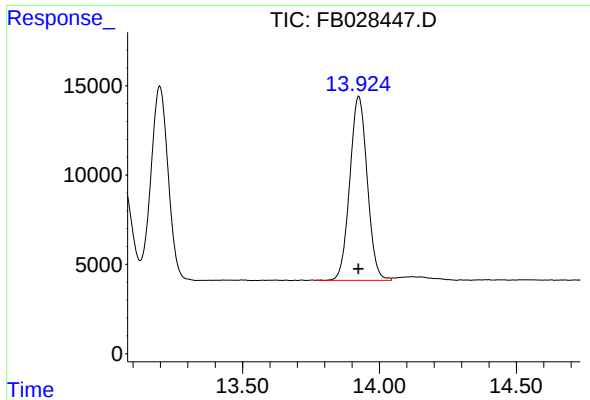

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.000 min
Response: 456114
Conc: 21.77 ng/ml

Instrument :
FID_E
ClientSampleId :

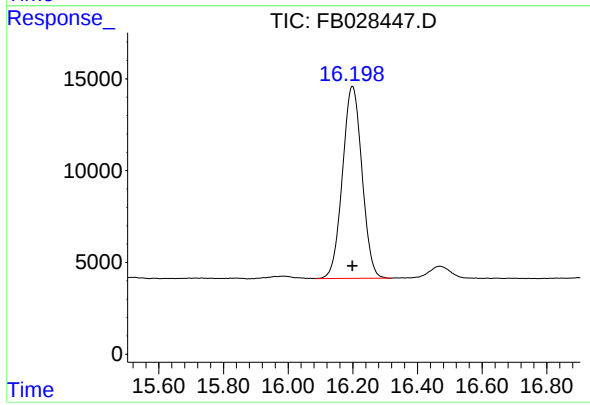

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.000 min
Response: 438045
Conc: 21.79 ng/ml