

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092719\
 Data File : FE030592.D
 Signal(s) : FID1B.CH
 Acq On : 27 Sep 2019 13:52
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 27 15:07:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE092619.M
 Quant Title :
 QLast Update : Thu Sep 26 13:30:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.675	6348385	20.698 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.675	6348385	41.397 ug/ml
11)	N-OCTACOSANE	16.843	55356	0.191 ug/ml
12)	N-DOTRIACONTANE	18.562	187096	0.671 ug/ml
14)	N-HEXATRIACONTANE	20.086	54490	0.214 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092719\
Data File : FE030592.D
Signal(s) : FID1B.CH
Acq On : 27 Sep 2019 13:52
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 27 15:07:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE092619.M
Quant Title :
QLast Update : Thu Sep 26 13:30:16 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

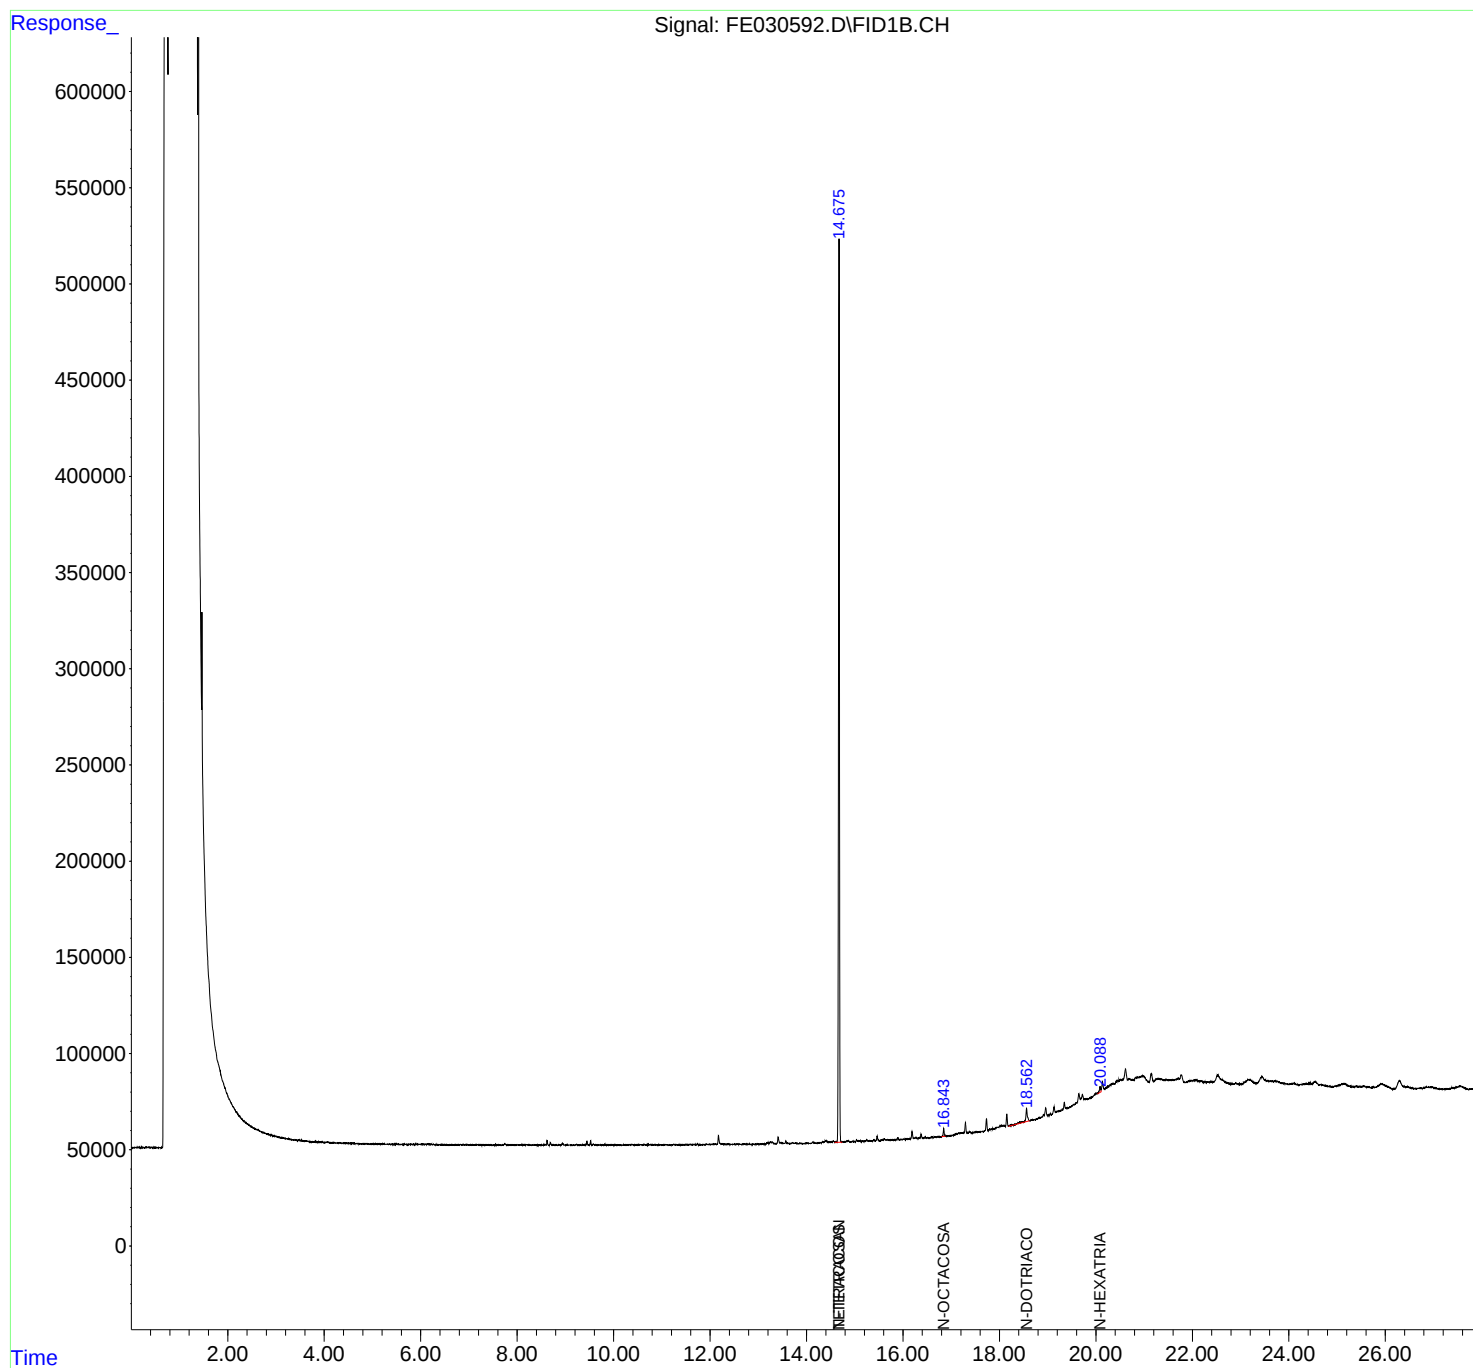

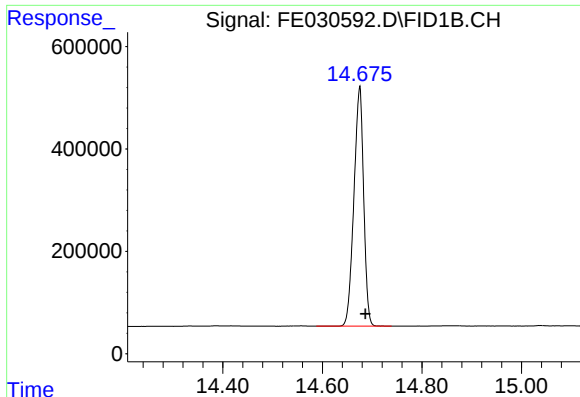


#10 N-TETRACOSANE

R.T.: 14.675 min
Delta R.T.: -0.012 min
Response: 6348385
Conc: 41.40 ug/ml

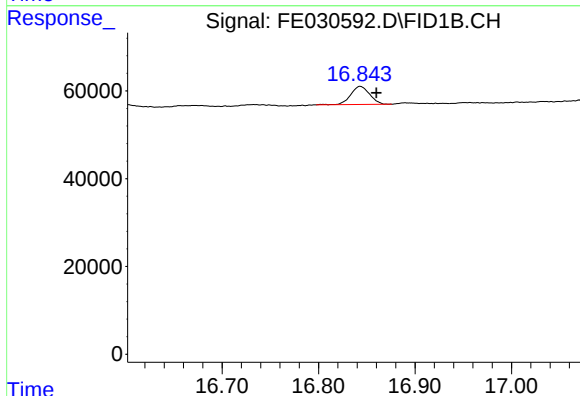


#11 N-OCTACOSANE

R.T.: 16.843 min
Delta R.T.: -0.017 min
Response: 55356
Conc: 0.19 ug/ml

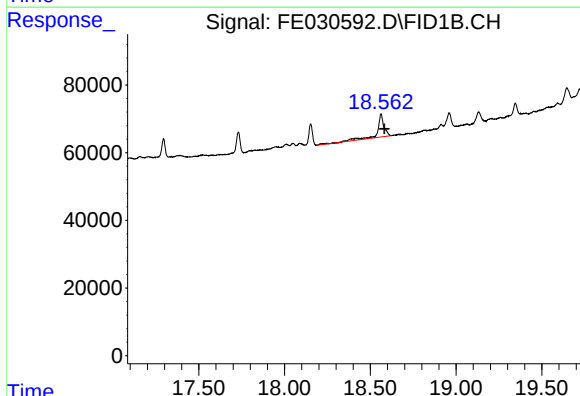


#12 N-DOTRIACONTANE

R.T.: 18.562 min
Delta R.T.: -0.019 min
Response: 187096
Conc: 0.67 ug/ml

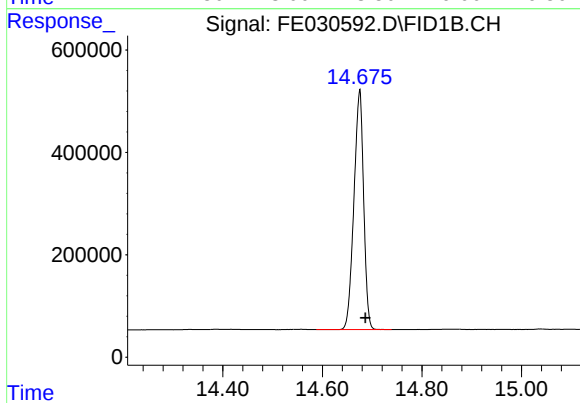

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.675 min
Delta R.T.: -0.012 min
Response: 6348385
Conc: 20.70 ug/ml

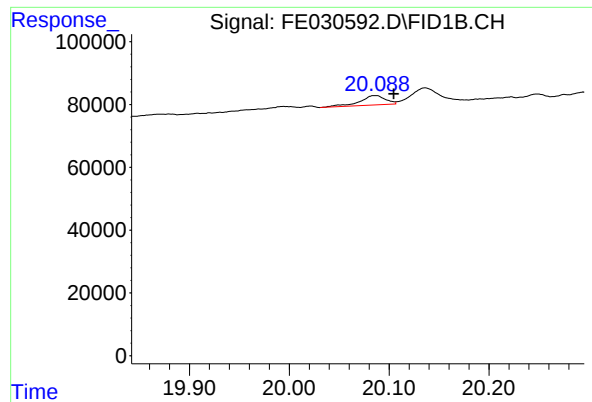

#14 N-HEXATRIACONTANE

R.T.: 20.086 min
Delta R.T.: -0.019 min
Response: 54490
Conc: 0.21 ug/ml