

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092925AL\
Data File : FC069865.D
Signal(s) : FID1A.ch
Acq On : 29 Sep 2025 15:24
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 30 04:33:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092325.M
Quant Title : GC Extractables
QLast Update : Tue Sep 23 14:56:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
8) T	n-Octadecane (C18)	11.402f	68524	0.384 ug/ml
15) T	n-Hexacosane (C26)	16.022	9490293	52.270 ug/ml
19) T	n-Tetratriacontane (C34)	19.409	1864132	13.339 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092925AL\
Data File : FC069865.D
Signal(s) : FID1A.ch
Acq On : 29 Sep 2025 15:24
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 30 04:33:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092325.M
Quant Title : GC Extractables
QLast Update : Tue Sep 23 14:56:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

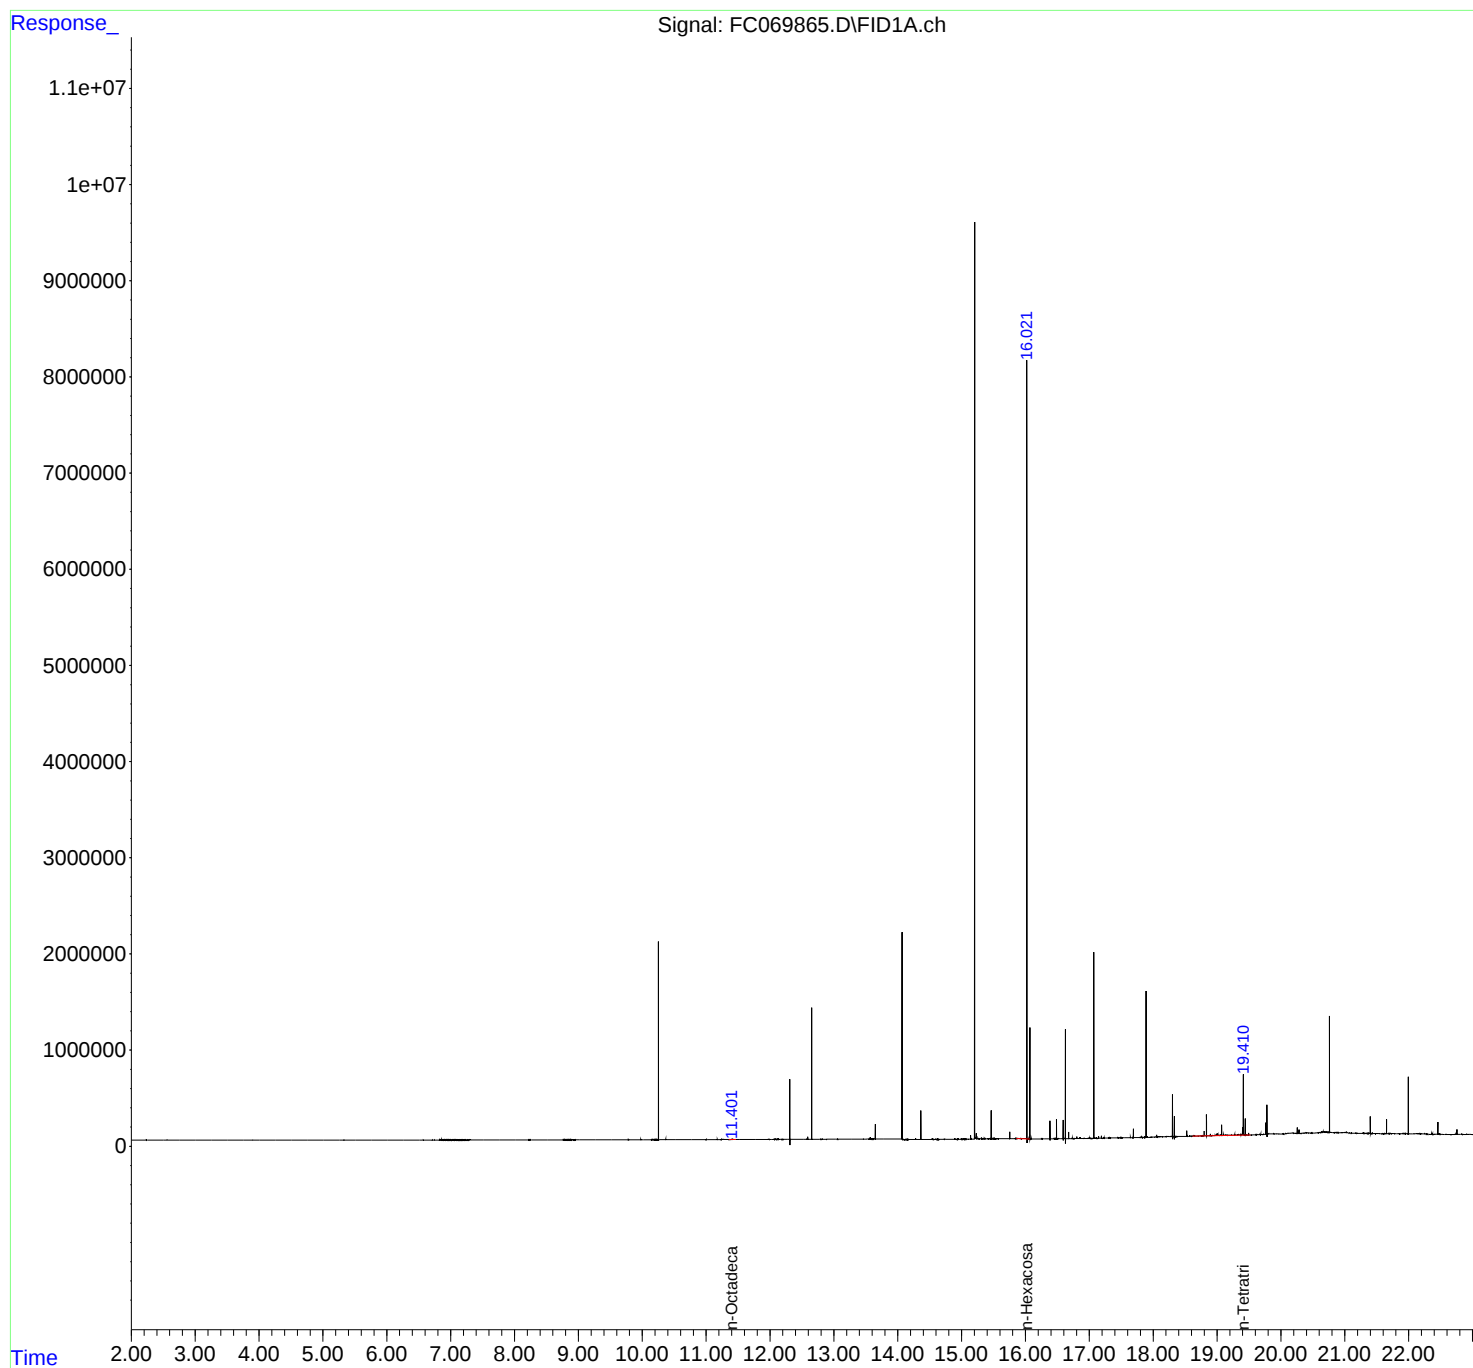


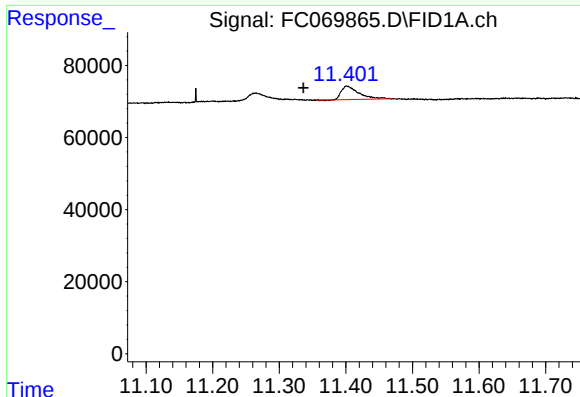

#8 n-Octadecane (C18)


R.T.: 11.402 min
Delta R.T.: 0.066 min
Response: 68524
Conc: 0.38 ug/ml

Instrument :
FID_E
ClientSampleId :

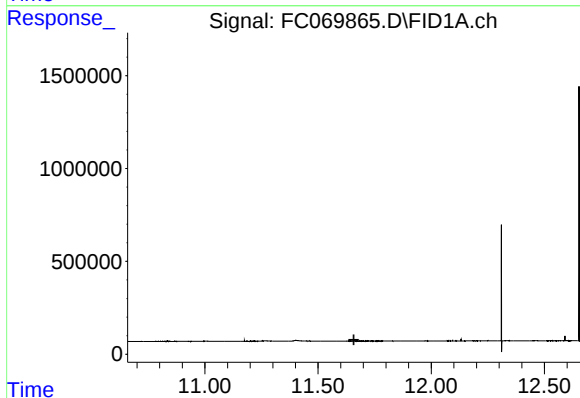


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.658 min
Response: 0
Conc: N.D.

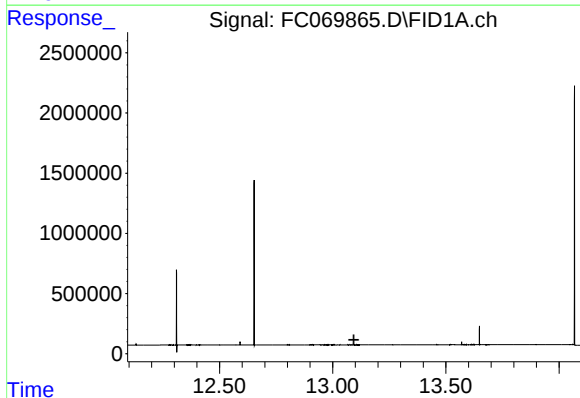


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.094 min
Response: 0
Conc: N.D.

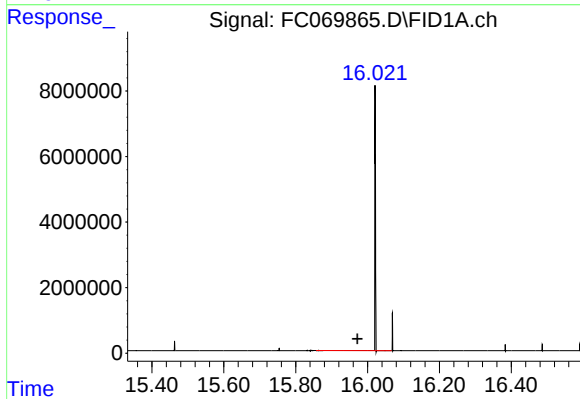

#15 n-Hexacosane (C26)

R.T.: 16.022 min
Delta R.T.: 0.049 min
Response: 9490293
Conc: 52.27 ug/ml

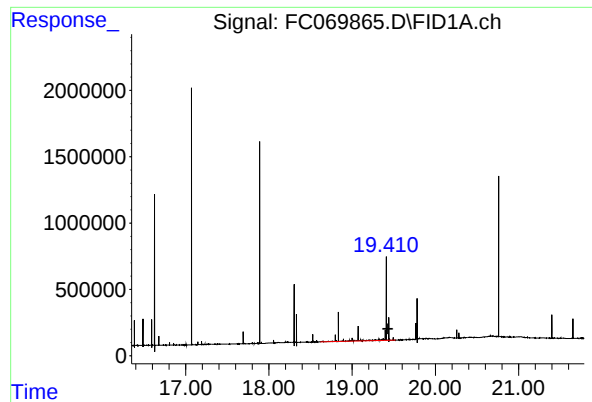

#19 n-Tetratriacontane (C34)

R.T.: 19.409 min
Delta R.T.: -0.019 min
Response: 1864132
Conc: 13.34 ug/ml

Instrument :
FID_E
ClientSampleId :