

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE092925AL\  
 Data File : FE056050.D  
 Signal(s) : FID1B.ch  
 Acq On : 29 Sep 2025 17:23  
 Operator : YP\AJ  
 Sample : Q3208-03  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Sep 30 00:29:33 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 092425.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Sep 24 12:55:37 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 12.076 | 6730686    | 35.868 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 71.74%       |
| 12) S 1-chlorooctadecane (S... | 13.512 | 5453615    | 39.076 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 78.15%       |
|                                |        |            |              |
| Target Compounds               |        |            |              |
| 14) T n-Tetracosane (C24)      | 15.364 | 602643     | 3.955 ug/ml  |
| 15) T n-Hexacosane (C26)       | 16.393 | 136338     | 0.956 ug/ml  |
| 16) T n-Octacosane (C28)       | 17.345 | 133271     | 0.957 ug/ml  |
| 17) T n-Tricontane (C30)       | 18.236 | 436971     | 2.949 ug/ml  |
| 18) T n-Dotriacontane (C32)    | 19.069 | 853882     | 5.723 ug/ml  |
| 19) T n-Tetratriacontane (C34) | 19.855 | 222197     | 1.571 ug/ml  |
| 20) T n-Hexatriacontane (C36)  | 20.597 | 149505     | 1.165 ug/ml  |
| 22) T n-Tetracontane (C40)     | 22.377 | 219415     | 1.844 ug/ml  |
| -----                          |        |            |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE092925AL\  
Data File : FE056050.D  
Signal(s) : FID1B.ch  
Acq On : 29 Sep 2025 17:23  
Operator : YP\AJ  
Sample : Q3208-03  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Sep 30 00:29:33 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 092425.M  
Quant Title : GC Extractables  
QLast Update : Wed Sep 24 12:55:37 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

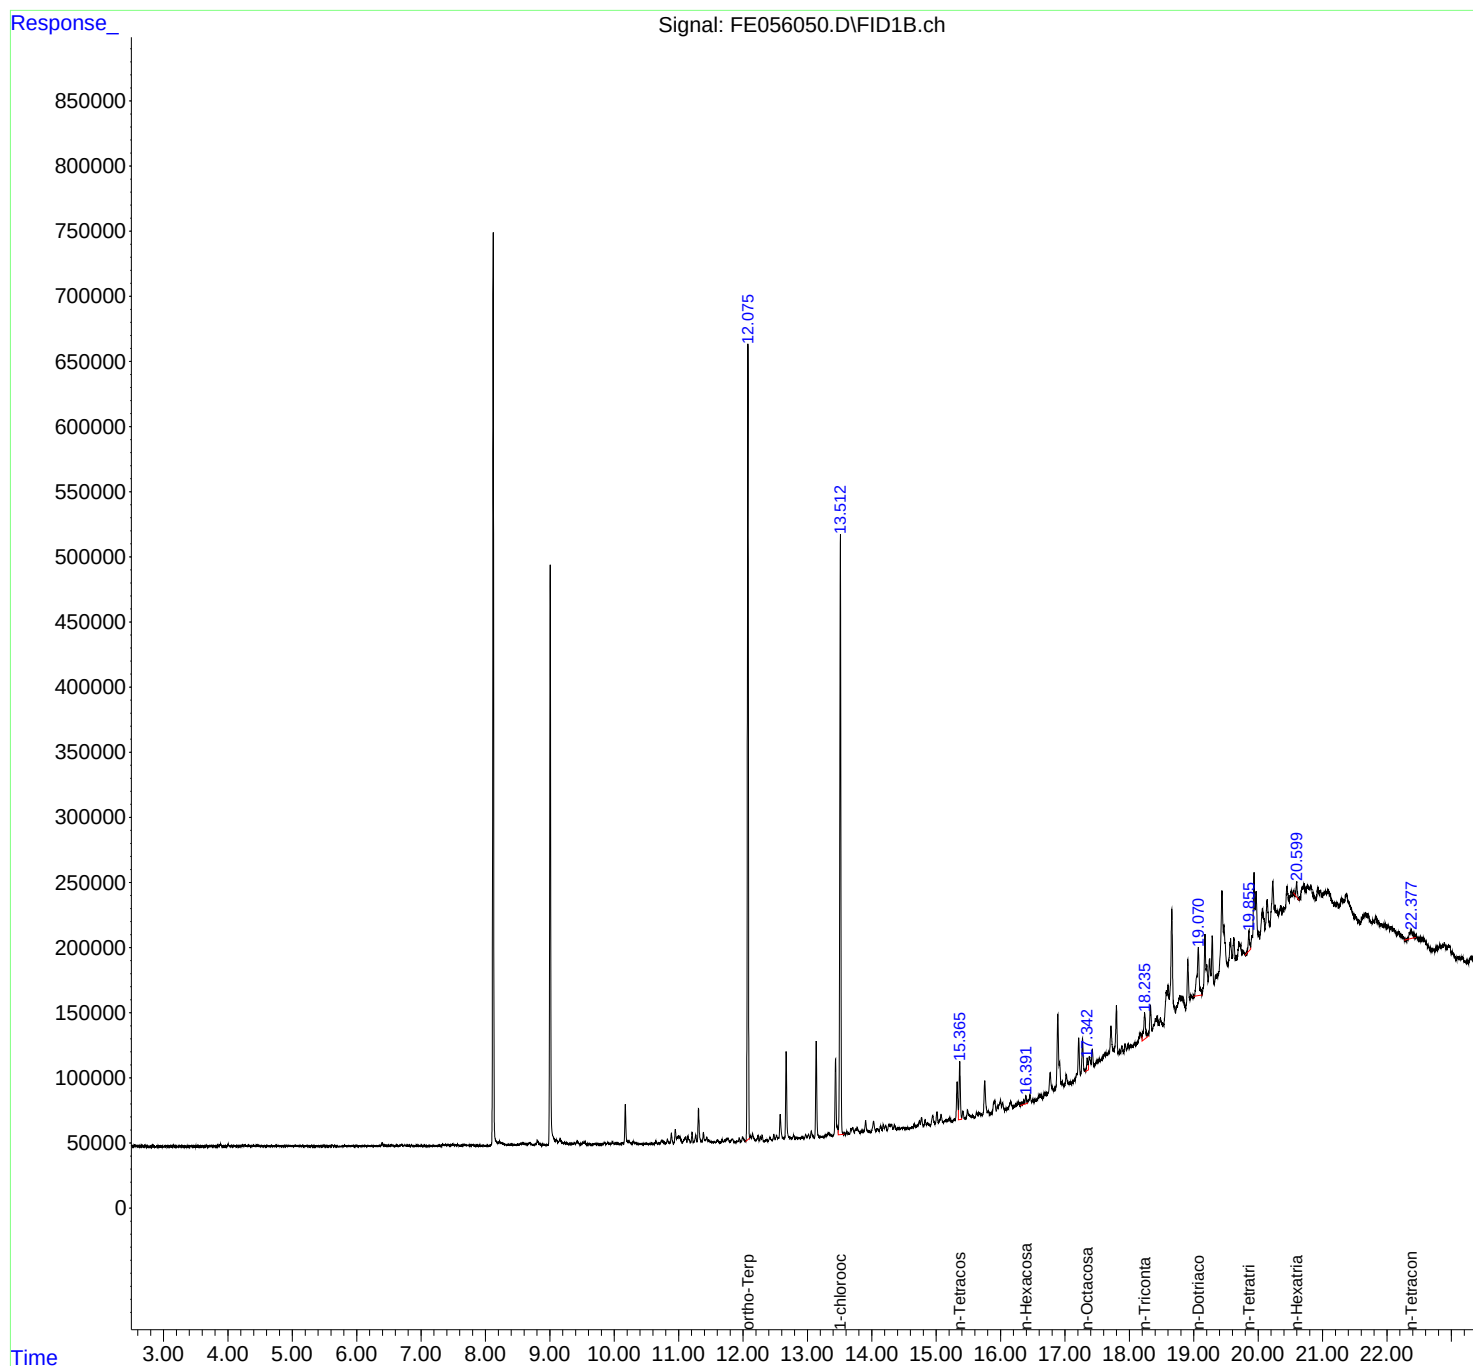


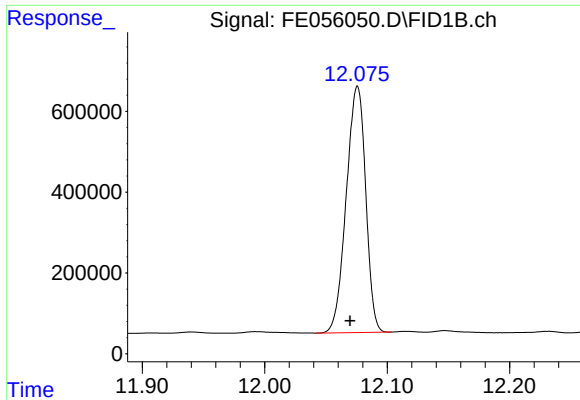

#9 ortho-Terphenyl (SURR)


R.T.: 12.076 min  
Delta R.T.: 0.006 min  
Response: 6730686  
Conc: 35.87 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

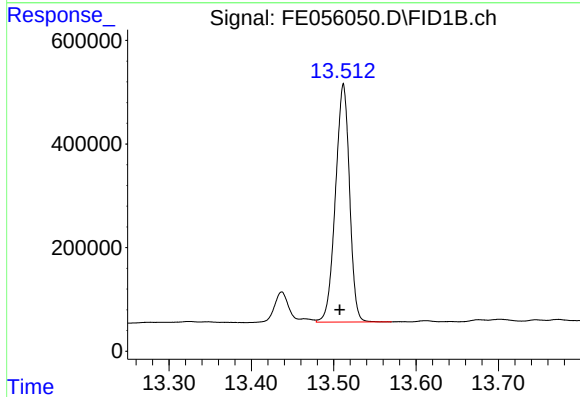


#12 1-chlorooctadecane (SURR)

R.T.: 13.512 min  
Delta R.T.: 0.004 min  
Response: 5453615  
Conc: 39.08 ug/ml

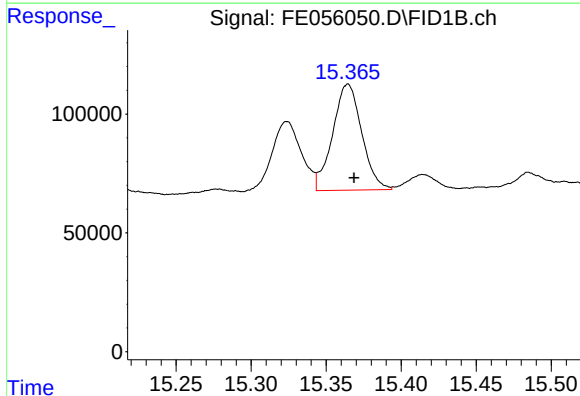


#14 n-Tetracosane (C24)

R.T.: 15.364 min  
Delta R.T.: -0.004 min  
Response: 602643  
Conc: 3.95 ug/ml

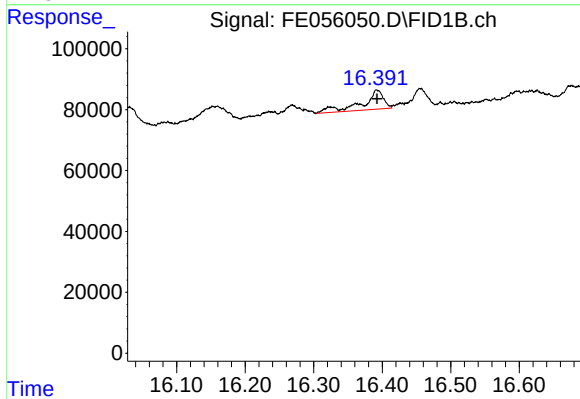

#15 n-Hexacosane (C26)


R.T.: 16.393 min  
Delta R.T.: 0.000 min  
Response: 136338  
Conc: 0.96 ug/ml

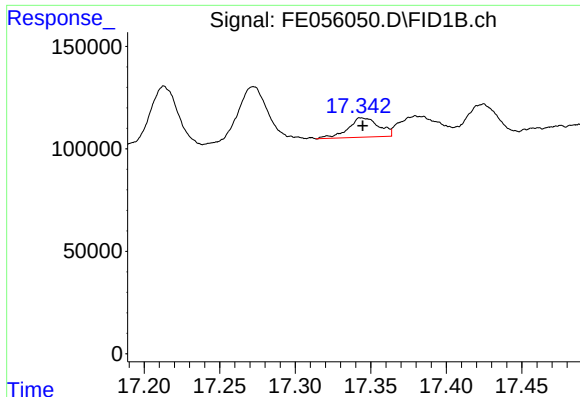

#16 n-Octacosane (C28)


R.T.: 17.345 min  
Delta R.T.: 0.000 min  
Response: 133271  
Conc: 0.96 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

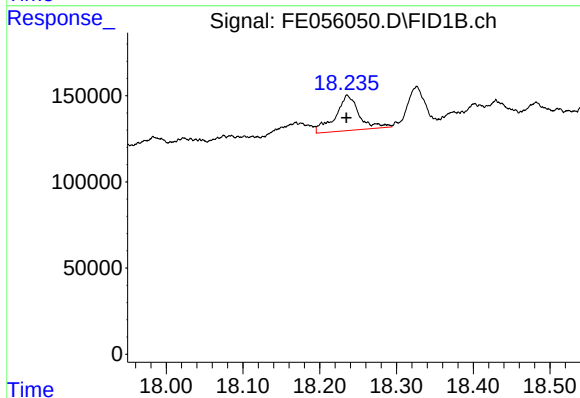


#17 n-Tricontane (C30)

R.T.: 18.236 min  
Delta R.T.: 0.002 min  
Response: 436971  
Conc: 2.95 ug/ml

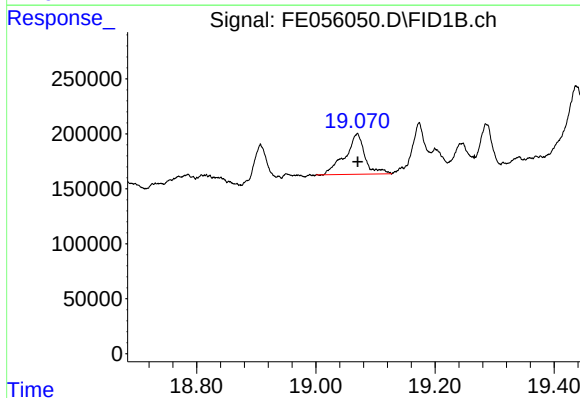


#18 n-Dotriacontane (C32)

R.T.: 19.069 min  
Delta R.T.: -0.001 min  
Response: 853882  
Conc: 5.72 ug/ml

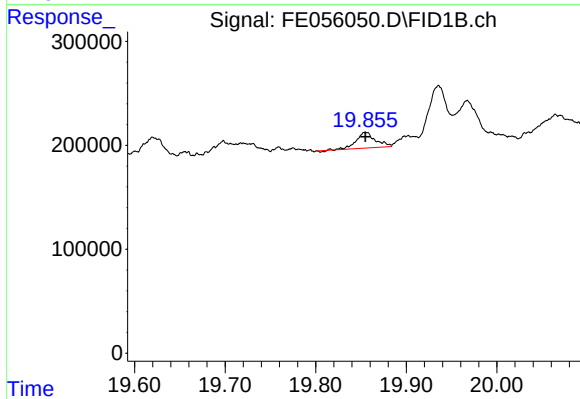

#19 n-Tetratriacontane (C34)


R.T.: 19.855 min  
Delta R.T.: 0.000 min  
Response: 222197  
Conc: 1.57 ug/ml

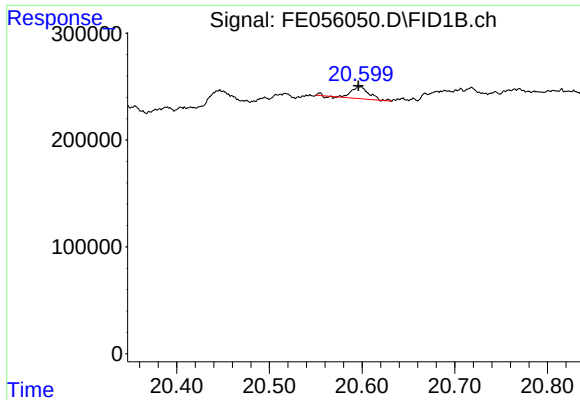

#20 n-Hexatriacontane (C36)

R.T.: 20.597 min  
Delta R.T.: 0.001 min  
Response: 149505  
Conc: 1.16 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

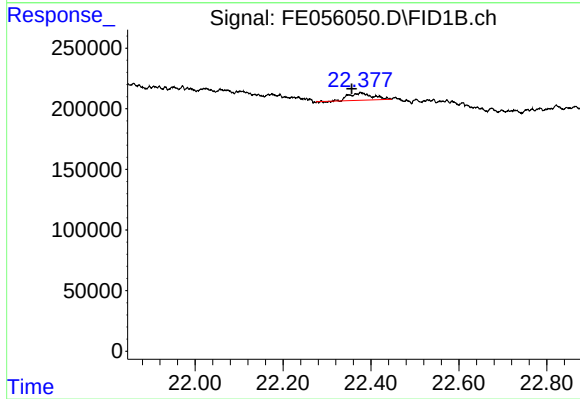

#22 n-Tetracontane (C40)

R.T.: 22.377 min  
Delta R.T.: 0.021 min  
Response: 219415  
Conc: 1.84 ug/ml