

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE093020\
 Data File : FE032823.D
 Signal(s) : FID1B.CH
 Acq On : 30 Sep 2020 9:32
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 01 01:15:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
 Quant Title :
 QLast Update : Tue Sep 15 03:21:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.669	5969869	19.055 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.853	132529	0.377 ug/ml
13) N-TRIACONTANE	17.726	89284	0.259 ug/ml
14) N-DOTRIACONTANE	18.559	122949	0.369 ug/ml
15) N-TETRATRIACONTANE	19.343	88805	0.279 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE093020\
Data File : FE032823.D
Signal(s) : FID1B.CH
Acq On : 30 Sep 2020 9:32
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 01 01:15:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

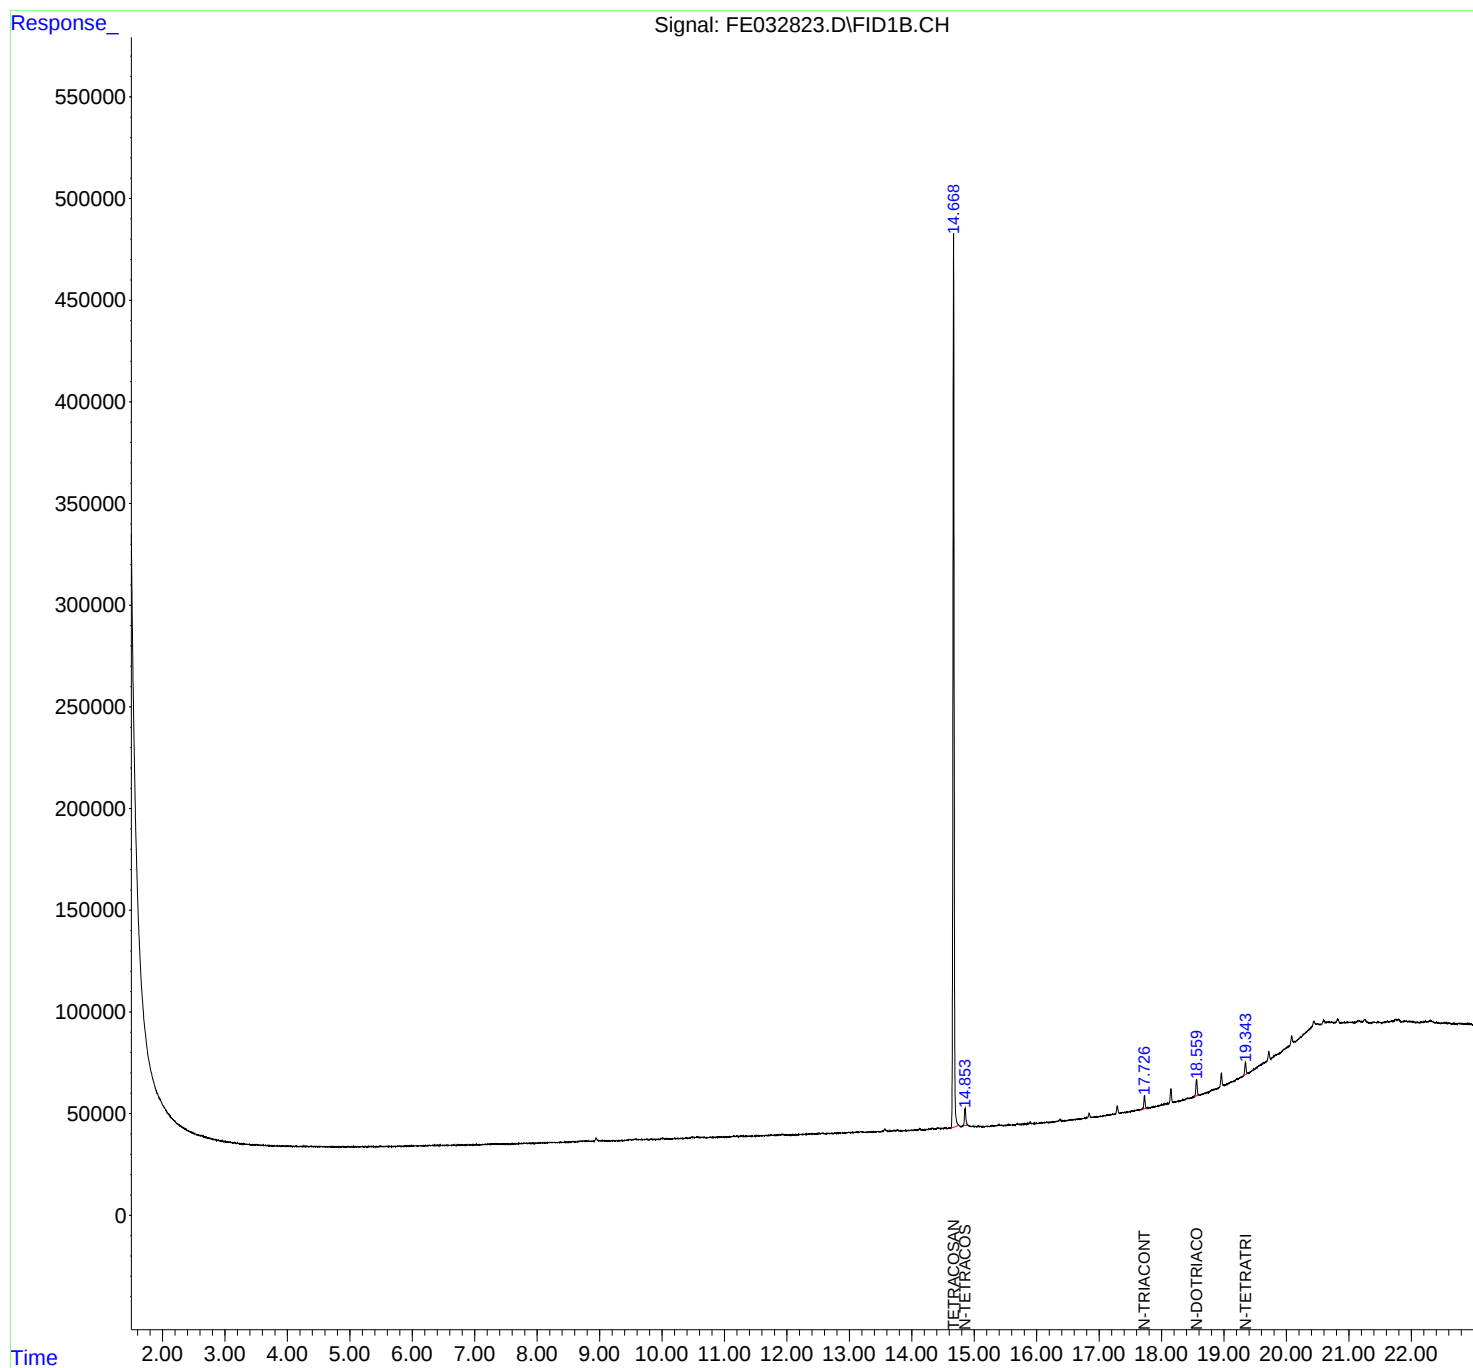


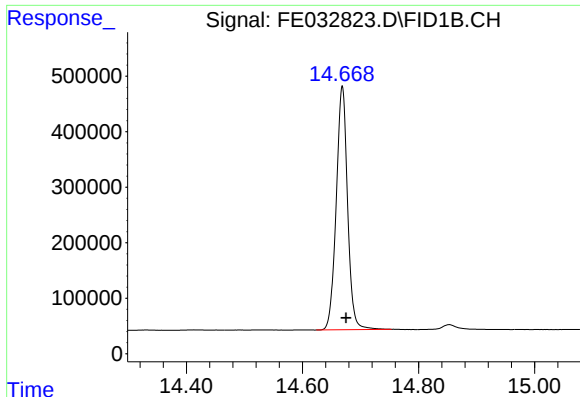

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.669 min
Delta R.T.: -0.007 min
Response: 5969869
Conc: 19.05 ug/ml

Instrument :
FID_E
ClientSampleId :

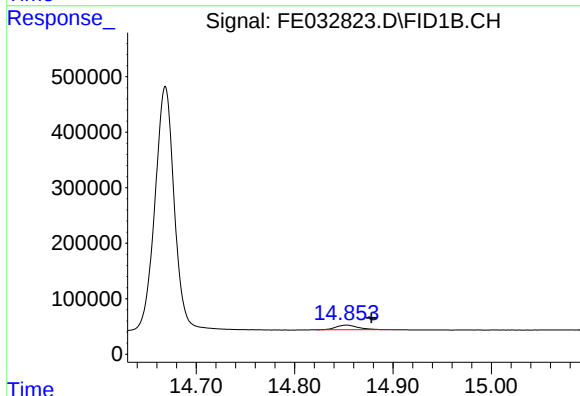


#10 N-TETRACOSANE

R.T.: 14.853 min
Delta R.T.: -0.025 min
Response: 132529
Conc: 0.38 ug/ml

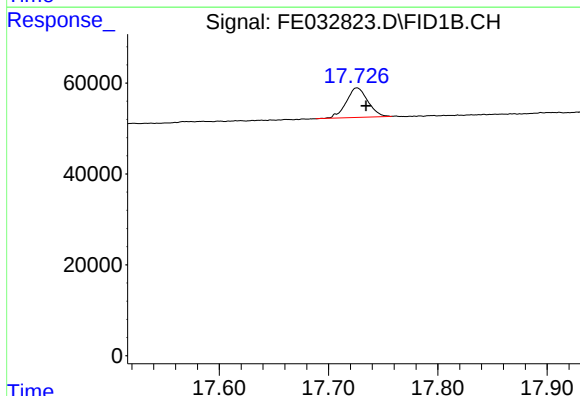


#13 N-TRIACONTANE

R.T.: 17.726 min
Delta R.T.: -0.008 min
Response: 89284
Conc: 0.26 ug/ml

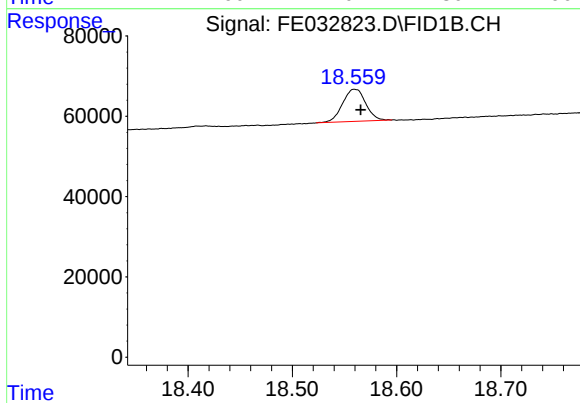

#14 N-DOTRIACONTANE

R.T.: 18.559 min
Delta R.T.: -0.006 min
Response: 122949
Conc: 0.37 ug/ml

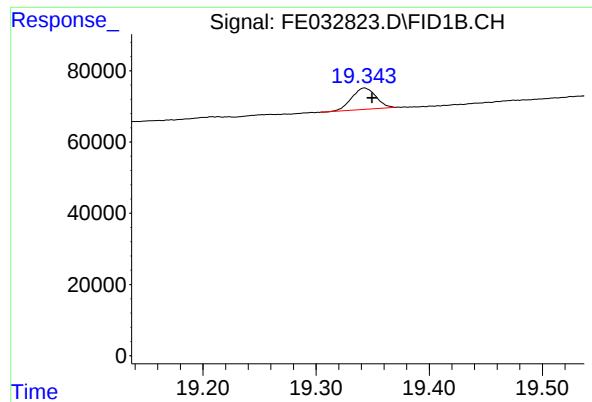

#15 N-TETRATRIACONTANE

R.T.: 19.343 min

Delta R.T.: -0.007 min

Response: 88805

Conc: 0.28 ug/ml

Instrument :
FID_E
ClientSampleId :