

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE093020\
 Data File : FE032826.D
 Signal(s) : FID1B.CH
 Acq On : 30 Sep 2020 11:57
 Operator : DD\AJ
 Sample : PB131990BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 01 01:16:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
 Quant Title :
 QLast Update : Tue Sep 15 03:21:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.666	6041896	19.285 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.846	509375	1.449 ug/ml
13) N-TRIACONTANE	17.724	113360	0.329 ug/ml
14) N-DOTRIACONTANE	18.557	153879	0.462 ug/ml
15) N-TETRATRIACONTANE	19.341	105492	0.332 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE093020\
Data File : FE032826.D
Signal(s) : FID1B.CH
Acq On : 30 Sep 2020 11:57
Operator : DD\AJ
Sample : PB131990BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 01 01:16:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

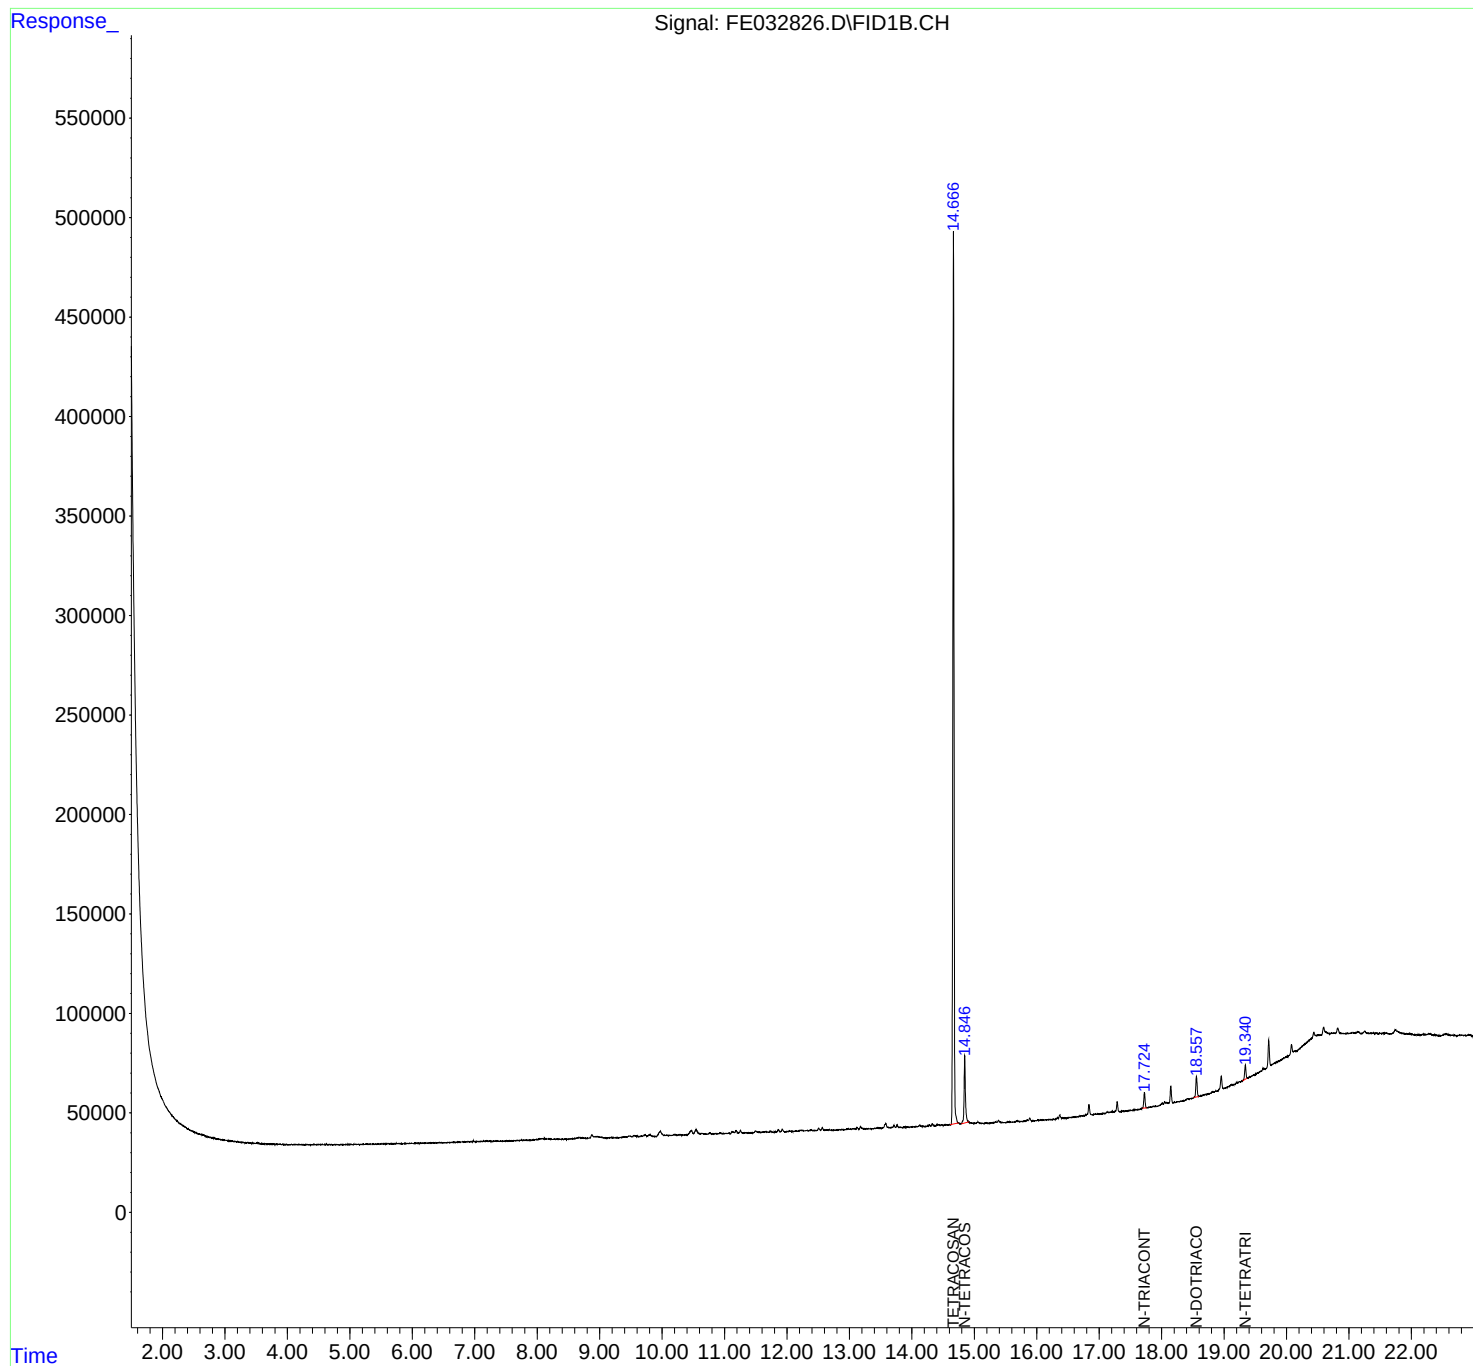


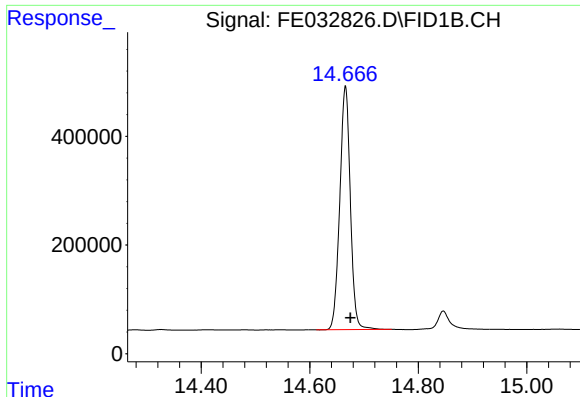

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.666 min
Delta R.T.: -0.009 min
Response: 6041896
Conc: 19.28 ug/ml

Instrument :
FID_E
ClientSampleId :

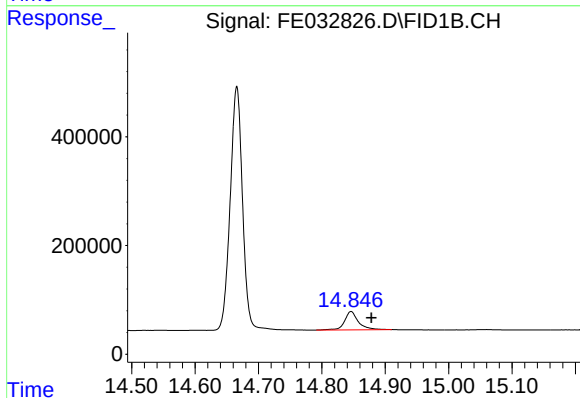


#10 N-TETRACOSANE

R.T.: 14.846 min
Delta R.T.: -0.032 min
Response: 509375
Conc: 1.45 ug/ml

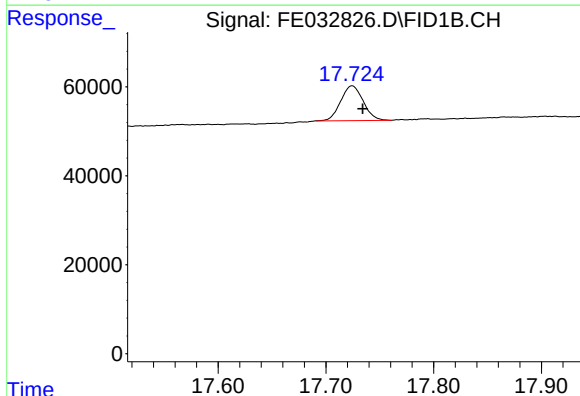


#13 N-TRIACONTANE

R.T.: 17.724 min
Delta R.T.: -0.010 min
Response: 113360
Conc: 0.33 ug/ml

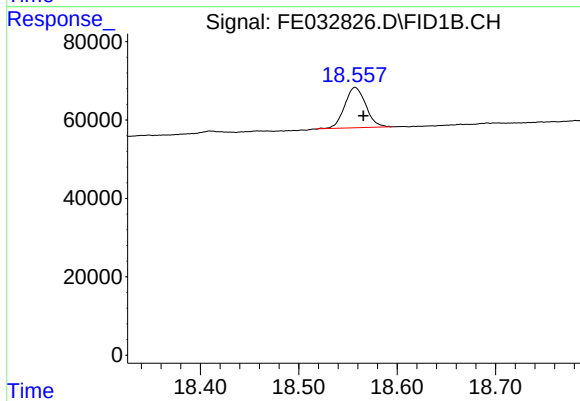

#14 N-DOTRIACONTANE

R.T.: 18.557 min
Delta R.T.: -0.009 min
Response: 153879
Conc: 0.46 ug/ml

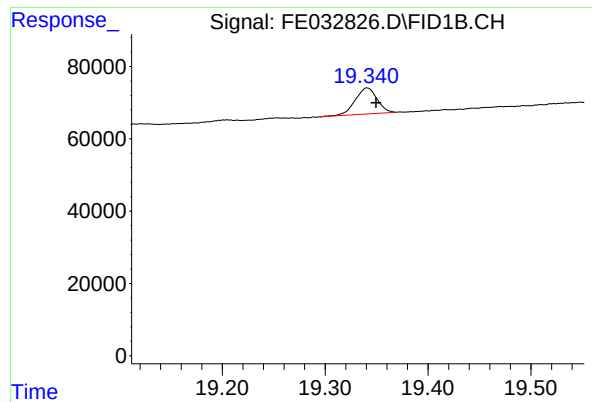

#15 N-TETRATRIACONTANE

R.T.: 19.341 min

Delta R.T.: -0.009 min

Response: 105492

Conc: 0.33 ug/ml

Instrument :
FID_E
ClientSampleId :