

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100119\
 Data File : FE030617.D
 Signal(s) : FID1B.CH
 Acq On : 01 Oct 2019 11:27
 Operator : DD\AJ
 Sample : K5064-01 50X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 02 00:37:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
 Quant Title :
 QLast Update : Wed Sep 25 02:50:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
7) N-EICOSANE	12.574	1209175	3.314 ug/ml
8) N-DOCOSANE	13.795	3933261	10.959 ug/ml
10) N-TETRACOSANE	14.935	1976356	5.559 ug/ml
13) N-TRIACONTANE	17.738	315799	0.942 ug/ml
14) N-DOTRIACONTANE	18.569	613838	1.902 ug/ml
16) N-HEXATRIACONTANE	20.090	661679	2.331 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100119\
Data File : FE030617.D
Signal(s) : FID1B.CH
Acq On : 01 Oct 2019 11:27
Operator : DD\AJ
Sample : K5064-01 50X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 02 00:37:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
Quant Title :
QLast Update : Wed Sep 25 02:50:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

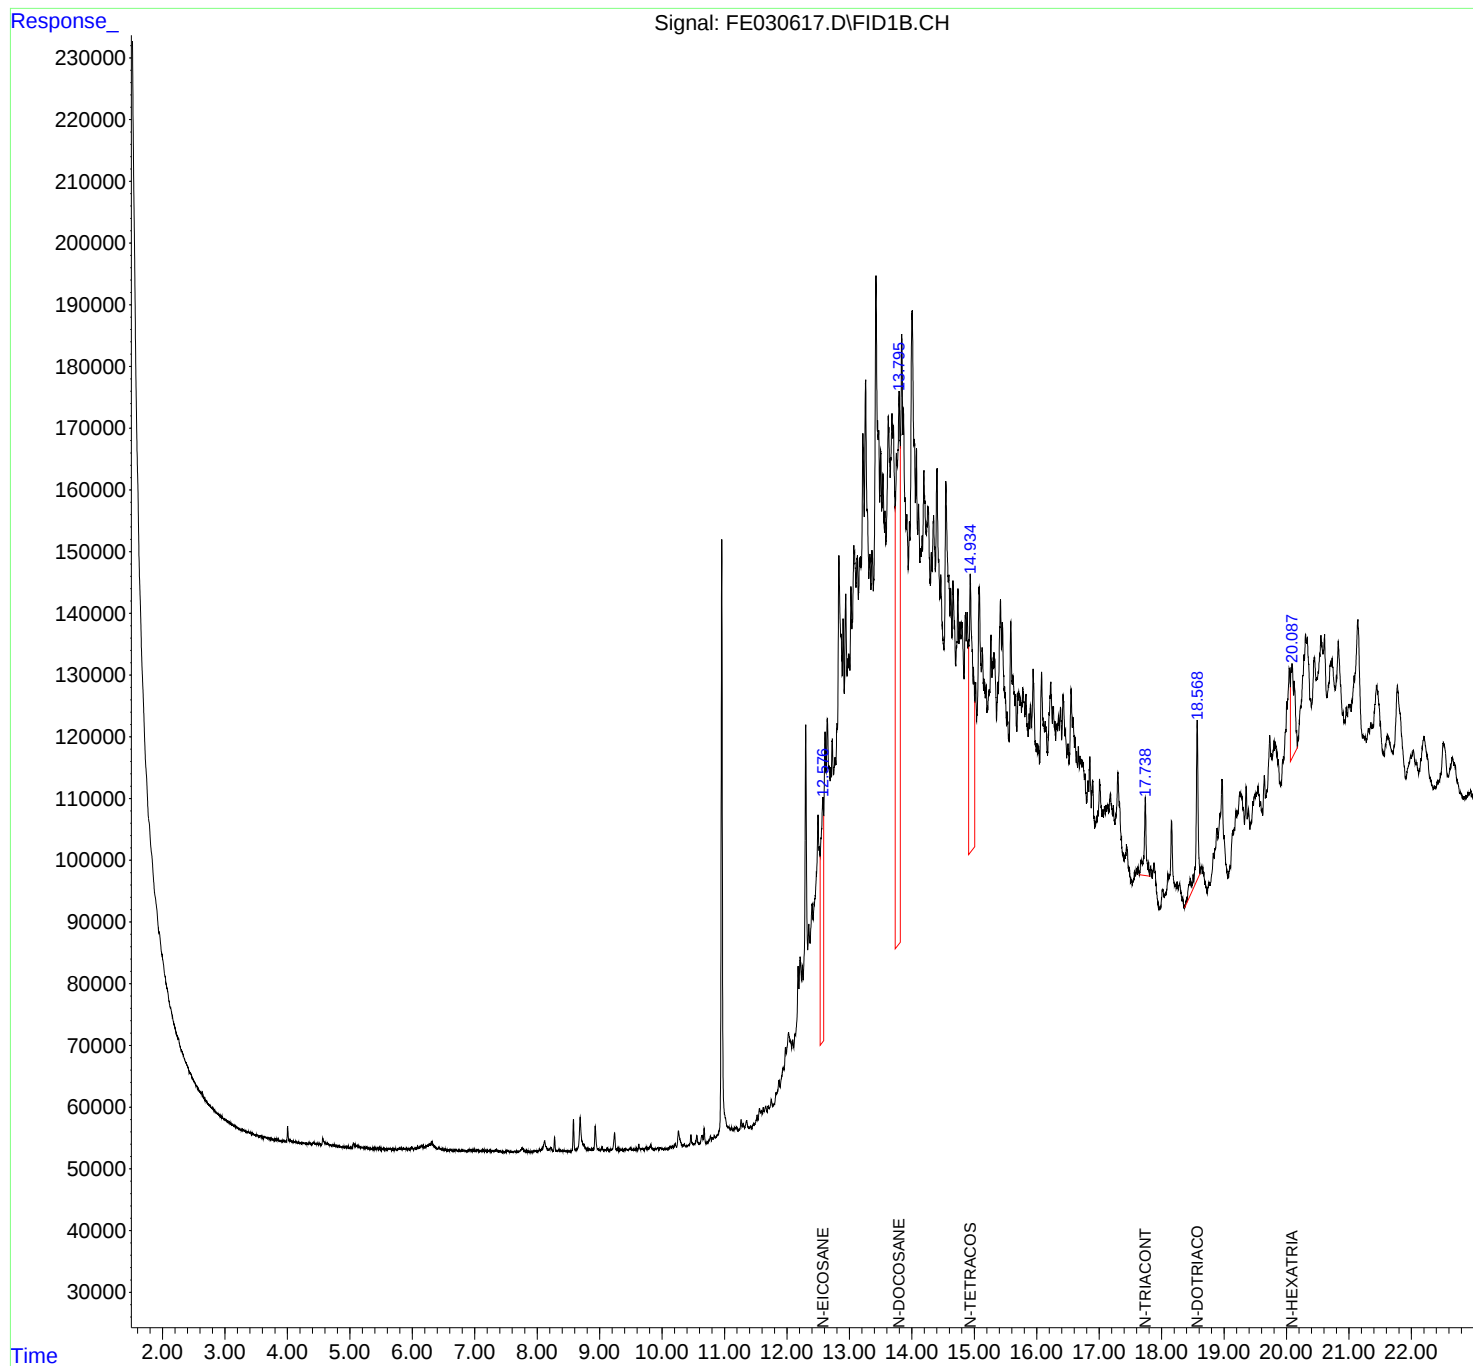


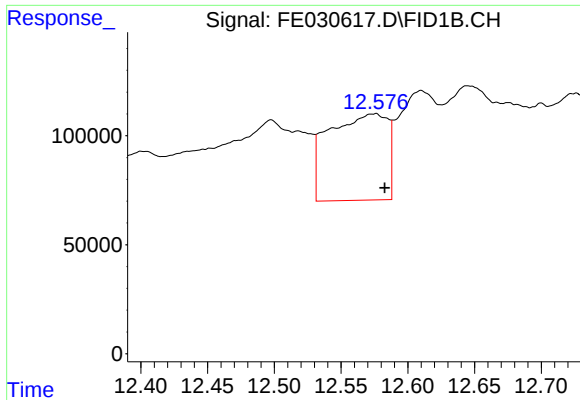

#7 N-EICOSANE


R.T.: 12.574 min
Delta R.T.: -0.008 min
Response: 1209175
Conc: 3.31 ug/ml

Instrument :
FID_E
ClientSampleId :

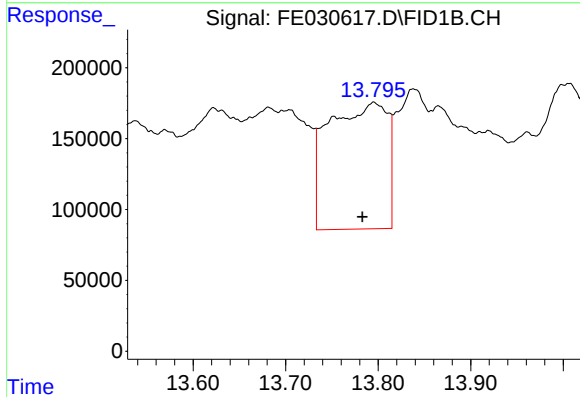


#8 N-DOCOSANE

R.T.: 13.795 min
Delta R.T.: 0.012 min
Response: 3933261
Conc: 10.96 ug/ml

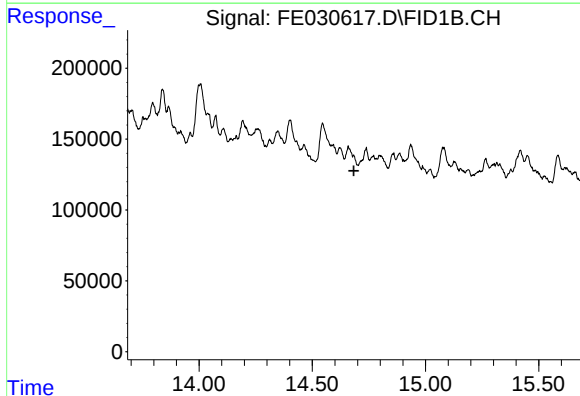


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.684 min
Response: 0
Conc: N.D.

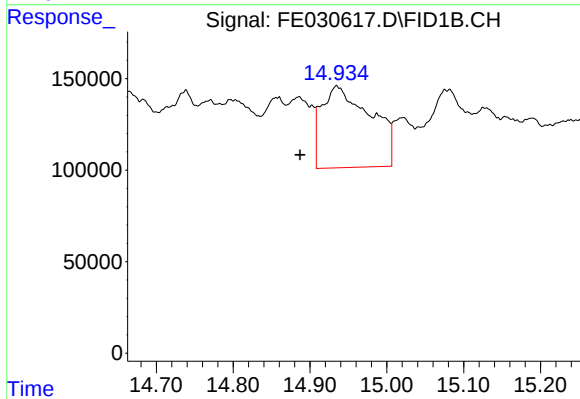

#10 N-TETRACOSANE


R.T.: 14.935 min
Delta R.T.: 0.048 min
Response: 1976356
Conc: 5.56 ug/ml

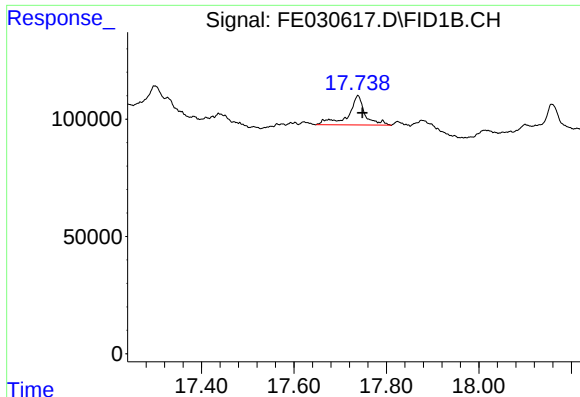

#13 N-TRIACONTANE


R.T.: 17.738 min
Delta R.T.: -0.010 min
Response: 315799
Conc: 0.94 ug/ml

Instrument :
FID_E
ClientSampleId :

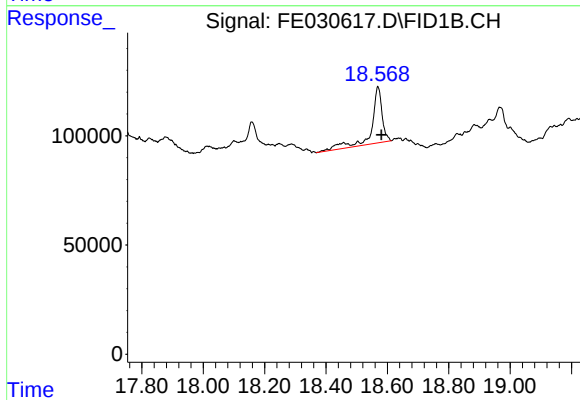

#14 N-DOTRIACONTANE

R.T.: 18.569 min
Delta R.T.: -0.011 min
Response: 613838
Conc: 1.90 ug/ml

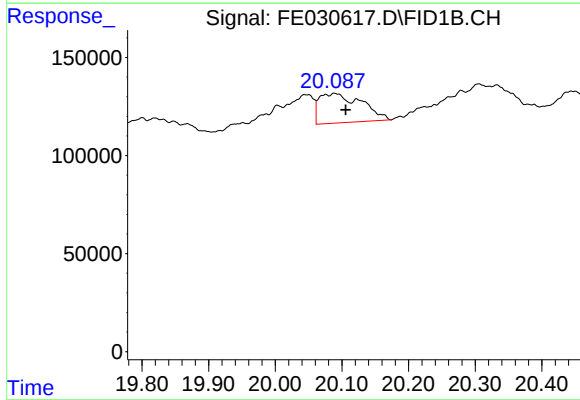

#16 N-HEXATRIACONTANE

R.T.: 20.090 min
Delta R.T.: -0.016 min
Response: 661679
Conc: 2.33 ug/ml