

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100119\
 Data File : FE030620.D
 Signal(s) : FID1B.CH
 Acq On : 01 Oct 2019 13:25
 Operator : DD\AJ
 Sample : K4946-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 02 00:38:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
 Quant Title :
 QLast Update : Wed Sep 25 02:50:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.677	5975400	19.274 ug/ml
Target Compounds			
4) N-TETRADECANE	8.278f	1635329	4.349 ug/ml
7) N-EICOSANE	12.637f	433345	1.188 ug/ml
11) N-HEXACOSANE	15.898	273931	0.782 ug/ml
12) N-OCTACOSANE	16.849	316366	0.919 ug/ml
13) N-TRIACONTANE	17.735	286540	0.855 ug/ml
14) N-DOTRIACONTANE	18.568	325266	1.008 ug/ml
15) N-TETRATRIACONTANE	19.355	257902	0.826 ug/ml
16) N-HEXATRIACONTANE	20.101	419451	1.478 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100119\
Data File : FE030620.D
Signal(s) : FID1B.CH
Acq On : 01 Oct 2019 13:25
Operator : DD\AJ
Sample : K4946-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 02 00:38:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
Quant Title :
QLast Update : Wed Sep 25 02:50:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

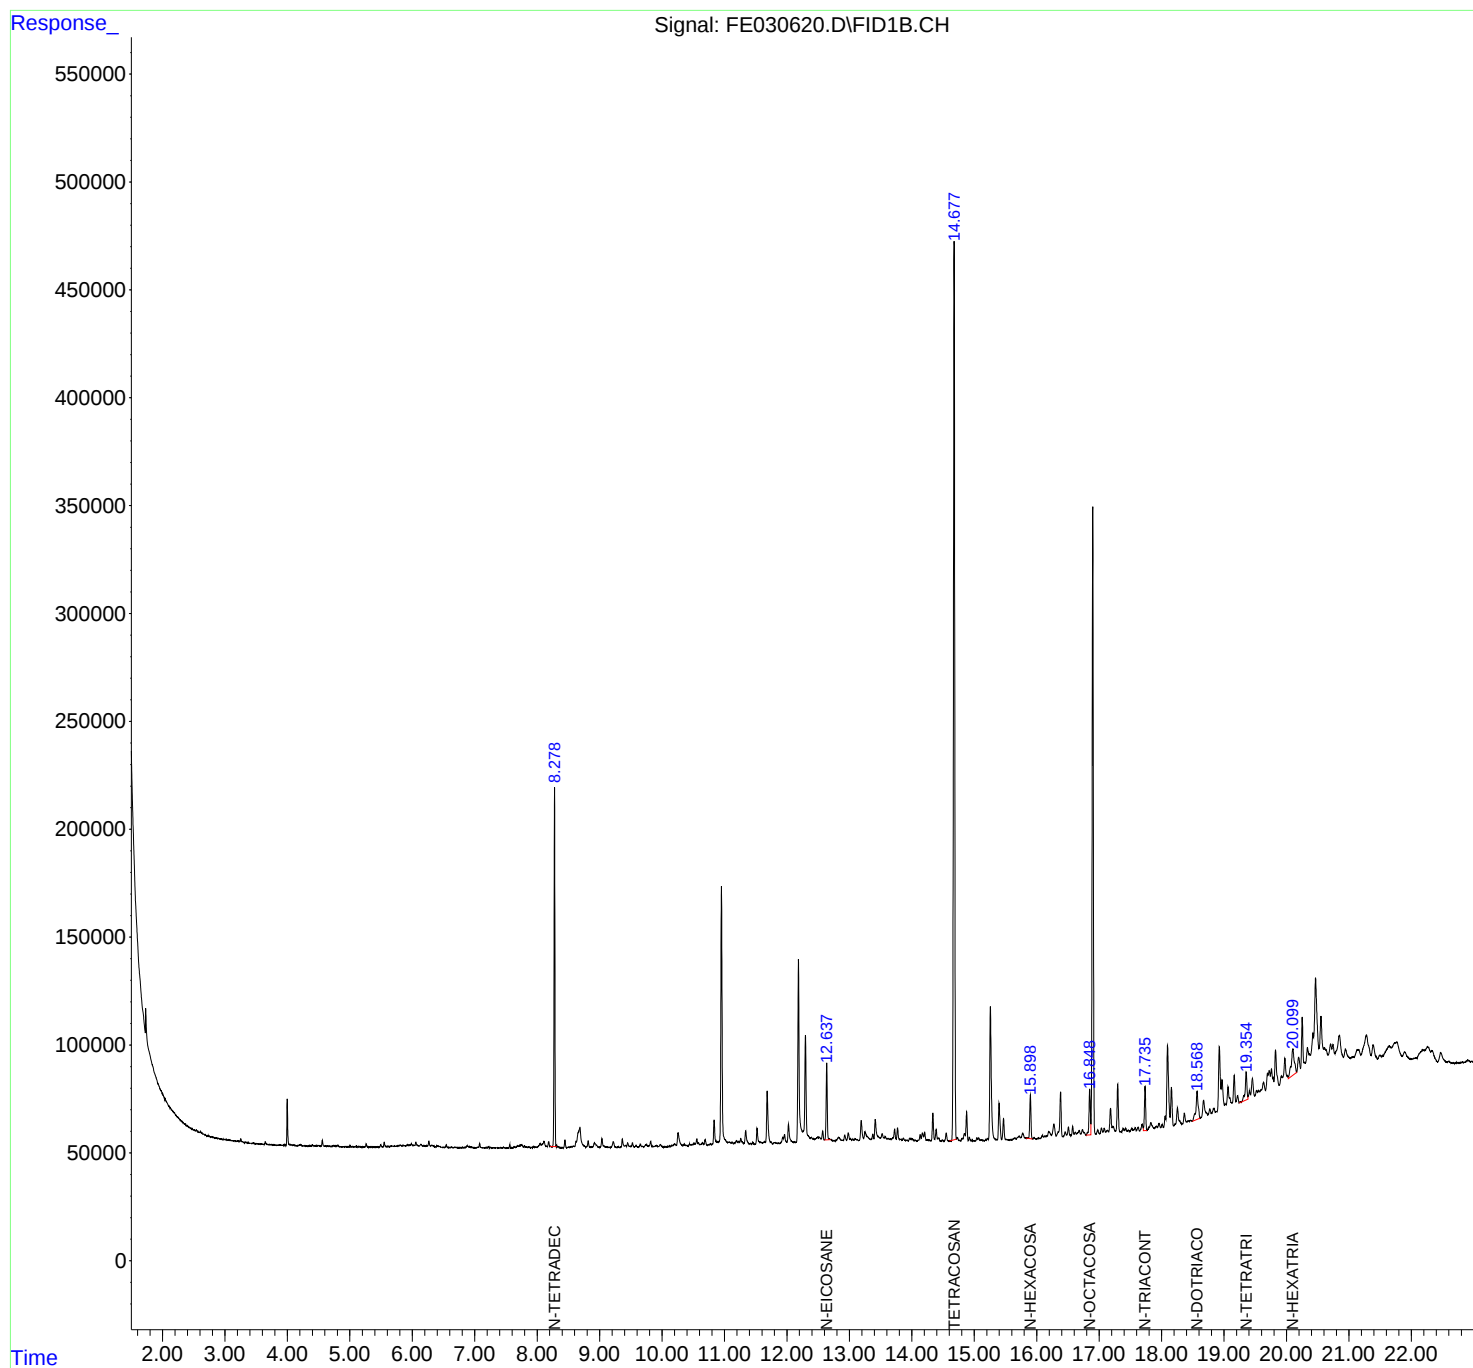


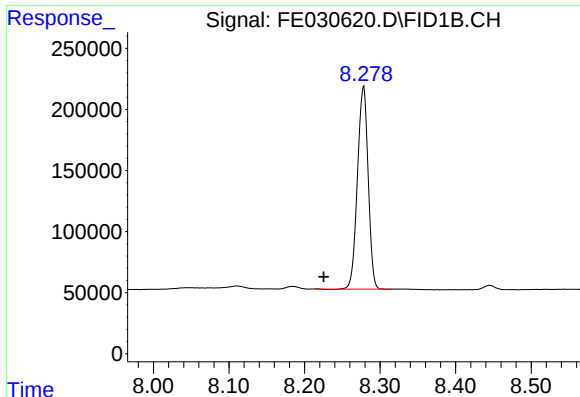

#4 N-TETRADECANE


R.T.: 8.278 min
Delta R.T.: 0.052 min
Response: 1635329
Conc: 4.35 ug/ml

Instrument :
FID_E
ClientSampleId :

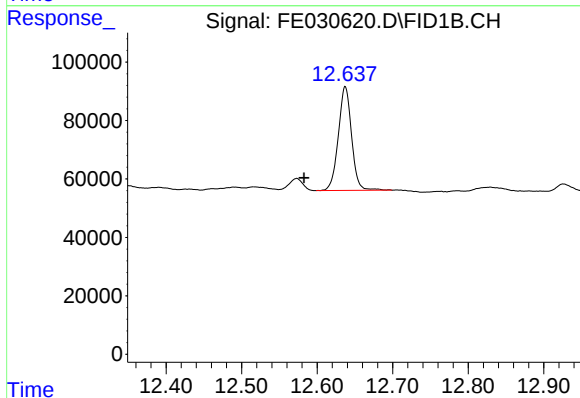


#7 N-EICOSANE

R.T.: 12.637 min
Delta R.T.: 0.055 min
Response: 433345
Conc: 1.19 ug/ml

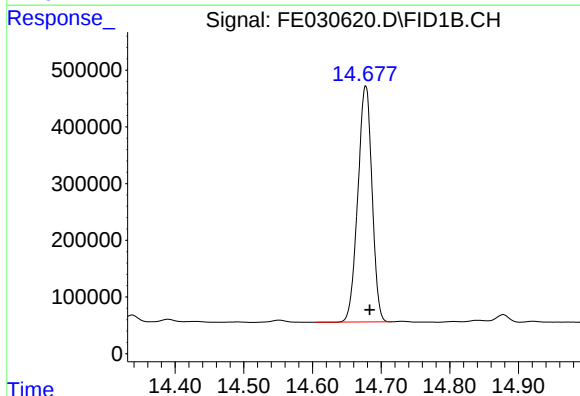


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.677 min
Delta R.T.: -0.006 min
Response: 5975400
Conc: 19.27 ug/ml

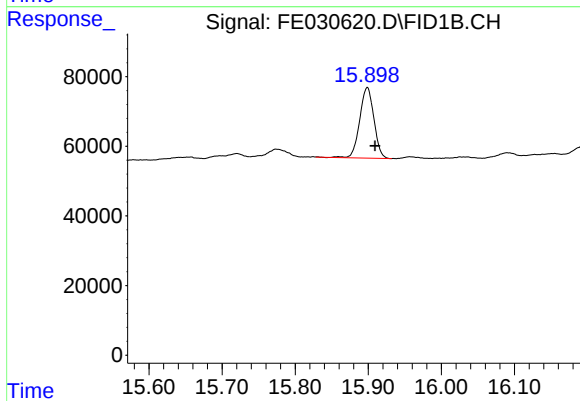

#11 N-HEXACOSANE


R.T.: 15.898 min
Delta R.T.: -0.011 min
Response: 273931
Conc: 0.78 ug/ml

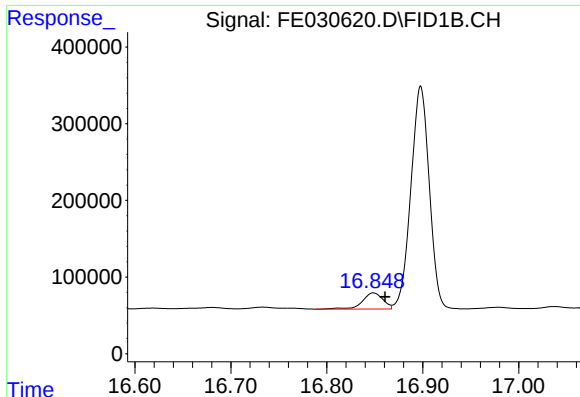

#12 N-OCTACOSANE


R.T.: 16.849 min
Delta R.T.: -0.012 min
Response: 316366
Conc: 0.92 ug/ml

Instrument :
FID_E
ClientSampleId :

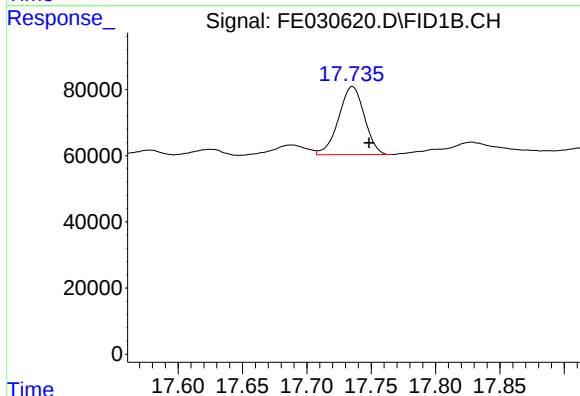


#13 N-TRIACONTANE

R.T.: 17.735 min
Delta R.T.: -0.013 min
Response: 286540
Conc: 0.85 ug/ml

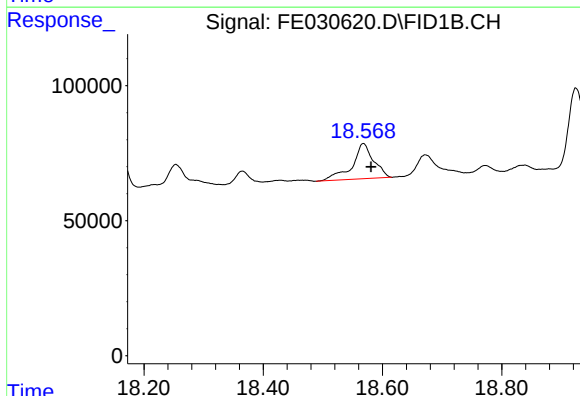


#14 N-DOTRIACONTANE

R.T.: 18.568 min
Delta R.T.: -0.013 min
Response: 325266
Conc: 1.01 ug/ml

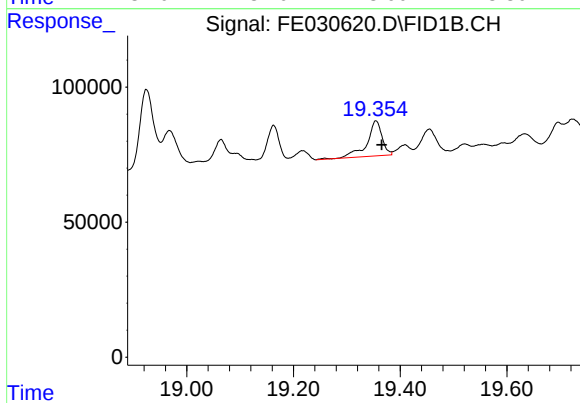

#15 N-TETRATRIACONTANE

R.T.: 19.355 min
Delta R.T.: -0.011 min
Response: 257902
Conc: 0.83 ug/ml

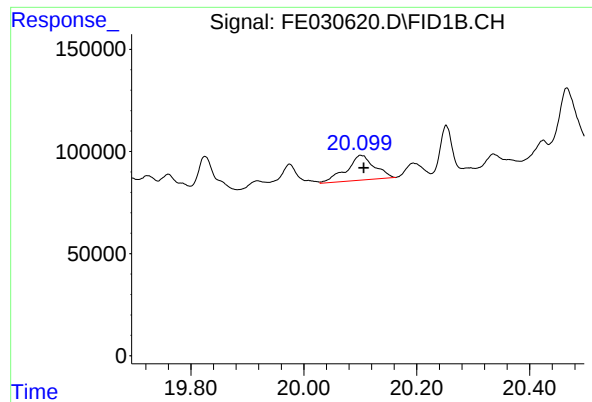

#16 N-HEXATRIACONTANE

R.T.: 20.101 min
Delta R.T.: -0.005 min
Response: 419451
Conc: 1.48 ug/ml

Instrument :
FID_E
ClientSampleId :