

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100119\
 Data File : FE030625.D
 Signal(s) : FID1B.CH
 Acq On : 01 Oct 2019 16:13
 Operator : DD\AJ
 Sample : K5094-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 02 00:39:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
 Quant Title :
 QLast Update : Wed Sep 25 02:50:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.680	4005814	12.921 ug/ml
Target Compounds			
4) N-TETRADECANE	8.282f	1423092	3.785 ug/ml
7) N-EICOSANE	12.641f	289070	0.792 ug/ml
11) N-HEXACOSANE	15.905	337409	0.963 ug/ml
12) N-OCTACOSANE	16.856	454278	1.320 ug/ml
13) N-TRIACONTANE	17.745	607346	1.812 ug/ml
14) N-DOTRIACONTANE	18.572	660496	2.047 ug/ml
15) N-TETRATRIACONTANE	19.366	248636	0.796 ug/ml
16) N-HEXATRIACONTANE	20.126	158710	0.559 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100119\
Data File : FE030625.D
Signal(s) : FID1B.CH
Acq On : 01 Oct 2019 16:13
Operator : DD\AJ
Sample : K5094-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 02 00:39:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
Quant Title :
QLast Update : Wed Sep 25 02:50:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

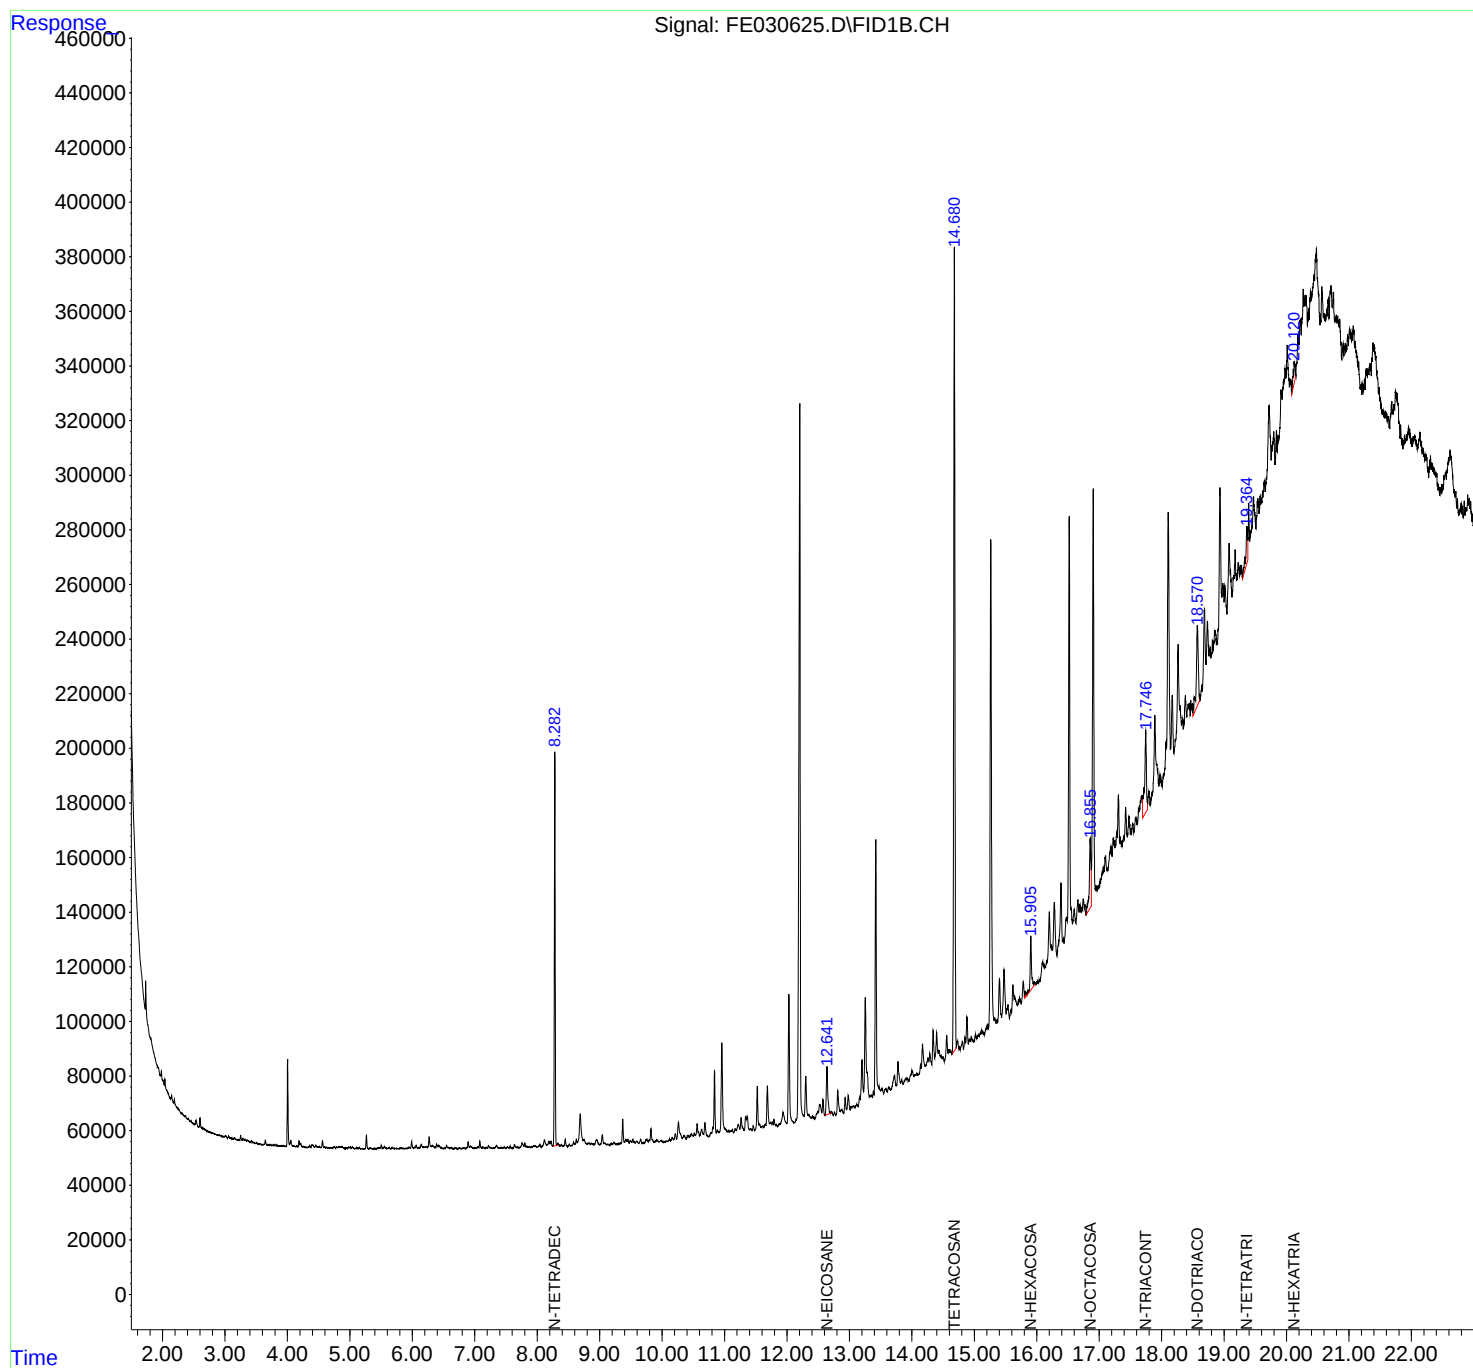


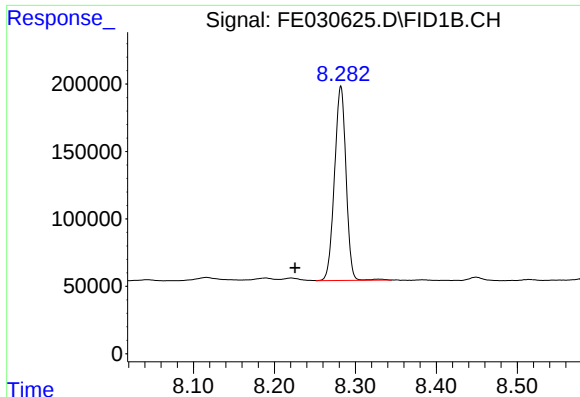

#4 N-TETRADECANE


R.T.: 8.282 min
Delta R.T.: 0.056 min
Response: 1423092
Conc: 3.78 ug/ml

Instrument :
FID_E
ClientSampleId :

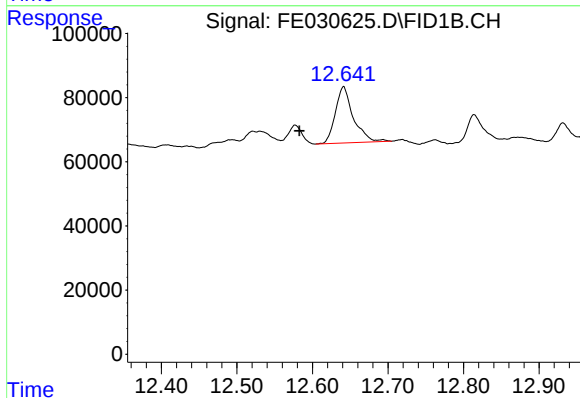


#7 N-EICOSANE

R.T.: 12.641 min
Delta R.T.: 0.058 min
Response: 289070
Conc: 0.79 ug/ml

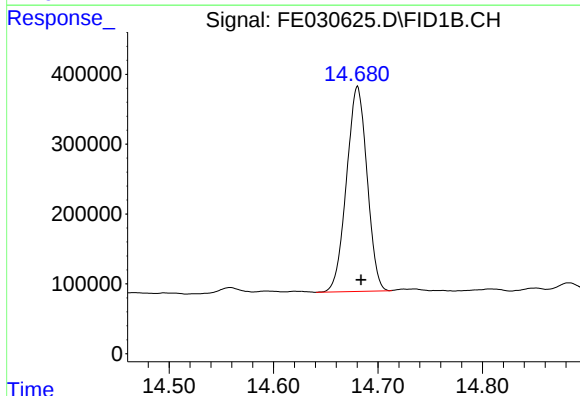


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.680 min
Delta R.T.: -0.003 min
Response: 4005814
Conc: 12.92 ug/ml

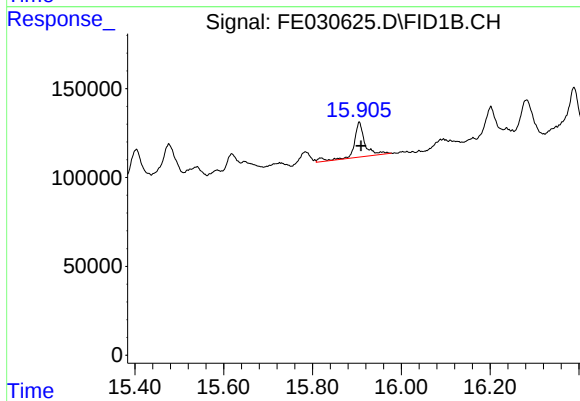

#11 N-HEXACOSANE


R.T.: 15.905 min
Delta R.T.: -0.004 min
Response: 337409
Conc: 0.96 ug/ml

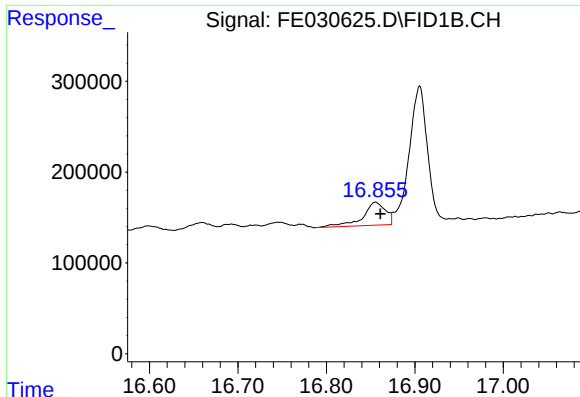

#12 N-OCTACOSANE


R.T.: 16.856 min
Delta R.T.: -0.005 min
Response: 454278
Conc: 1.32 ug/ml

Instrument :
FID_E
ClientSampleId :

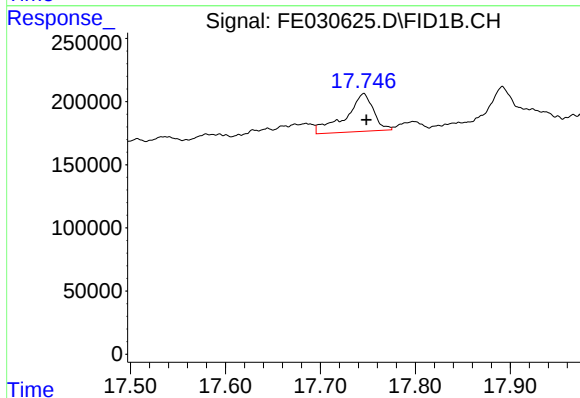


#13 N-TRIACONTANE

R.T.: 17.745 min
Delta R.T.: -0.003 min
Response: 607346
Conc: 1.81 ug/ml

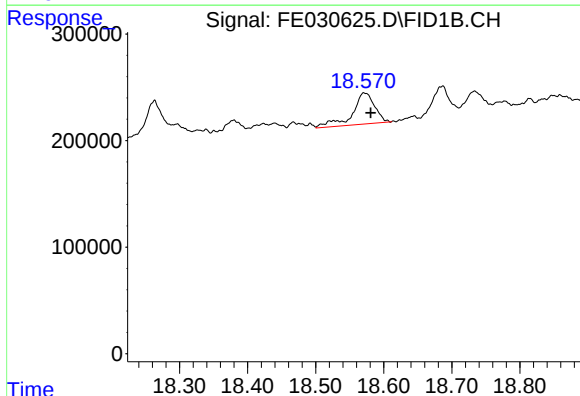


#14 N-DOTRIACONTANE

R.T.: 18.572 min
Delta R.T.: -0.009 min
Response: 660496
Conc: 2.05 ug/ml

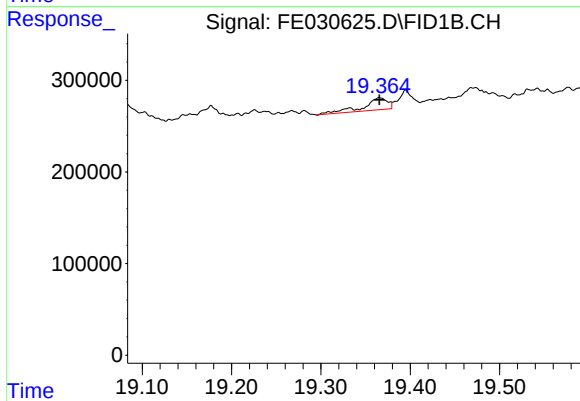

#15 N-TETRATRIACONTANE

R.T.: 19.366 min
Delta R.T.: 0.000 min
Response: 248636
Conc: 0.80 ug/ml

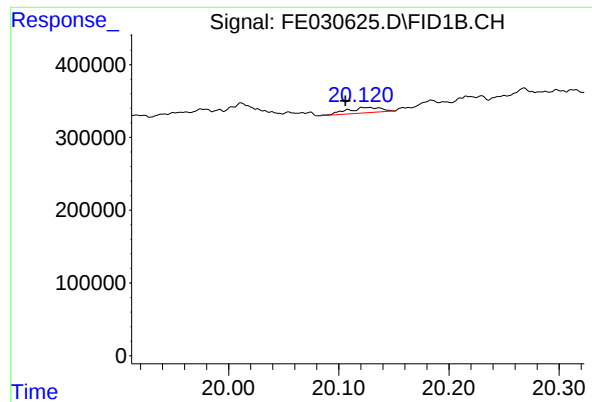

#16 N-HEXATRIACONTANE

R.T.: 20.126 min
Delta R.T.: 0.020 min
Response: 158710
Conc: 0.56 ug/ml

Instrument :
FID_E
ClientSampleId :