

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100119\
Data File : FE030624.D
Signal(s) : FID1B.CH
Acq On : 01 Oct 2019 15:39
Operator : DD\AJ
Sample : K4663-10 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
OK-01-093019

Integration File: autoint1.e
Quant Time: Oct 02 00:39:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
Quant Title :
QLast Update : Wed Sep 25 02:50:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.678	1349846	4.354 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100119\
Data File : FE030624.D
Signal(s) : FID1B.CH
Acq On : 01 Oct 2019 15:39
Operator : DD\AJ
Sample : K4663-10 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
OK-01-093019

Integration File: autoint1.e
Quant Time: Oct 02 00:39:00 2019
Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
Quant Title :
QLast Update : Wed Sep 25 02:50:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

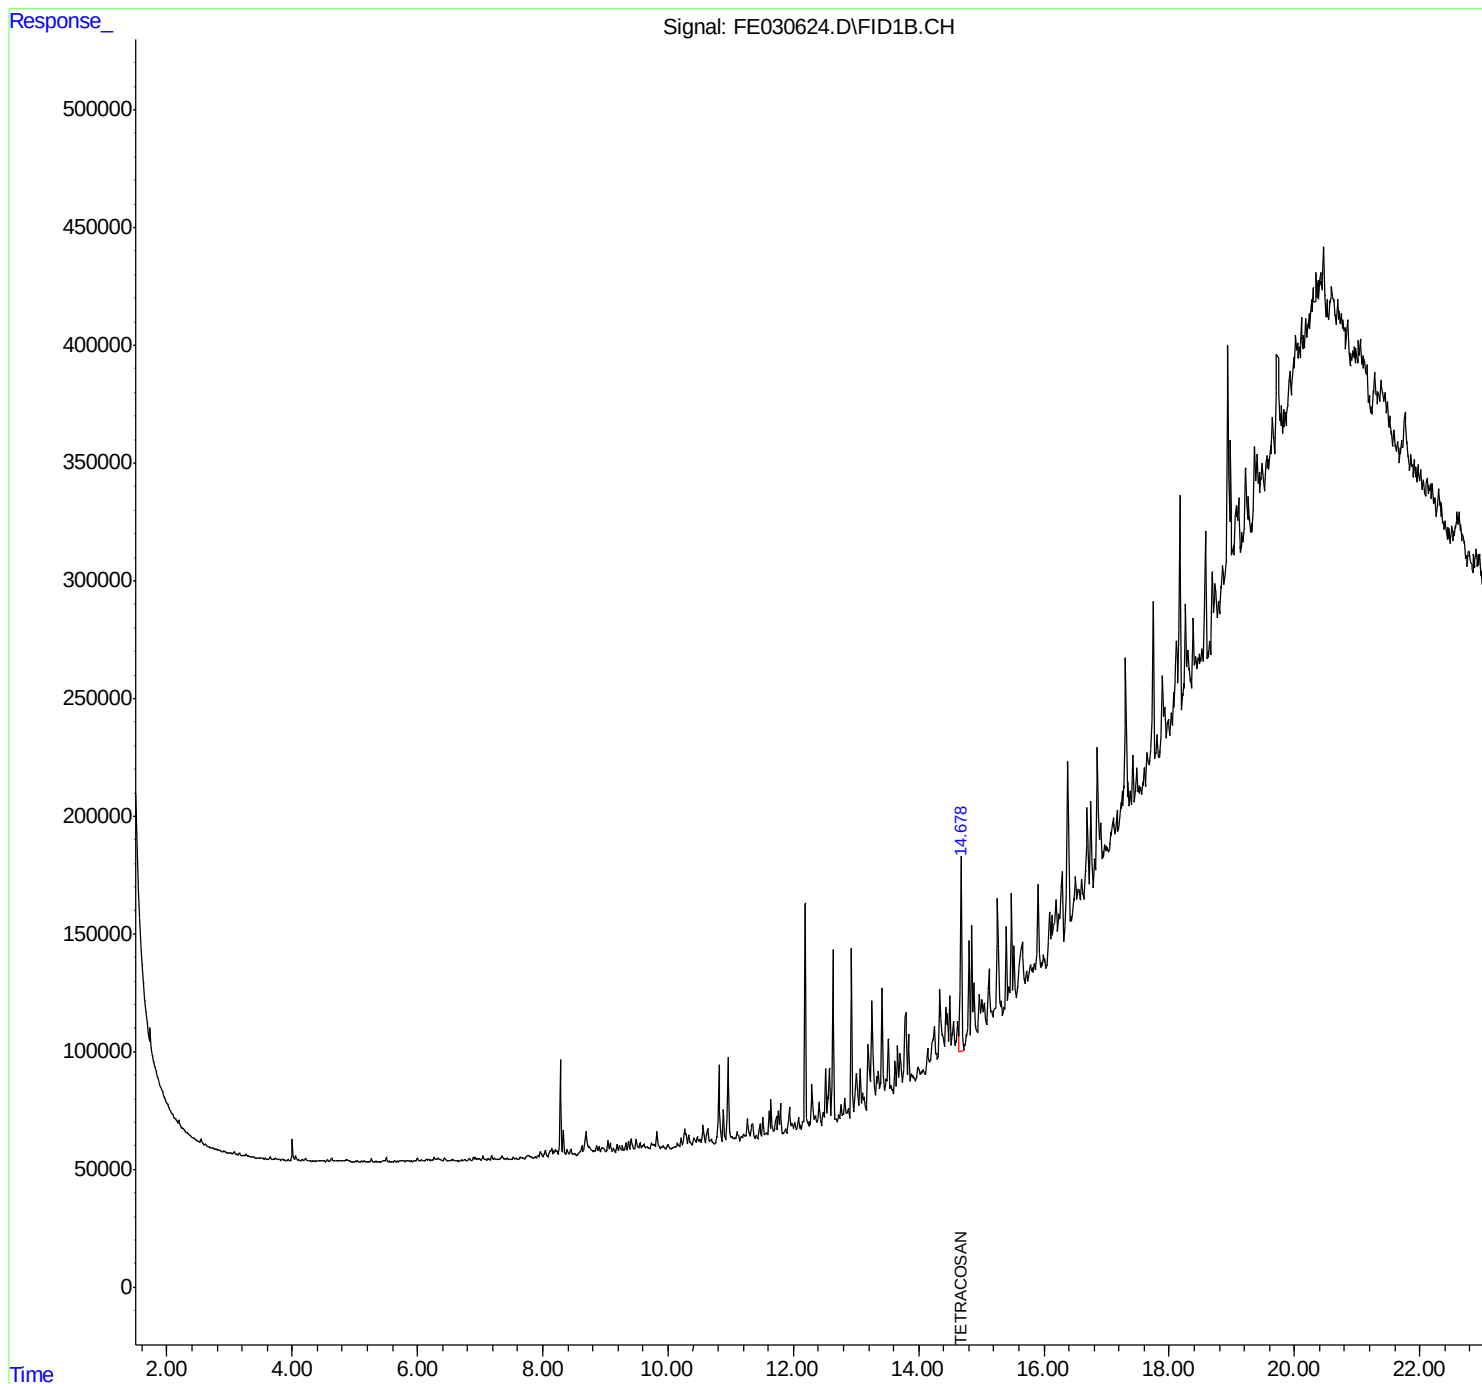

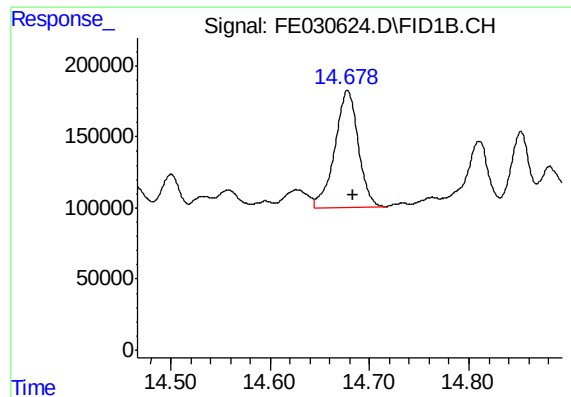

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.678 min
Delta R.T.: -0.006 min
Response: 1349846
Conc: 4.35 ug/ml

Instrument :
FID_E
ClientSampleId :
OK-01-093019