

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100120\
Data File : FE032840.D
Signal(s) : FID1B.CH
Acq On : 01 Oct 2020 9:33
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 02 01:18:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.864	218542	0.622 ug/ml
14)	N-DOTRIACONTANE	18.575	92178	0.277 ug/ml
15)	N-TETRATRIACONTANE	19.358	56906	0.179 ug/ml
16)	N-HEXATRIACONTANE	20.102	64242	0.218 ug/ml
18)	N-TETRACONTANE	21.797	206958	0.766 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100120\
Data File : FE032840.D
Signal(s) : FID1B.CH
Acq On : 01 Oct 2020 9:33
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 02 01:18:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

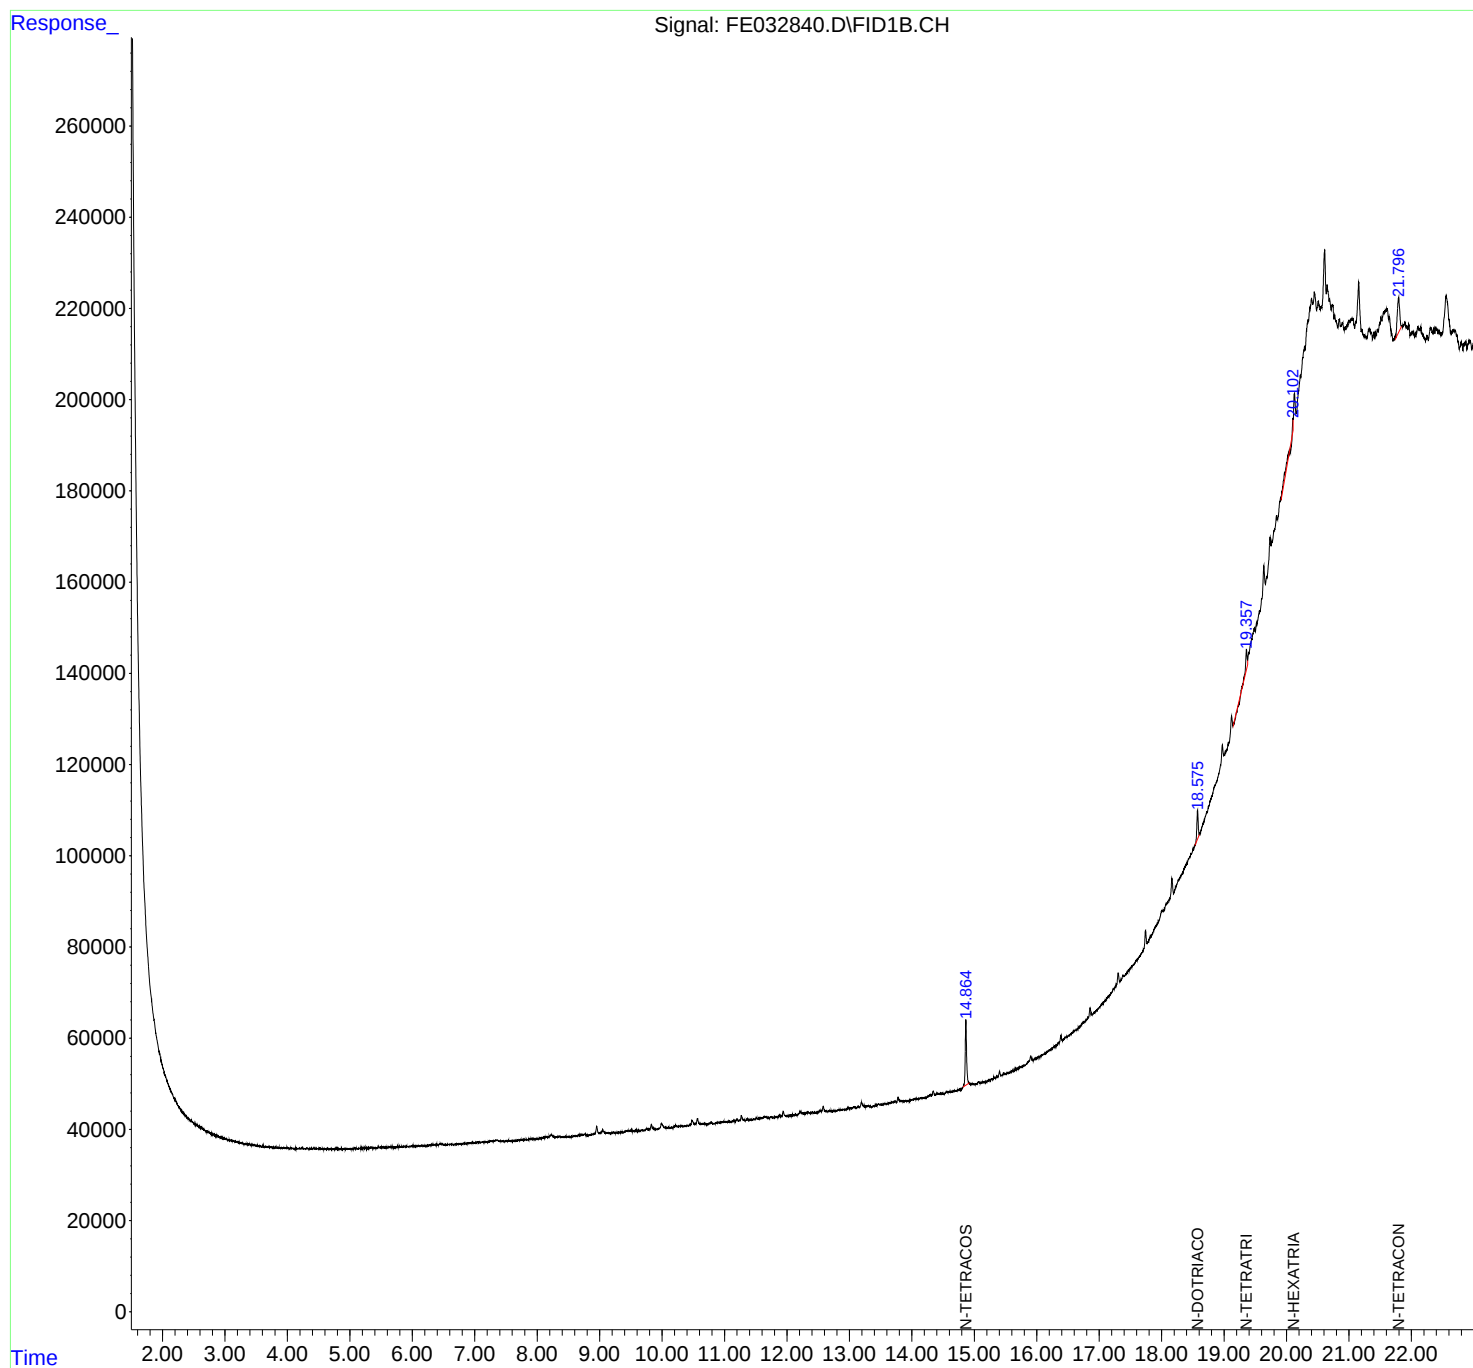


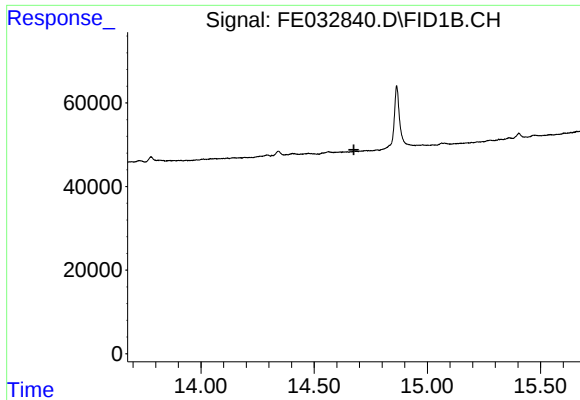

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.675 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

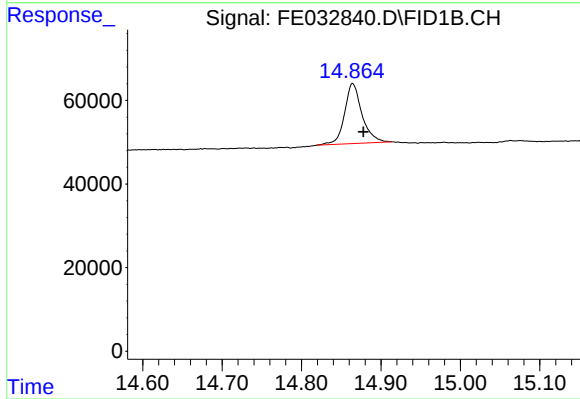


#10 N-TETRACOSANE

R.T.: 14.864 min
Delta R.T.: -0.014 min
Response: 218542
Conc: 0.62 ug/ml

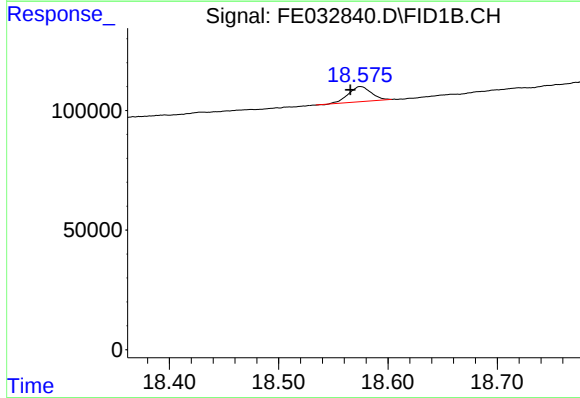


#14 N-DOTRIACONTANE

R.T.: 18.575 min
Delta R.T.: 0.009 min
Response: 92178
Conc: 0.28 ug/ml

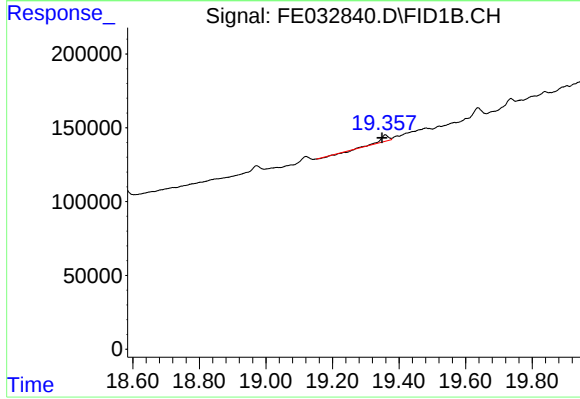

#15 N-TETRATRIACONTANE


R.T.: 19.358 min
Delta R.T.: 0.008 min
Response: 56906
Conc: 0.18 ug/ml

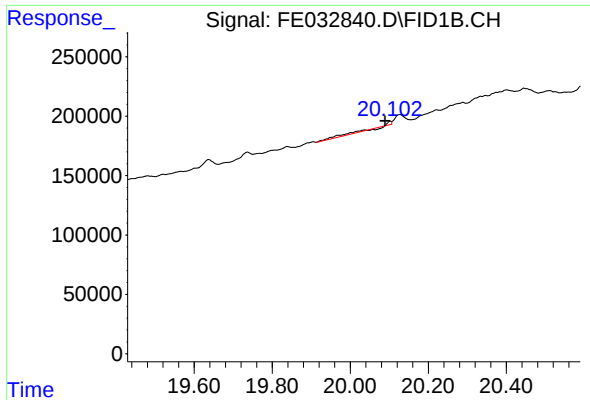

#16 N-HEXATRIACONTANE

R.T.: 20.102 min
Delta R.T.: 0.013 min
Response: 64242
Conc: 0.22 ug/ml

Instrument :
FID_E
ClientSampleId :

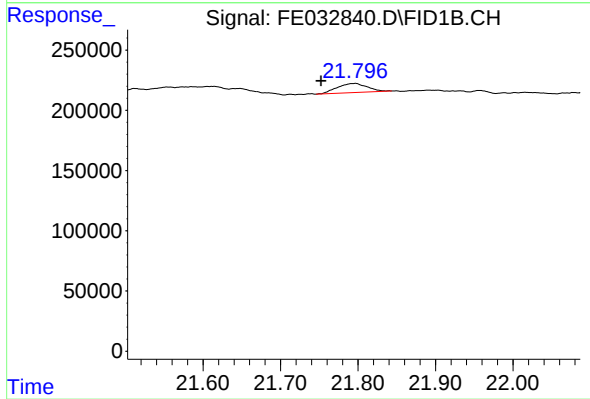

#18 N-TETRACONTANE

R.T.: 21.797 min
Delta R.T.: 0.045 min
Response: 206958
Conc: 0.77 ug/ml