

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100120\
 Data File : FE032863.D
 Signal(s) : FID1B.CH
 Acq On : 02 Oct 2020 00:23
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 02 01:23:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
 Quant Title :
 QLast Update : Tue Sep 15 03:21:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.673	5843483	18.651 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.856	228737	0.651 ug/ml
13) N-TRIACONTANE	17.733	107899	0.313 ug/ml
14) N-DOTRIACONTANE	18.563	156257	0.469 ug/ml
15) N-TETRATRIACONTANE	19.349	109285	0.344 ug/ml
16) N-HEXATRIACONTANE	20.091	145912	0.494 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100120\
Data File : FE032863.D
Signal(s) : FID1B.CH
Acq On : 02 Oct 2020 00:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 02 01:23:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

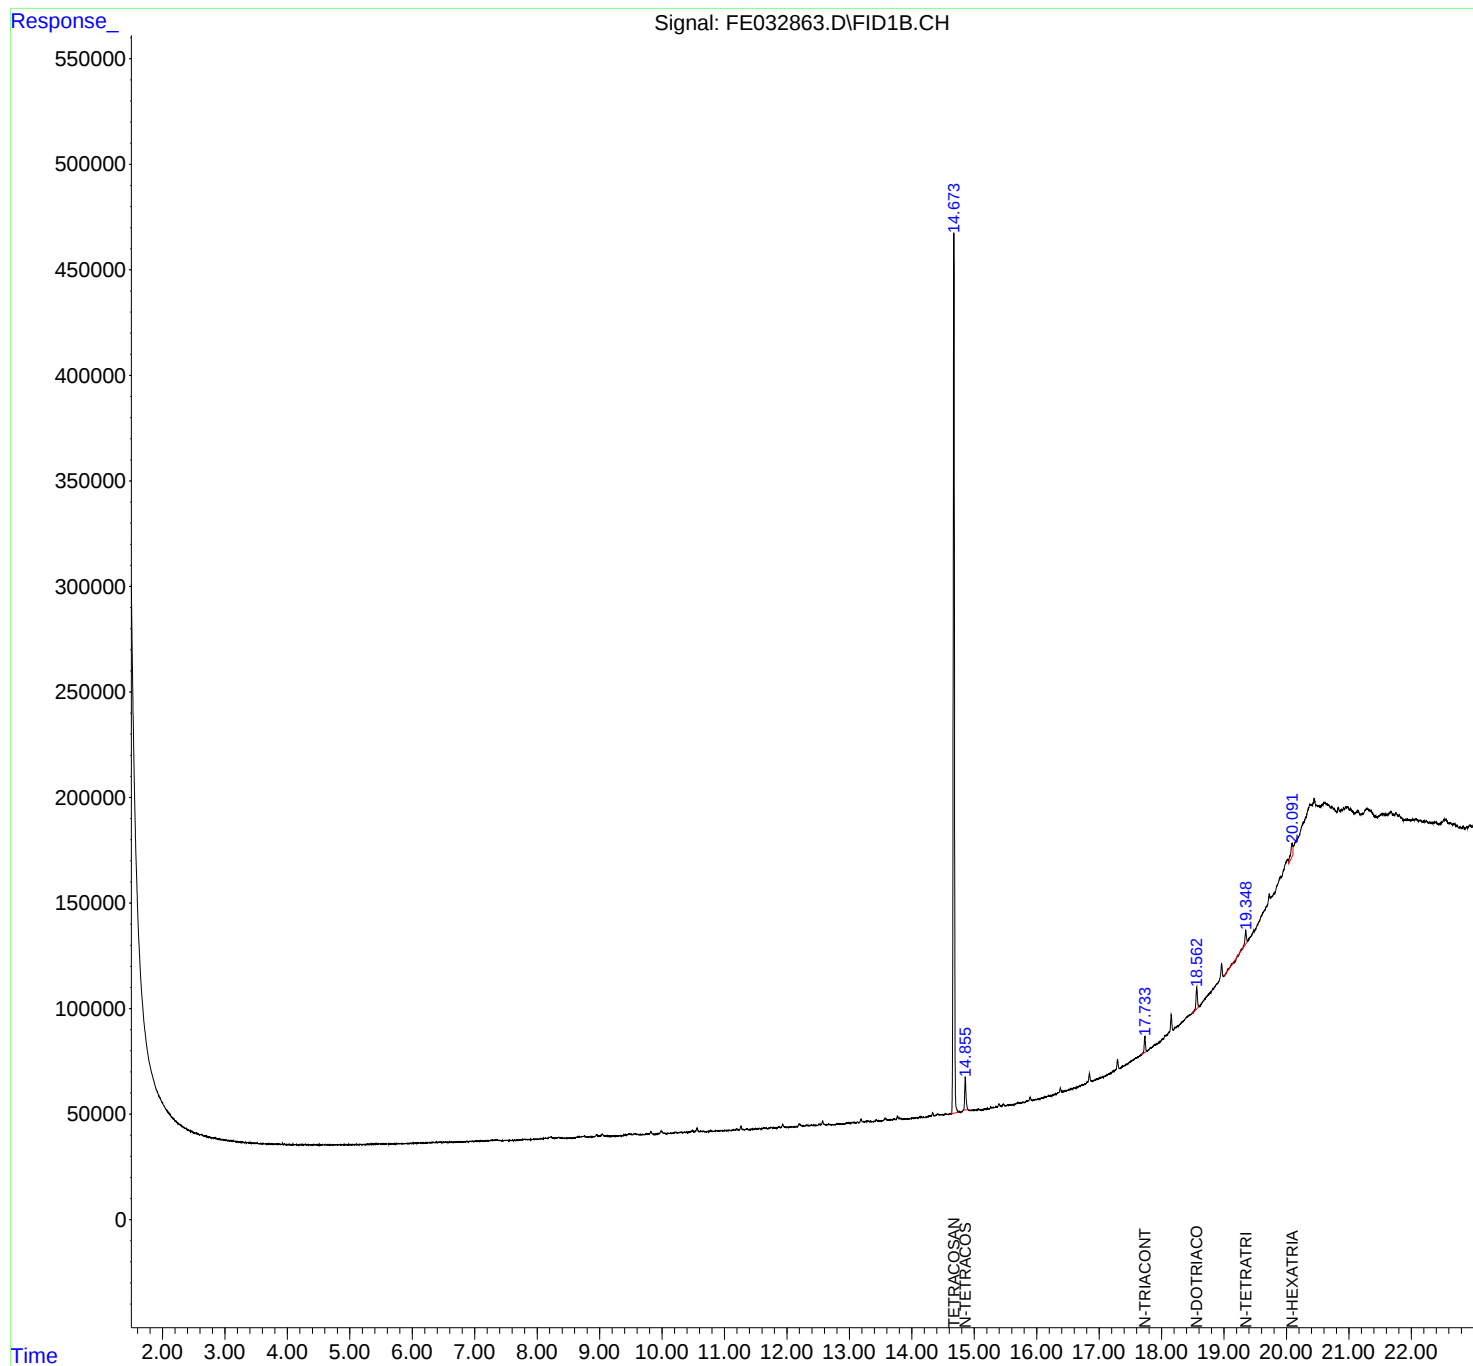


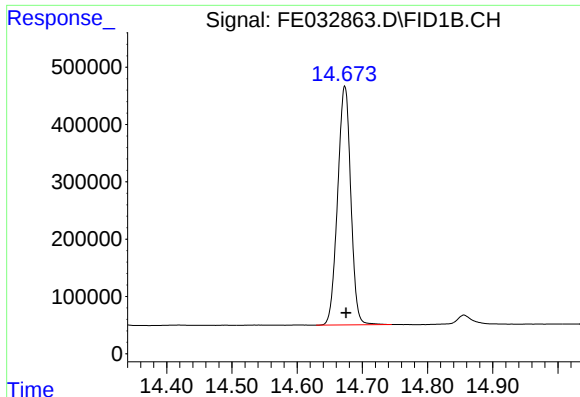

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.673 min
Delta R.T.: -0.002 min
Response: 5843483
Conc: 18.65 ug/ml

Instrument :
FID_E
ClientSampleId :

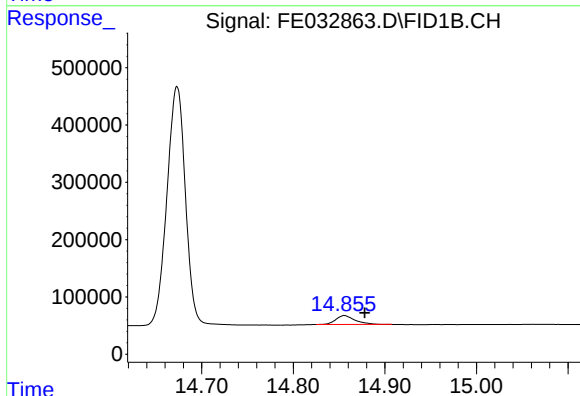


#10 N-TETRACOSANE

R.T.: 14.856 min
Delta R.T.: -0.022 min
Response: 228737
Conc: 0.65 ug/ml

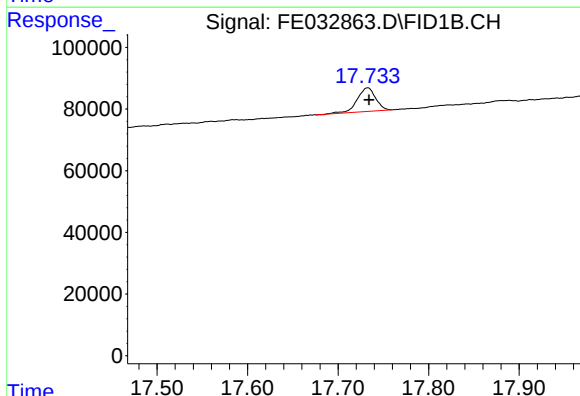


#13 N-TRIACONTANE

R.T.: 17.733 min
Delta R.T.: -0.001 min
Response: 107899
Conc: 0.31 ug/ml

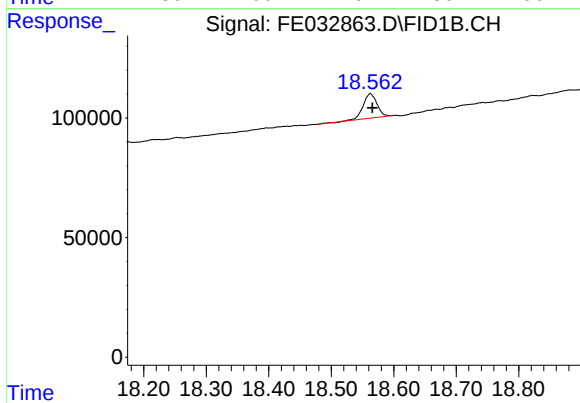

#14 N-DOTRIACONTANE

R.T.: 18.563 min
Delta R.T.: -0.003 min
Response: 156257
Conc: 0.47 ug/ml

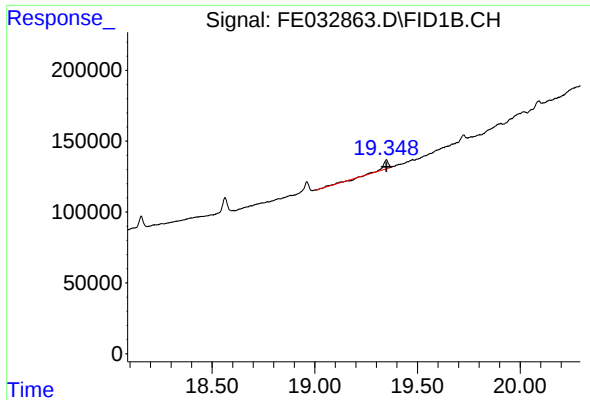

#15 N-TETRATRIACONTANE


R.T.: 19.349 min

Delta R.T.: 0.000 min

Response: 109285

Conc: 0.34 ug/ml

Instrument :
FID_E
ClientSampleId :

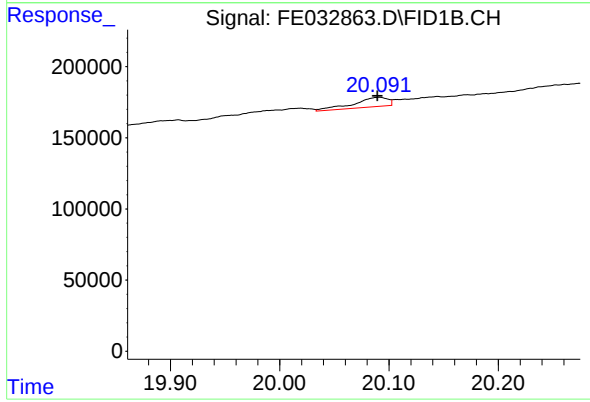

#16 N-HEXATRIACONTANE

R.T.: 20.091 min

Delta R.T.: 0.002 min

Response: 145912

Conc: 0.49 ug/ml