

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100120\
 Data File : FE032855.D
 Signal(s) : FID1B.CH
 Acq On : 01 Oct 2020 19:22
 Operator : DD\AJ
 Sample : L4190-13MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 PAV-B18-092920-10-20MSD

Integration File: autoint1.e
 Quant Time: Oct 02 01:21:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
 Quant Title :
 QLast Update : Tue Sep 15 03:21:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.678	4997163	15.950 ug/ml
Target Compounds			
2) N-DECANE	4.421	7664202	22.787 ug/ml
3) N-DODECANE	6.435	7906196	23.367 ug/ml
4) N-TETRADECANE	8.230	8245677	24.472 ug/ml
5) N-HEXADECANE	9.830	8198568	23.679 ug/ml
6) N-OCTADECANE	11.273	8350203	23.797 ug/ml
7) N-EICOSANE	12.584	8601341	24.598 ug/ml
8) N-DOCOSANE	13.782	8448746	24.272 ug/ml
10) N-TETRACOSANE	14.885	9329678	26.544 ug/ml
11) N-HEXACOSANE	15.907	8092715	23.208 ug/ml
12) N-OCTACOSANE	16.857	8012897	23.098 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100120\
Data File : FE032855.D
Signal(s) : FID1B.CH
Acq On : 01 Oct 2020 19:22
Operator : DD\AJ
Sample : L4190-13MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PAV-B18-092920-10-20MSD

Integration File: autoint1.e
Quant Time: Oct 02 01:21:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

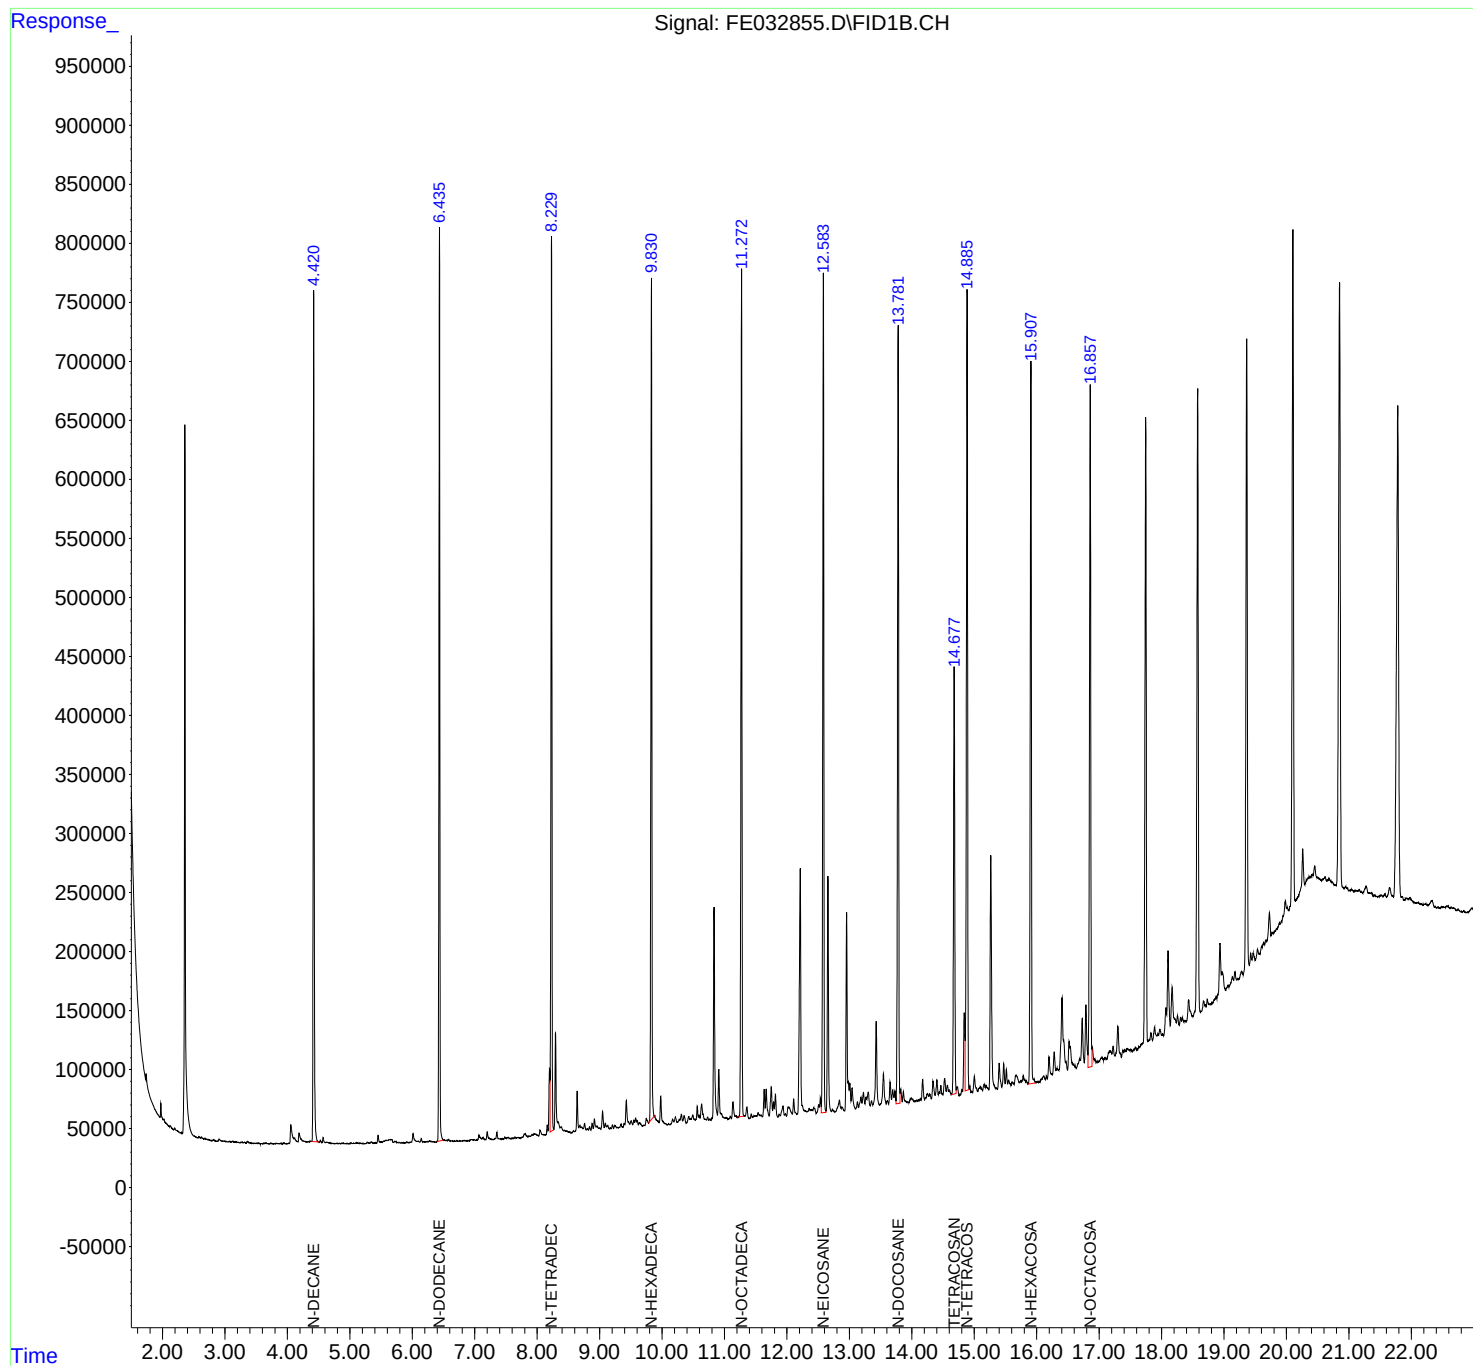


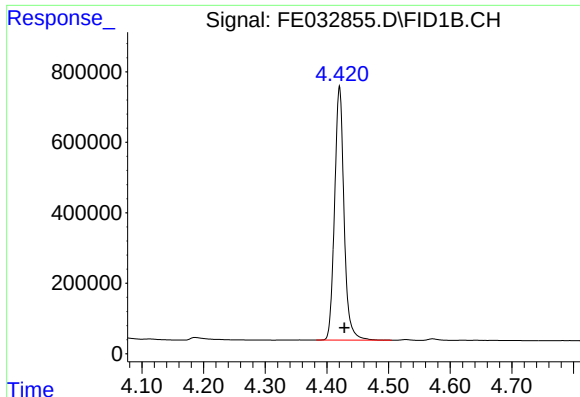

#2 N-DECANE


R.T.: 4.421 min
Delta R.T.: -0.008 min
Response: 7664202
Conc: 22.79 ug/ml

Instrument :
FID_E
ClientSampleId :
PAV-B18-092920-10-20MSD

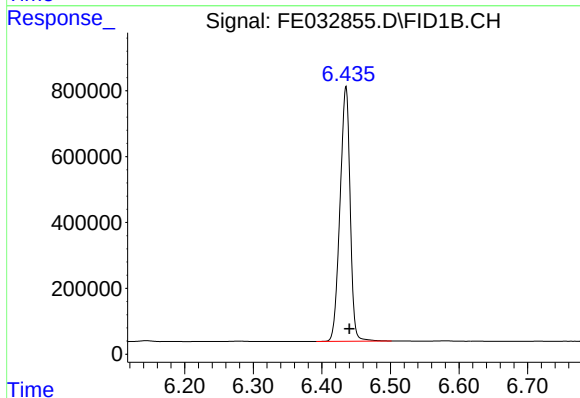


#3 N-DODECANE

R.T.: 6.435 min
Delta R.T.: -0.005 min
Response: 7906196
Conc: 23.37 ug/ml

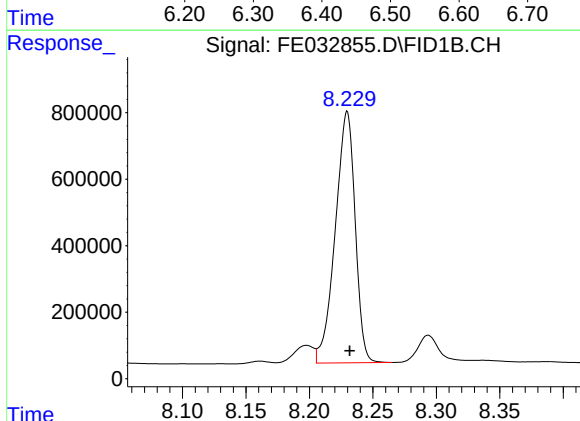


#4 N-TETRADECANE

R.T.: 8.230 min
Delta R.T.: -0.002 min
Response: 8245677
Conc: 24.47 ug/ml

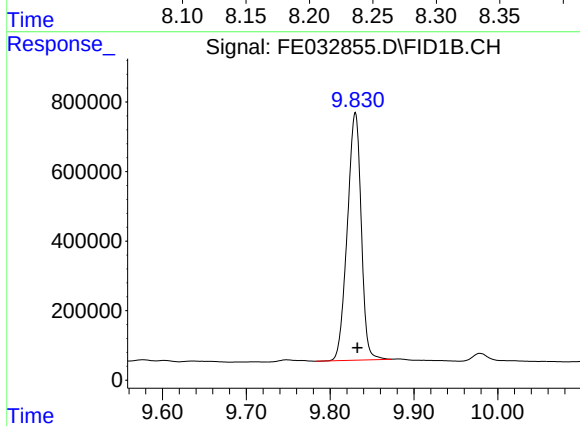

#5 N-HEXADECANE


R.T.: 9.830 min
Delta R.T.: -0.002 min
Response: 8198568
Conc: 23.68 ug/ml

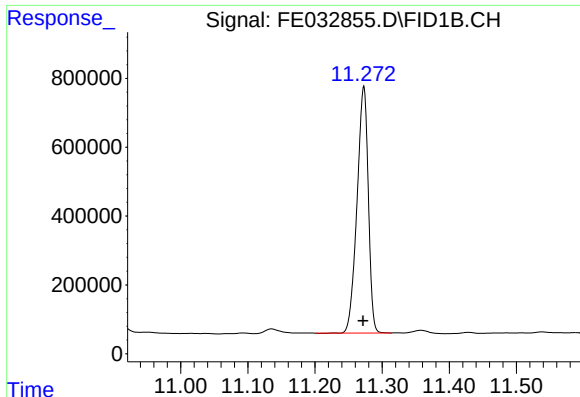

#6 N-OCTADECANE


R.T.: 11.273 min
Delta R.T.: 0.000 min
Response: 8350203
Conc: 23.80 ug/ml

Instrument :
FID_E
ClientSampleId :
PAV-B18-092920-10-20MSD

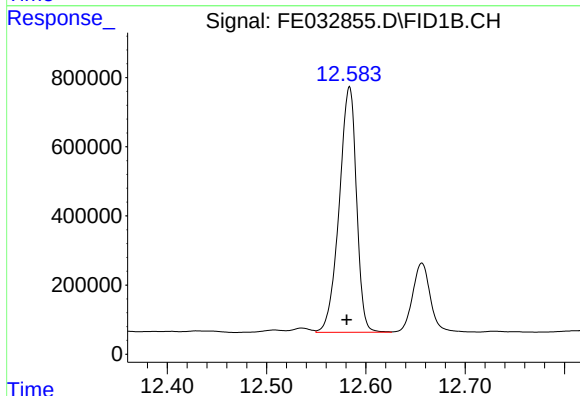


#7 N-EICOSANE

R.T.: 12.584 min
Delta R.T.: 0.003 min
Response: 8601341
Conc: 24.60 ug/ml

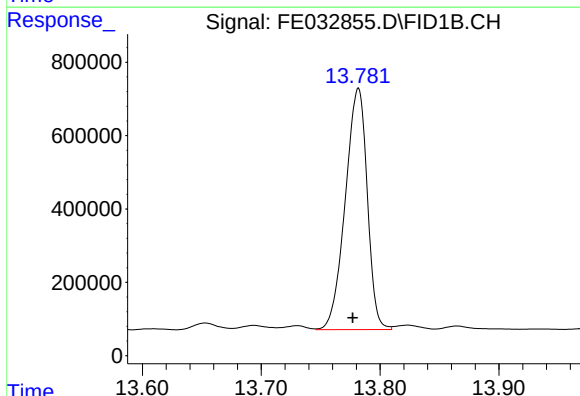


#8 N-DOCOSANE

R.T.: 13.782 min
Delta R.T.: 0.005 min
Response: 8448746
Conc: 24.27 ug/ml

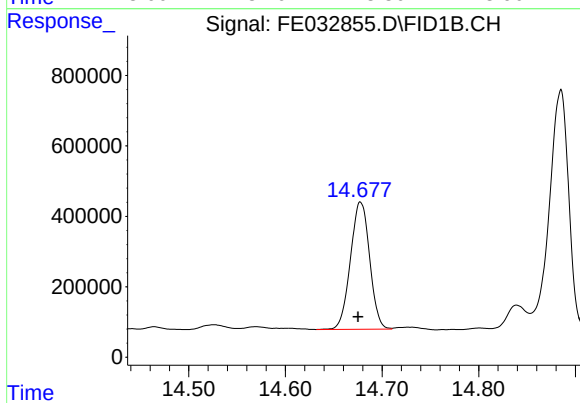

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.678 min
Delta R.T.: 0.002 min
Response: 4997163
Conc: 15.95 ug/ml

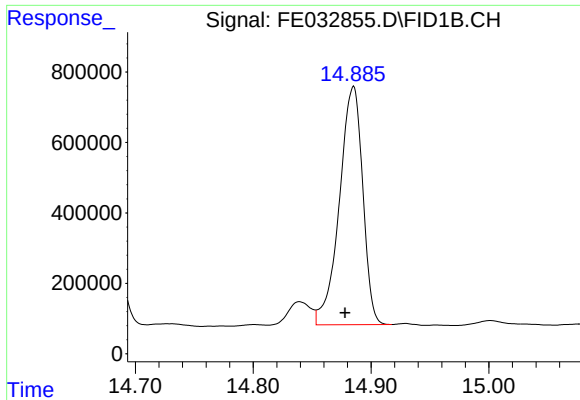

#10 N-TETRACOSANE


R.T.: 14.885 min
Delta R.T.: 0.007 min
Response: 9329678
Conc: 26.54 ug/ml

Instrument :
FID_E
ClientSampleId :
PAV-B18-092920-10-20MSD

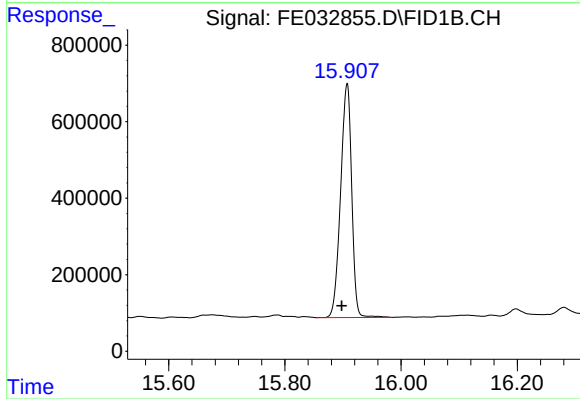

#11 N-HEXACOSANE

R.T.: 15.907 min
Delta R.T.: 0.009 min
Response: 8092715
Conc: 23.21 ug/ml

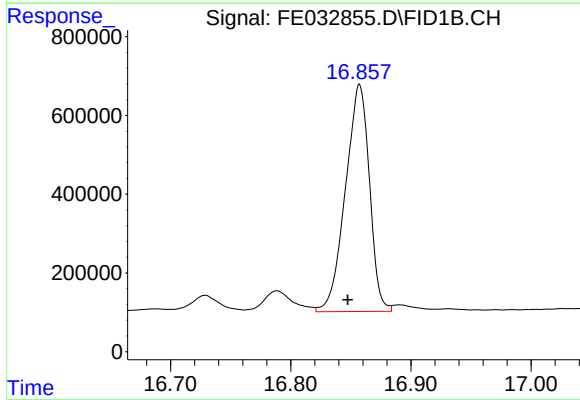

#12 N-OCTACOSANE

R.T.: 16.857 min
Delta R.T.: 0.010 min
Response: 8012897
Conc: 23.10 ug/ml