

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100220\
Data File : FE032871.D
Signal(s) : FID1B.CH
Acq On : 02 Oct 2020 15:07
Operator : DD\AJ
Sample : PB132051BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB132051BL

Integration File: autoint1.e
Quant Time: Oct 03 00:39:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.668	5309572	16.947 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.849	295141	0.840 ug/ml
14)	N-DOTRIACONTANE	18.560	106512	0.320 ug/ml
15)	N-TETRATRIACONTANE	19.343	79619	0.251 ug/ml
16)	N-HEXATRIACONTANE	20.083	60313	0.204 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100220\
Data File : FE032871.D
Signal(s) : FID1B.CH
Acq On : 02 Oct 2020 15:07
Operator : DD\AJ
Sample : PB132051BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB132051BL

Integration File: autoint1.e
Quant Time: Oct 03 00:39:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

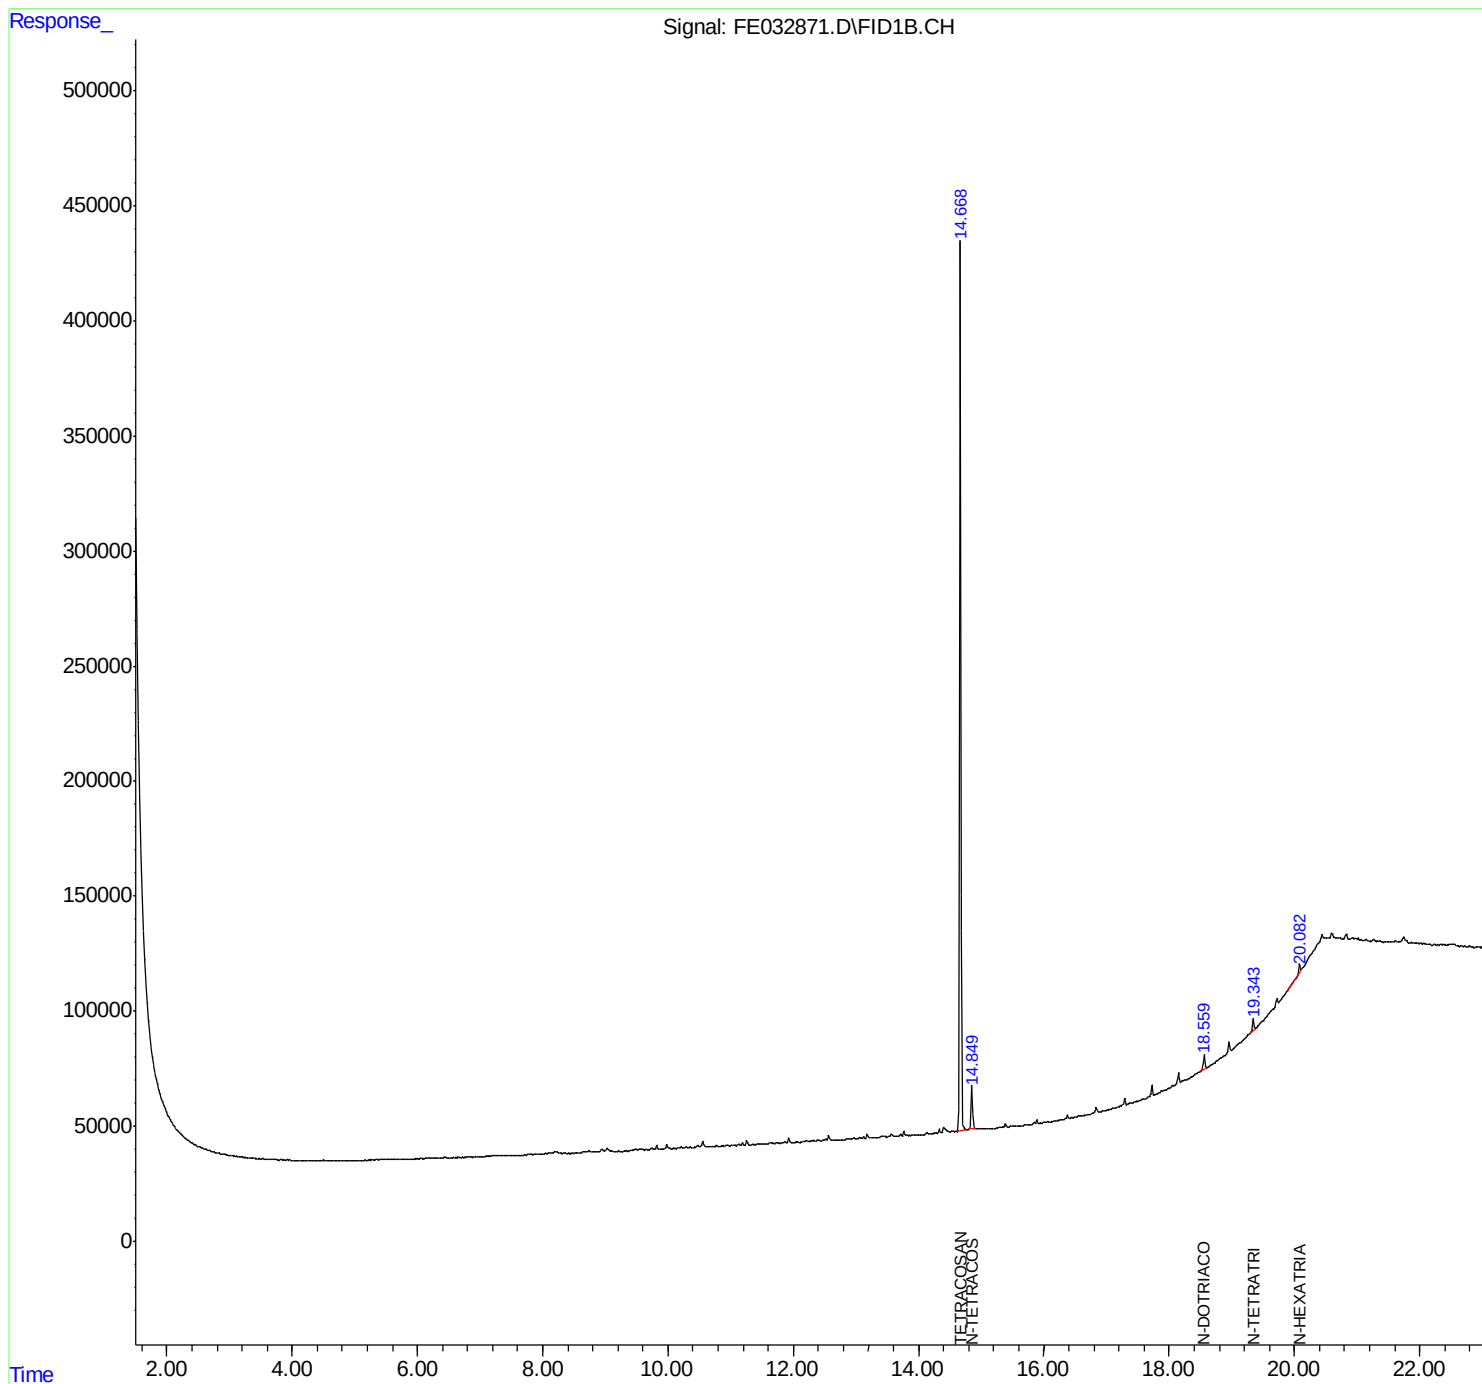


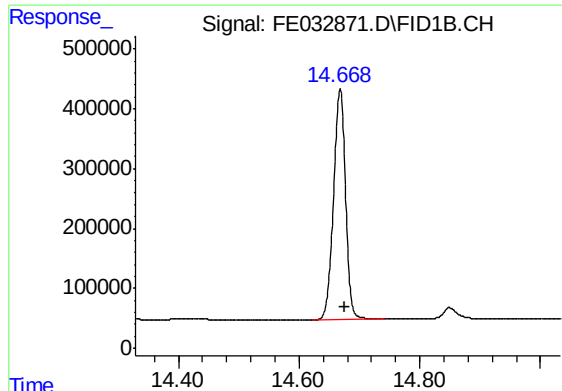

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.668 min
Delta R.T.: -0.007 min
Response: 5309572
Conc: 16.95 ug/ml

Instrument :
FID_E
ClientSampleId :
PB132051BL

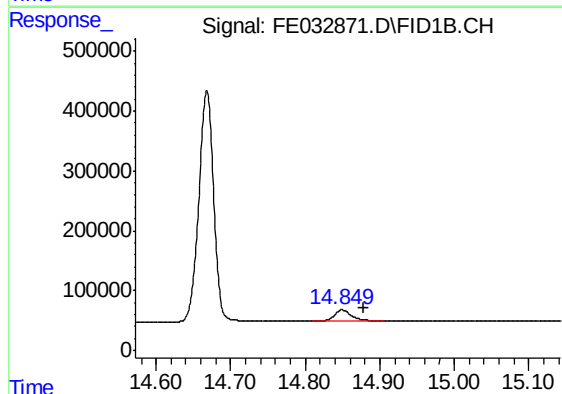


#10 N-TETRACOSANE

R.T.: 14.849 min
Delta R.T.: -0.029 min
Response: 295141
Conc: 0.84 ug/ml

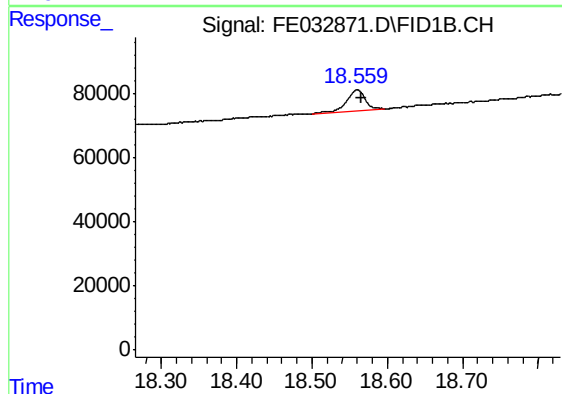


#14 N-DOTRIACONTANE

R.T.: 18.560 min
Delta R.T.: -0.006 min
Response: 106512
Conc: 0.32 ug/ml

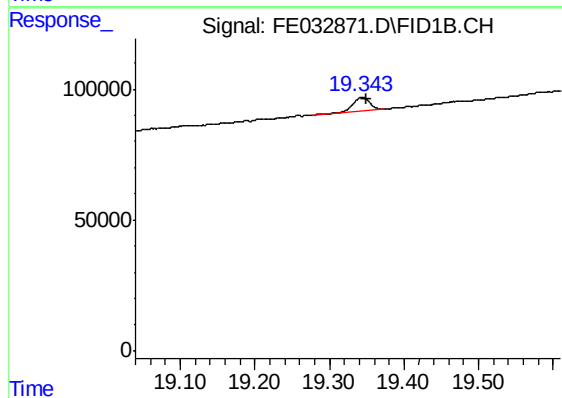

#15 N-TETRATRIACONTANE

R.T.: 19.343 min
Delta R.T.: -0.006 min
Response: 79619
Conc: 0.25 ug/ml

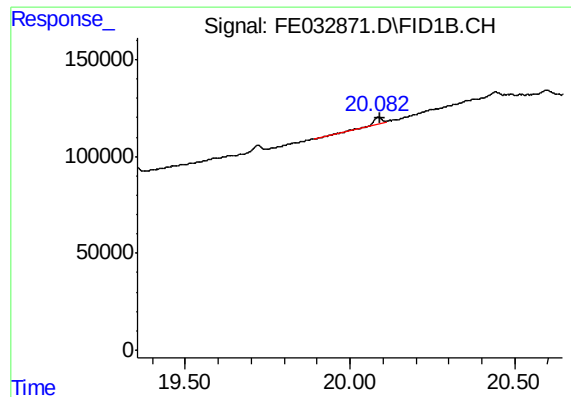

#16 N-HEXATRIACONTANE

R.T.: 20.083 min

Delta R.T.: -0.006 min

Response: 60313

Conc: 0.20 ug/ml

Instrument :
FID_E
ClientSampleId :
PB132051BL