

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100220\
 Data File : FE032883.D
 Signal(s) : FID1B.CH
 Acq On : 02 Oct 2020 22:54
 Operator : DD\AJ
 Sample : L4226-01 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 TR-05-100120

Integration File: autoint1.e
 Quant Time: Oct 03 00:42:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
 Quant Title :
 QLast Update : Tue Sep 15 03:21:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.669	2155557	6.880 ug/ml
Target Compounds			
4) N-TETRADECANE	8.286f	295836	0.878 ug/ml
7) N-EICOSANE	12.568	152964	0.437 ug/ml
8) N-DOCOSANE	13.769	182358	0.524 ug/ml
10) N-TETRACOSANE	14.871	1558593	4.434 ug/ml
11) N-HEXACOSANE	15.894	219413	0.629 ug/ml
12) N-OCTACOSANE	16.843	396078	1.142 ug/ml
13) N-TRIACONTANE	17.732	690762	2.003 ug/ml
14) N-DOTRIACONTANE	18.561	883145	2.653 ug/ml
15) N-TETRATRIACONTANE	19.349	345862	1.088 ug/ml
16) N-HEXATRIACONTANE	20.091	529034	1.793 ug/ml
17) N-OCTATRIACONTANE	20.830	148682	0.547 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100220\
Data File : FE032883.D
Signal(s) : FID1B.CH
Acq On : 02 Oct 2020 22:54
Operator : DD\AJ
Sample : L4226-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TR-05-100120

Integration File: autoint1.e
Quant Time: Oct 03 00:42:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

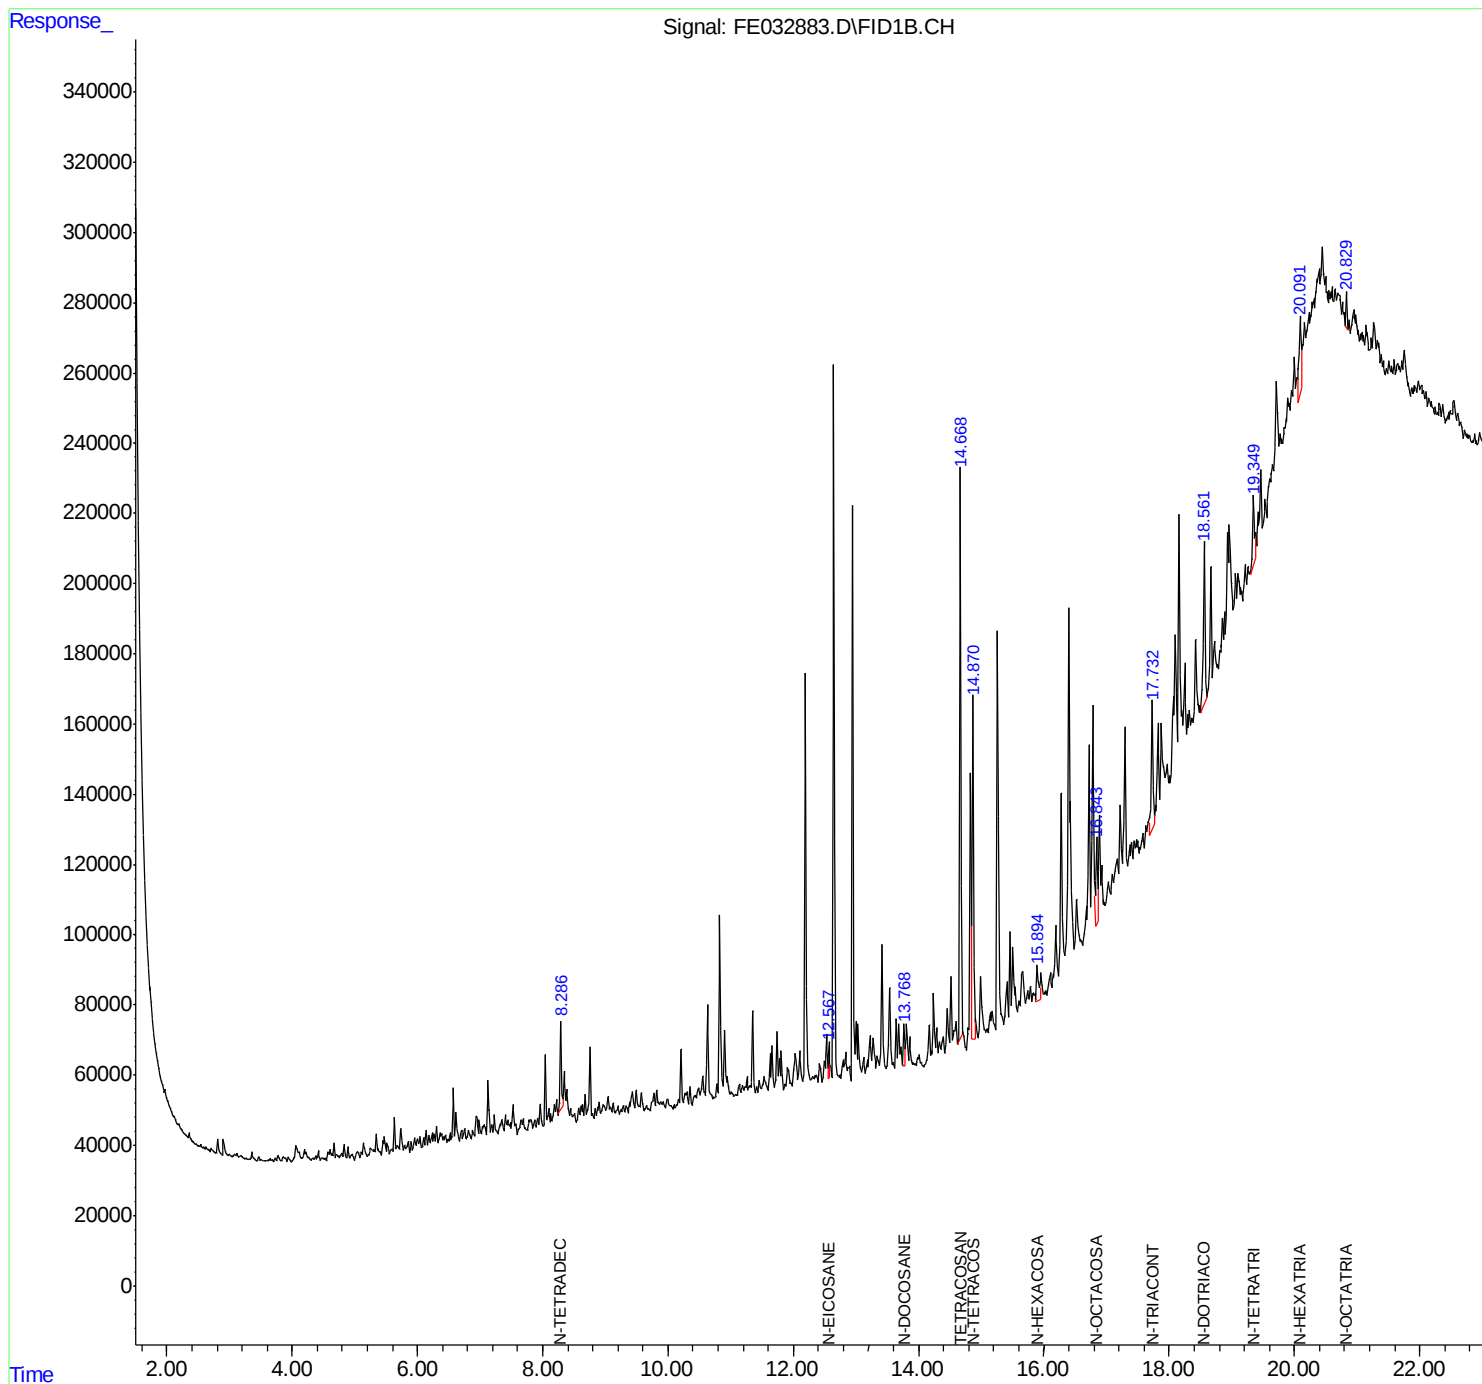


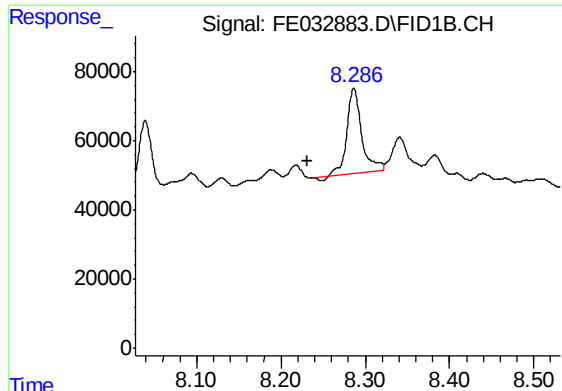

#4 N-TETRADECANE


R.T.: 8.286 min
Delta R.T.: 0.055 min
Response: 295836
Conc: 0.88 ug/ml

Instrument :
FID_E
ClientSampleId :
TR-05-100120

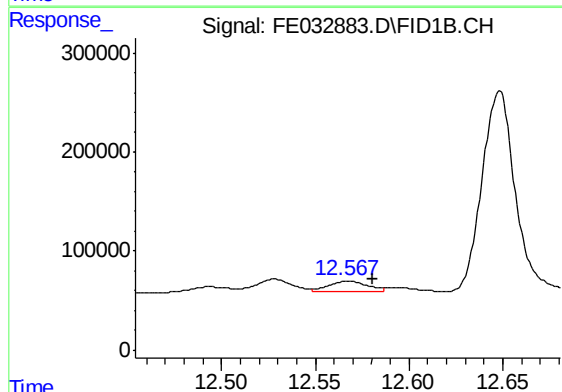


#7 N-EICOSANE

R.T.: 12.568 min
Delta R.T.: -0.013 min
Response: 152964
Conc: 0.44 ug/ml

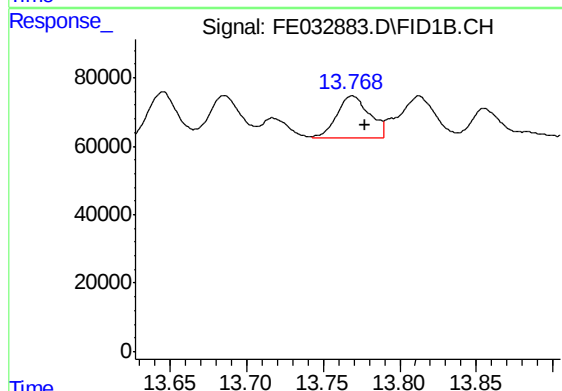


#8 N-DOCOSANE

R.T.: 13.769 min
Delta R.T.: -0.008 min
Response: 182358
Conc: 0.52 ug/ml

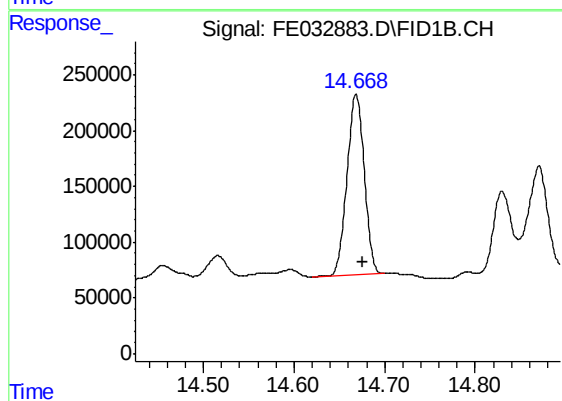

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.669 min
Delta R.T.: -0.007 min
Response: 215557
Conc: 6.88 ug/ml

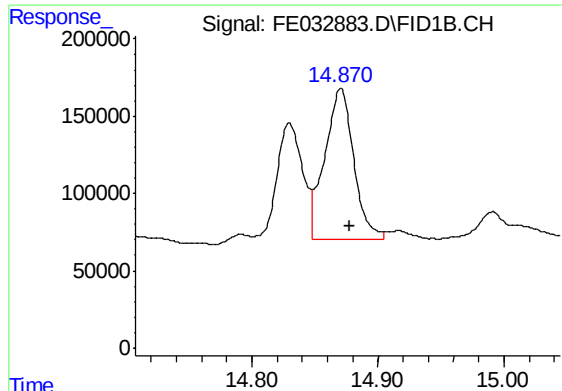

#10 N-TETRACOSANE


R.T.: 14.871 min
Delta R.T.: -0.008 min
Response: 1558593
Conc: 4.43 ug/ml

Instrument :
FID_E
ClientSampleId :
TR-05-100120

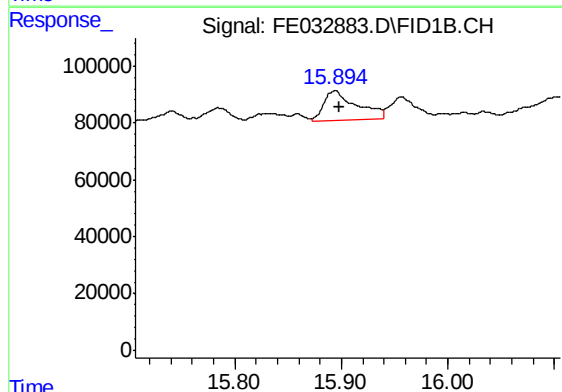


#11 N-HEXACOSANE

R.T.: 15.894 min
Delta R.T.: -0.004 min
Response: 219413
Conc: 0.63 ug/ml

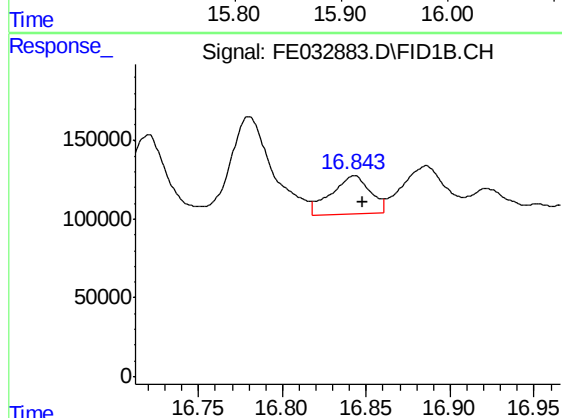


#12 N-OCTACOSANE

R.T.: 16.843 min
Delta R.T.: -0.005 min
Response: 396078
Conc: 1.14 ug/ml

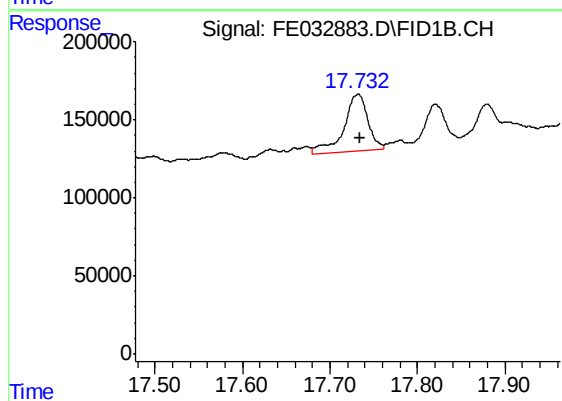

#13 N-TRIACONTANE


R.T.: 17.732 min
Delta R.T.: -0.002 min
Response: 690762
Conc: 2.00 ug/ml

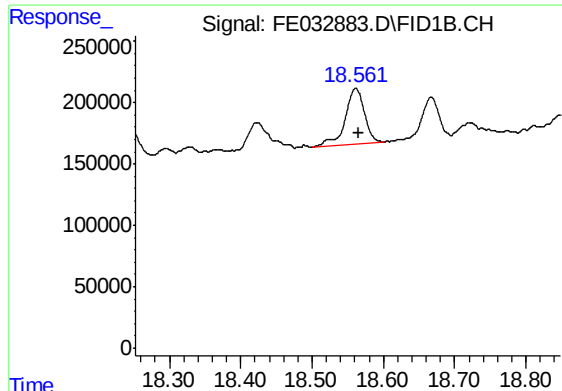

#14 N-DOTRIACONTANE


R.T.: 18.561 min
Delta R.T.: -0.004 min
Response: 883145
Conc: 2.65 ug/ml

Instrument :
FID_E
ClientSampleId :
TR-05-100120

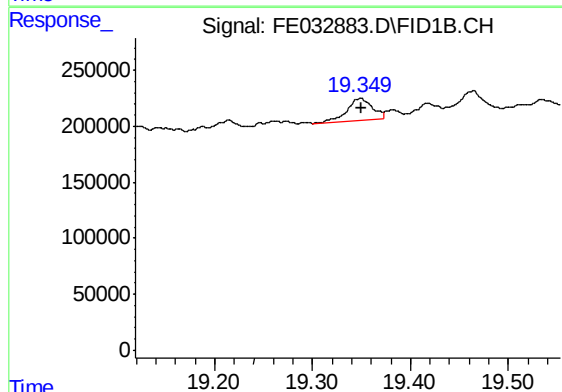


#15 N-TETRATRIACONTANE

R.T.: 19.349 min
Delta R.T.: 0.000 min
Response: 345862
Conc: 1.09 ug/ml

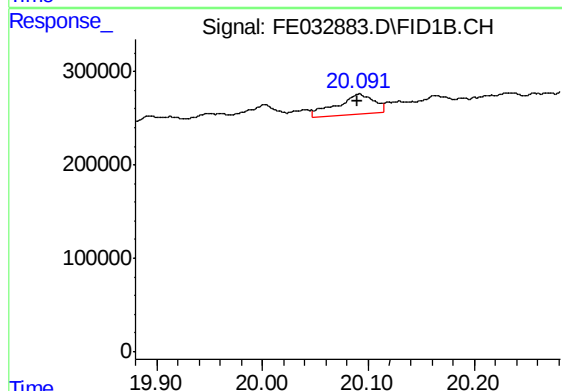

#16 N-HEXATRIACONTANE

R.T.: 20.091 min
Delta R.T.: 0.002 min
Response: 529034
Conc: 1.79 ug/ml

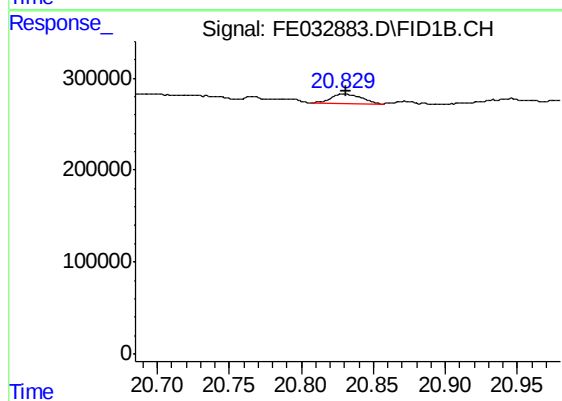

#17 N-OCTATRIACONTANE

R.T.: 20.830 min
Delta R.T.: -0.001 min
Response: 148682
Conc: 0.55 ug/ml