

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100220\
 Data File : FE032893.D
 Signal(s) : FID1B.CH
 Acq On : 03 Oct 2020 6:10
 Operator : DD\AJ
 Sample : L4238-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 03 07:55:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
 Quant Title :
 QLast Update : Tue Sep 15 03:21:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.666	5480240	17.492 ug/ml
Target Compounds			
4) N-TETRADECANE	8.219	178868	0.531 ug/ml
7) N-EICOSANE	12.567	194645	0.557 ug/ml
8) N-DOCOSANE	13.763	233974	0.672 ug/ml
10) N-TETRACOSANE	14.866	764202	2.174 ug/ml
11) N-HEXACOSANE	15.886	290769	0.834 ug/ml
12) N-OCTACOSANE	16.836	550049	1.586 ug/ml
13) N-TRIACONTANE	17.724	529447	1.535 ug/ml
14) N-DOTRIACONTANE	18.554	1032811	3.103 ug/ml
15) N-TETRATRIACONTANE	19.338	264711	0.833 ug/ml
16) N-HEXATRIACONTANE	20.078	441631	1.496 ug/ml
17) N-OCTATRIACONTANE	20.820	158044	0.581 ug/ml
18) N-TETRACONTANE	21.741	302505	1.120 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100220\
Data File : FE032893.D
Signal(s) : FID1B.CH
Acq On : 03 Oct 2020 6:10
Operator : DD\AJ
Sample : L4238-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Oct 03 07:55:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

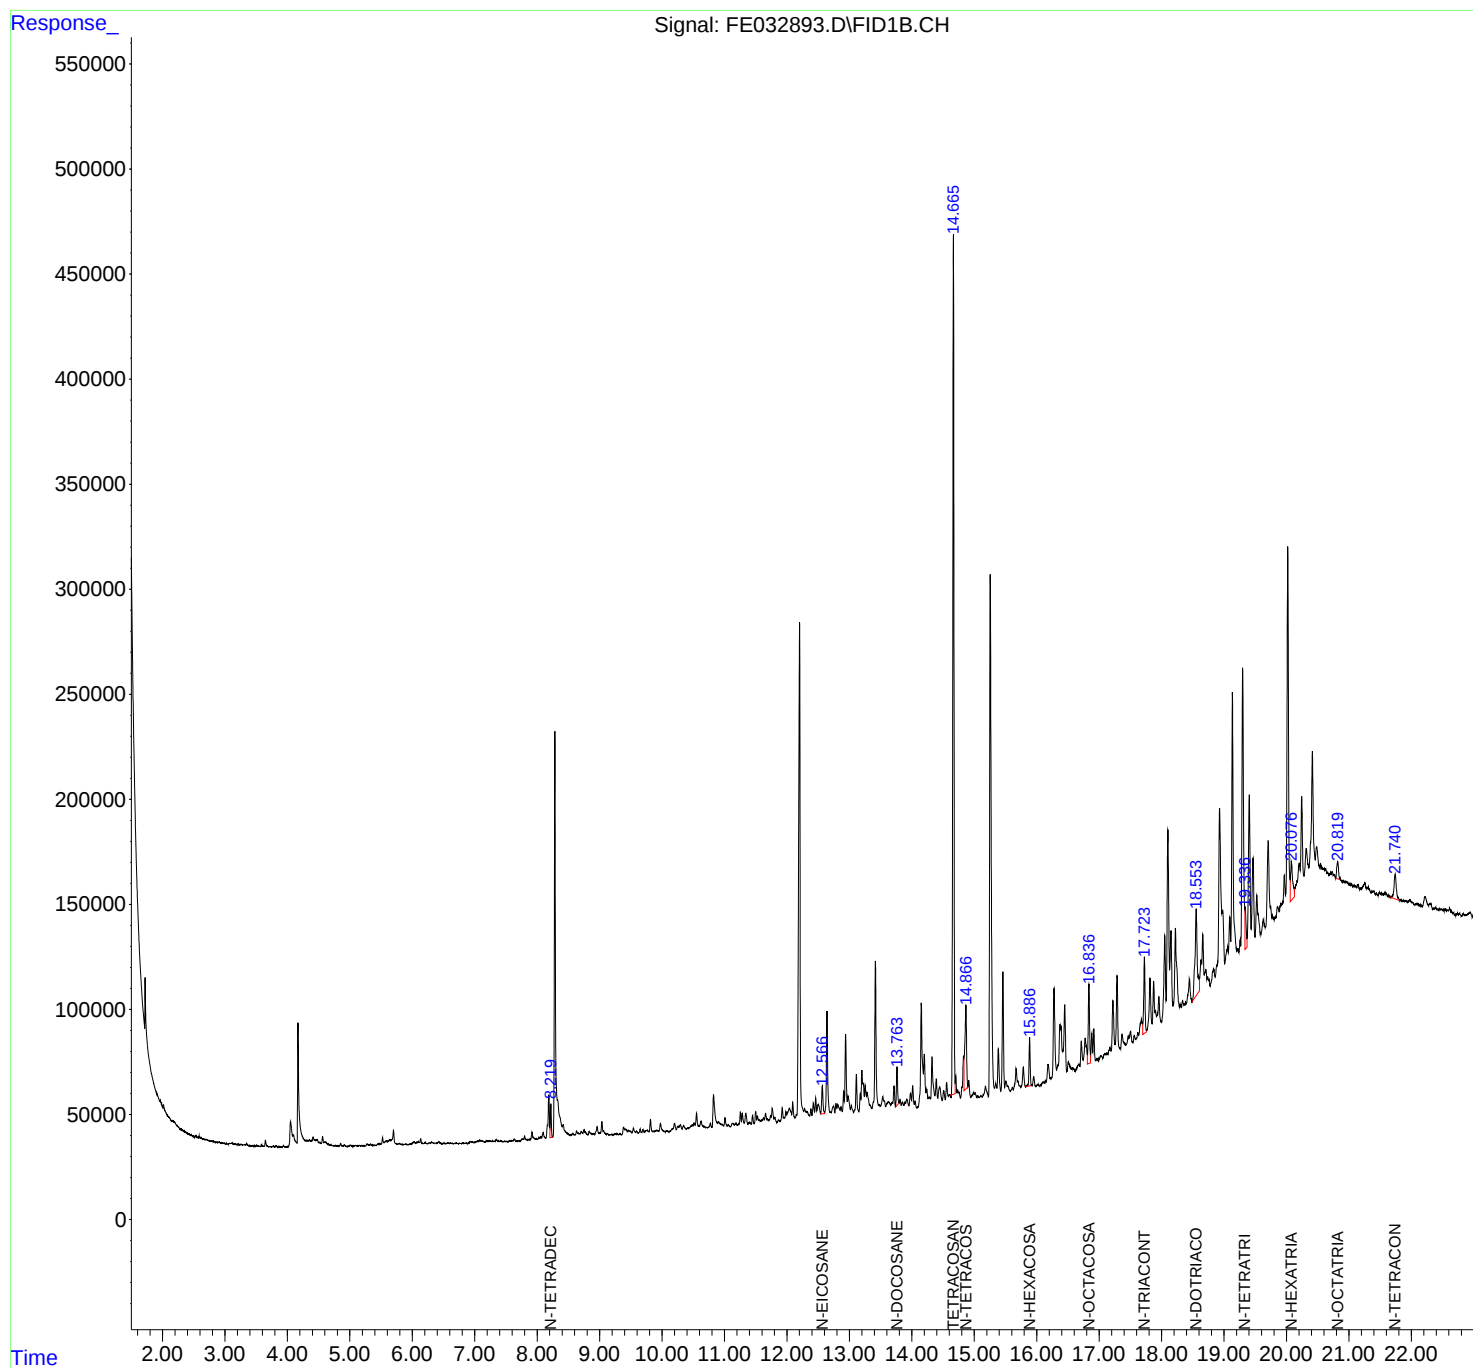


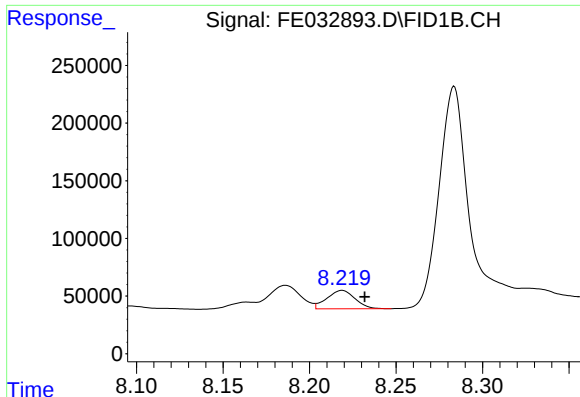

#4 N-TETRADECANE


R.T.: 8.219 min
Delta R.T.: -0.013 min
Response: 178868
Conc: 0.53 ug/ml

Instrument :
FID_E
ClientSampleId :

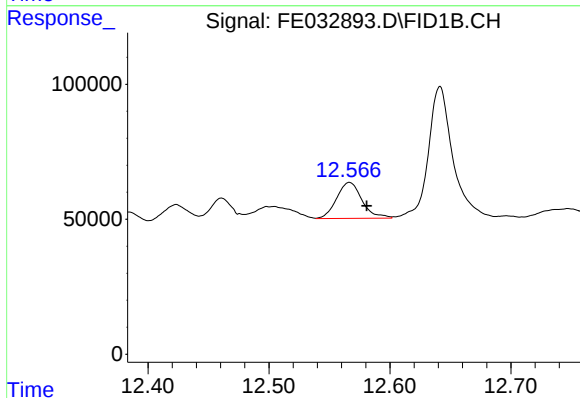


#7 N-EICOSANE

R.T.: 12.567 min
Delta R.T.: -0.014 min
Response: 194645
Conc: 0.56 ug/ml

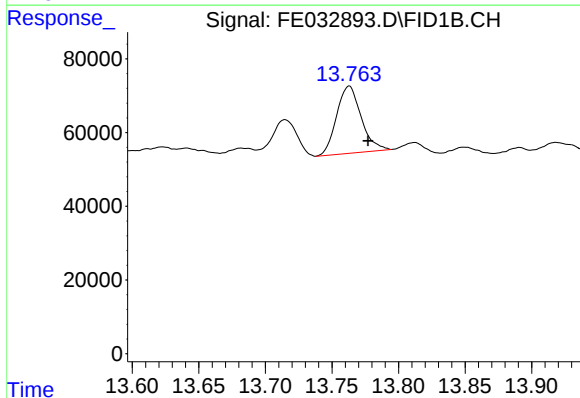


#8 N-DOCOSANE

R.T.: 13.763 min
Delta R.T.: -0.014 min
Response: 233974
Conc: 0.67 ug/ml

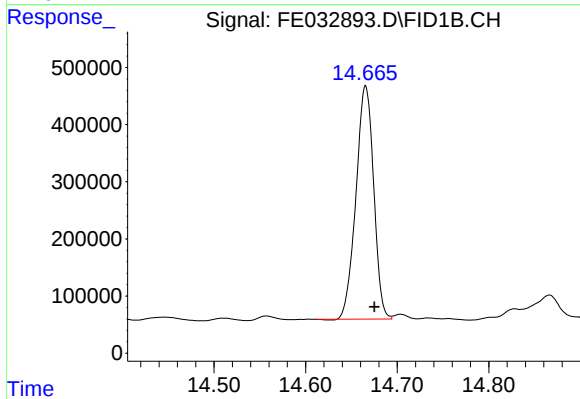

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.666 min
Delta R.T.: -0.010 min
Response: 5480240
Conc: 17.49 ug/ml

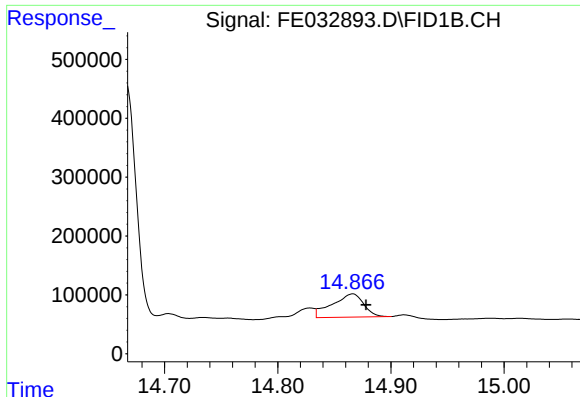

#10 N-TETRACOSANE


R.T.: 14.866 min
Delta R.T.: -0.012 min
Response: 764202
Conc: 2.17 ug/ml

Instrument :
FID_E
ClientSampleId :

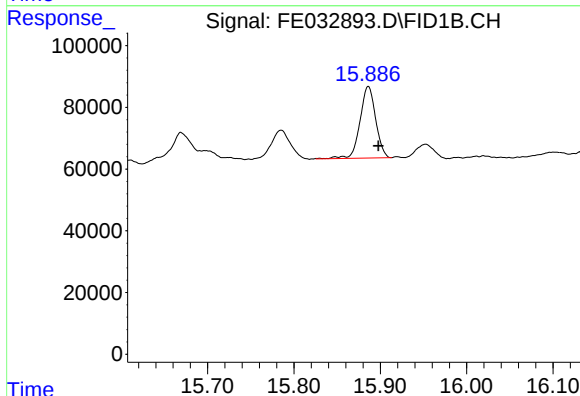


#11 N-HEXACOSANE

R.T.: 15.886 min
Delta R.T.: -0.012 min
Response: 290769
Conc: 0.83 ug/ml

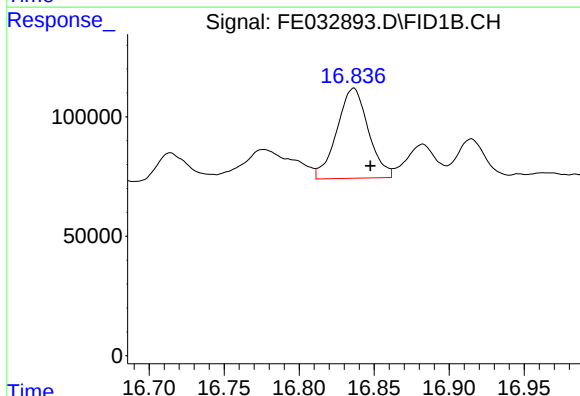


#12 N-OCTACOSANE

R.T.: 16.836 min
Delta R.T.: -0.011 min
Response: 550049
Conc: 1.59 ug/ml

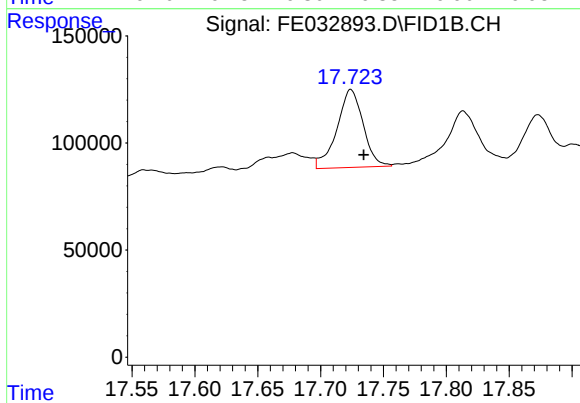

#13 N-TRIACONTANE


R.T.: 17.724 min
Delta R.T.: -0.010 min
Response: 529447
Conc: 1.54 ug/ml

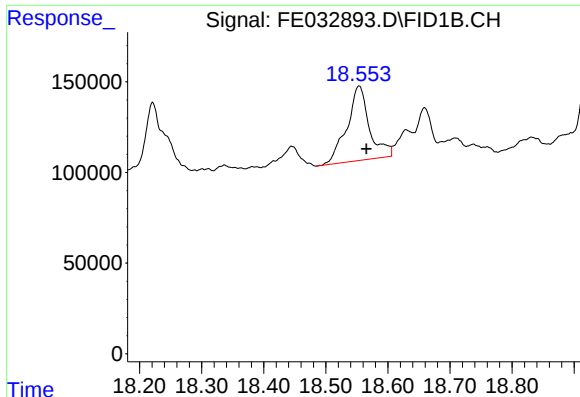

#14 N-DOTRIACONTANE


R.T.: 18.554 min
Delta R.T.: -0.012 min
Response: 1032811
Conc: 3.10 ug/ml

Instrument :
FID_E
ClientSampleId :

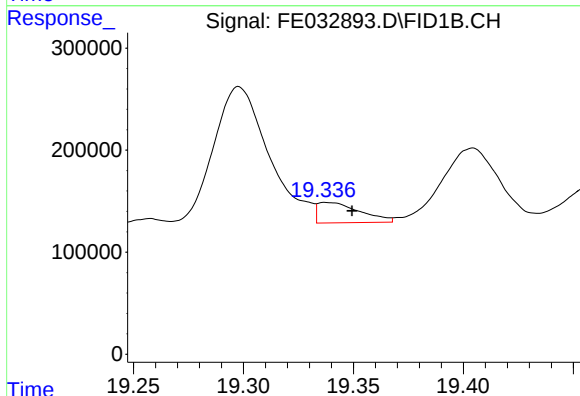


#15 N-TETRATRIACONTANE

R.T.: 19.338 min
Delta R.T.: -0.012 min
Response: 264711
Conc: 0.83 ug/ml

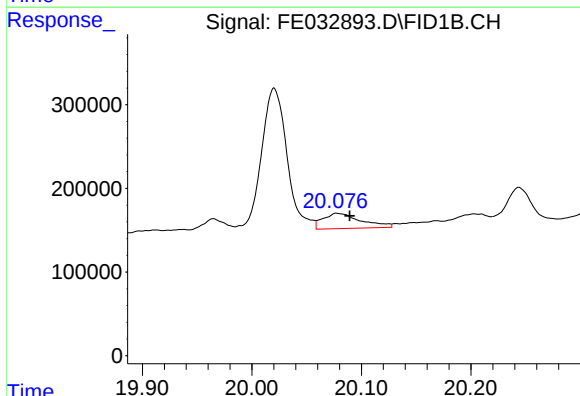


#16 N-HEXATRIACONTANE

R.T.: 20.078 min
Delta R.T.: -0.012 min
Response: 441631
Conc: 1.50 ug/ml

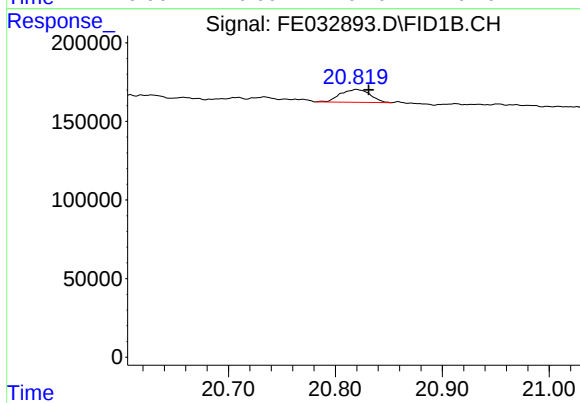

#17 N-OCTATRIACONTANE

R.T.: 20.820 min
Delta R.T.: -0.011 min
Response: 158044
Conc: 0.58 ug/ml

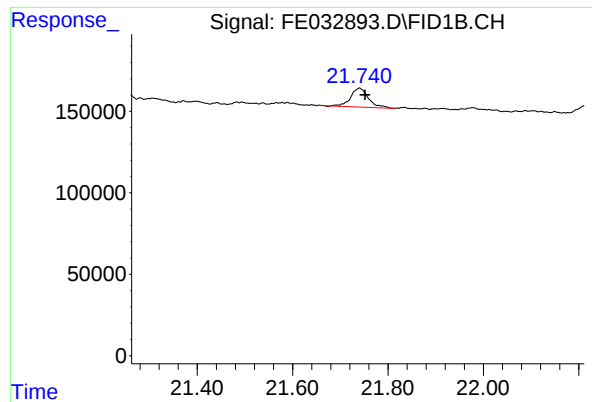

#18 N-TETRACONTANE

R.T.: 21.741 min
Delta R.T.: -0.012 min
Response: 302505
Conc: 1.12 ug/ml

Instrument :
FID_E
ClientSampleId :