

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100220\
Data File : FE032883.D
Signal(s) : FID1B.CH
Acq On : 02 Oct 2020 22:54
Operator : DD\AJ
Sample : L4226-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TR-05-100120

Integration File: autoint1.e
Quant Time: Oct 03 00:42:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.669	2155557	6.880 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100220\
Data File : FE032883.D
Signal(s) : FID1B.CH
Acq On : 02 Oct 2020 22:54
Operator : DD\AJ
Sample : L4226-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TR-05-100120

Integration File: autoint1.e
Quant Time: Oct 03 00:42:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

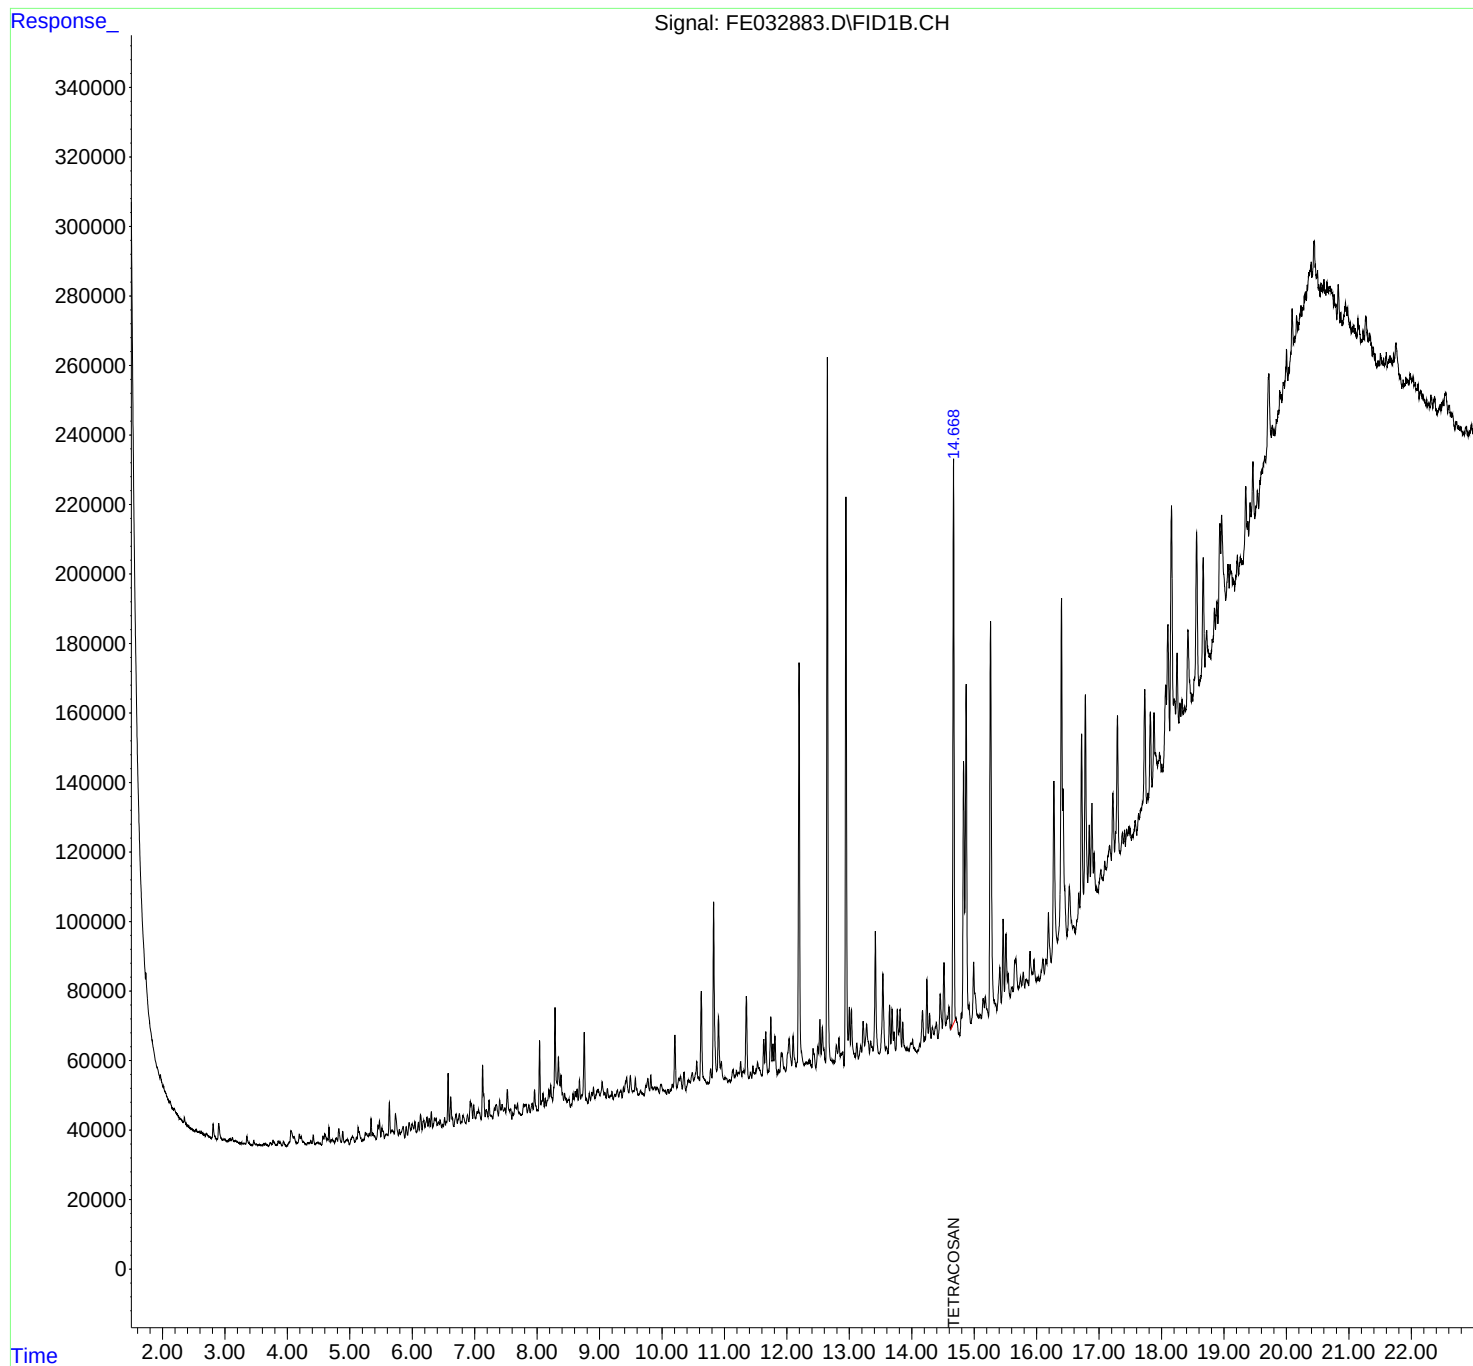

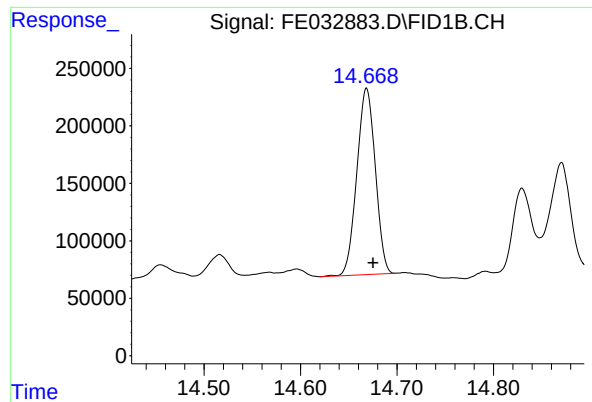

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.669 min
Delta R.T.: -0.007 min
Response: 2155557
Conc: 6.88 ug/ml

Instrument :
FID_E
ClientSampleId :
TR-05-100120