

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100220\  
 Data File : FE032890.D  
 Signal(s) : FID1B.CH  
 Acq On : 03 Oct 2020 4:29  
 Operator : DD\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 RT MARKER

Integration File: autoint1.e  
 Quant Time: Oct 03 05:36:41 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE091420.M  
 Quant Title :  
 QLast Update : Tue Sep 15 03:21:18 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.433  | 18003820 | 53.212 ug/ml |
| 12) N-OCTACOSANE            | 16.851 | 18268167 | 52.659 ug/ml |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100220\  
Data File : FE032890.D  
Signal(s) : FID1B.CH  
Acq On : 03 Oct 2020 4:29  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Oct 03 05:36:41 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE091420.M  
Quant Title :  
QLast Update : Tue Sep 15 03:21:18 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

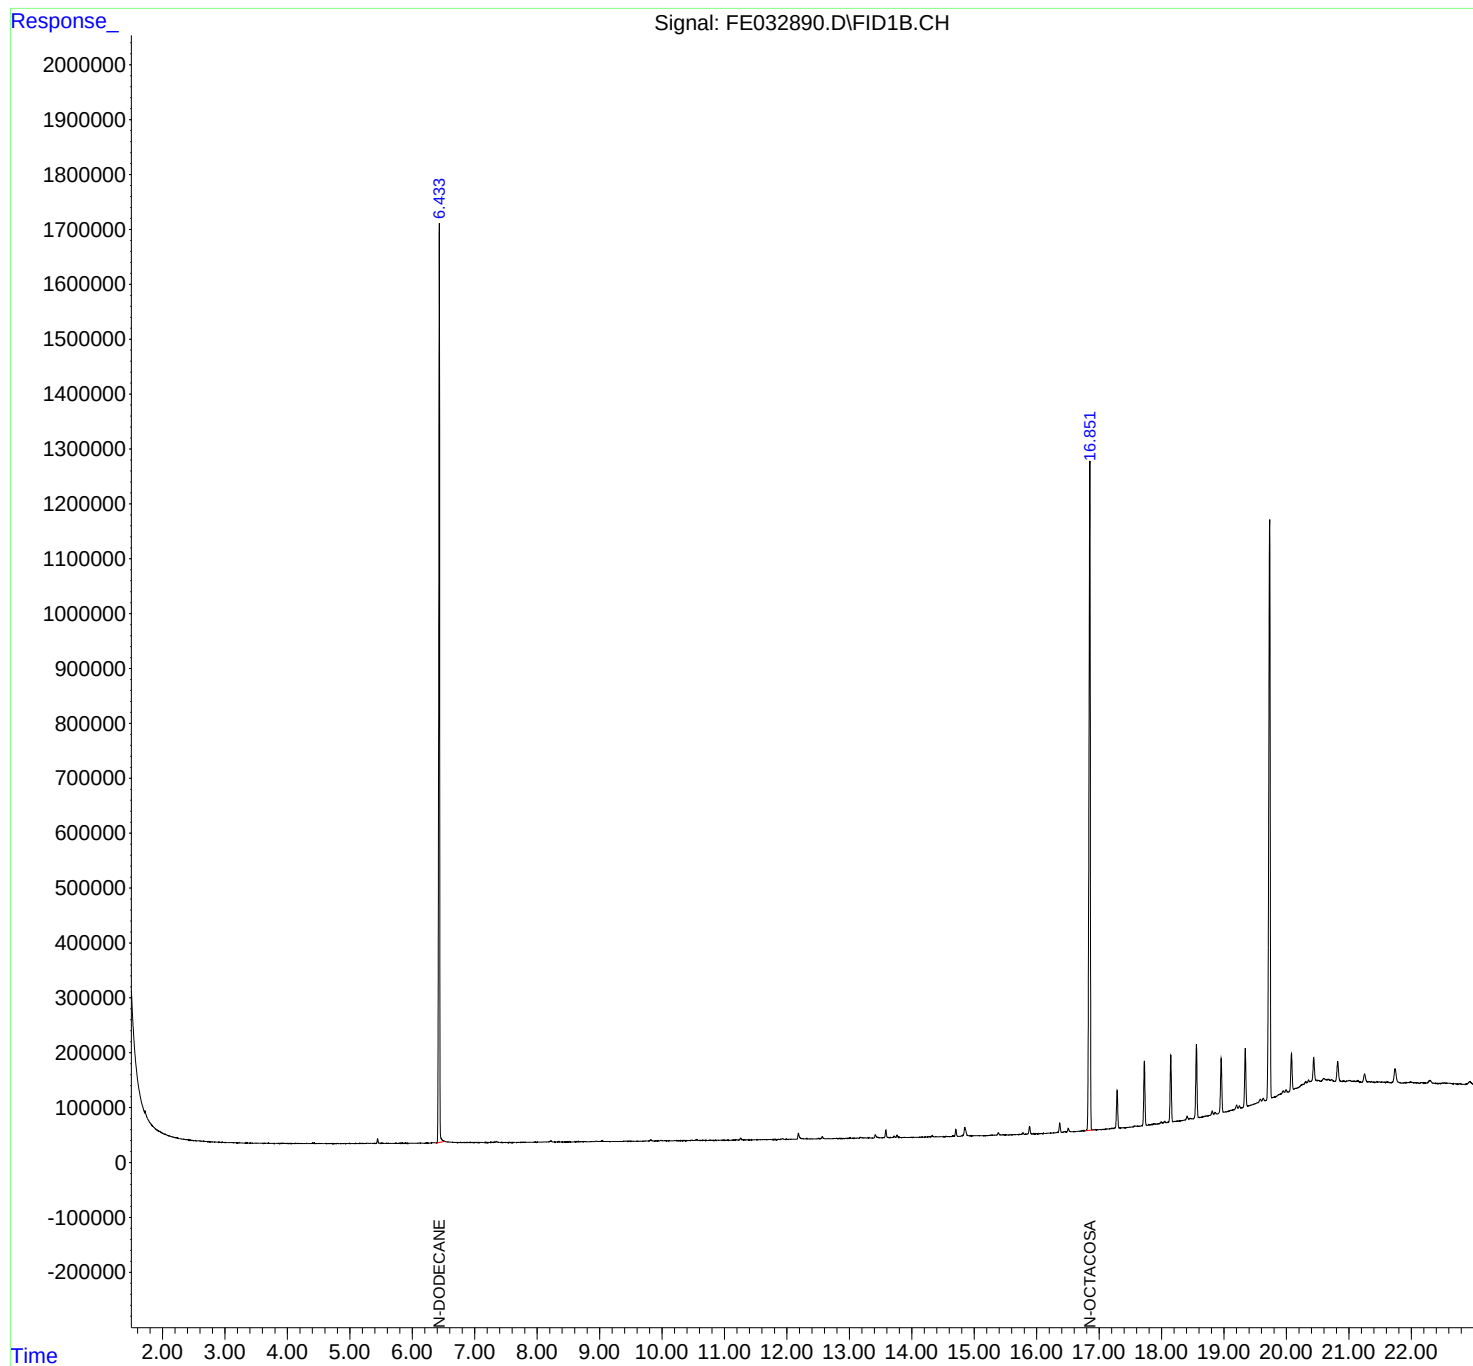


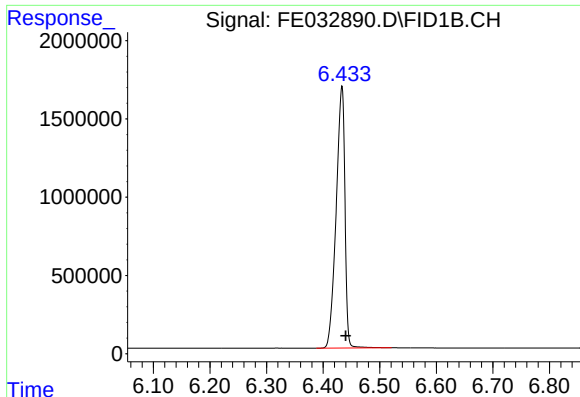

#3 N-DODECANE


R.T.: 6.433 min  
Delta R.T.: -0.006 min  
Response: 18003820  
Conc: 53.21 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
RT MARKER

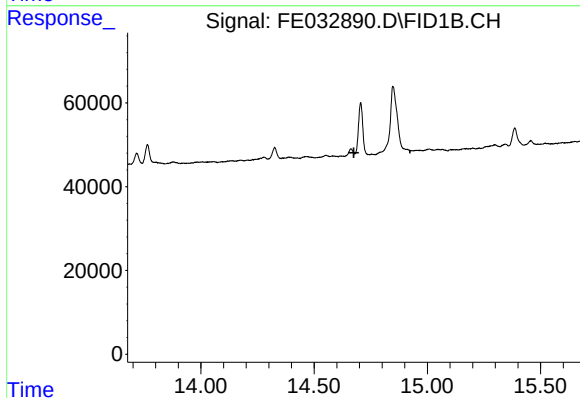

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.675 min  
Response: 0  
Conc: N.D.

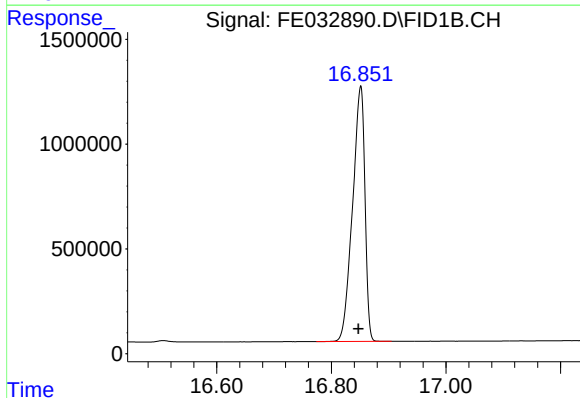

#12 N-OCTACOSANE

R.T.: 16.851 min  
Delta R.T.: 0.004 min  
Response: 18268167  
Conc: 52.66 ug/ml