

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100223AL\
 Data File : FE044536.D
 Signal(s) : FID1B.ch
 Acq On : 02 Oct 2023 07:41
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 03 00:17:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092523.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 25 11:06:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13) T	n-Docosane (C22)	14.099	345216	2.238 ug/ml
14) T	n-Tetracosane (C24)	15.215	622282	4.117 ug/ml
15) T	n-Hexacosane (C26)	16.243	722208	4.910 ug/ml
16) T	n-Octacosane (C28)	17.195	585412	4.082 ug/ml
17) T	n-Tricontane (C30)	18.084	489681	3.303 ug/ml
18) T	n-Dotriacontane (C32)	18.918	1034256	6.987 ug/ml
19) T	n-Tetratriacontane (C34)	19.703	652890	4.467 ug/ml
20) T	n-Hexatriacontane (C36)	20.446	220602	1.521 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100223AL\
Data File : FE044536.D
Signal(s) : FID1B.ch
Acq On : 02 Oct 2023 07:41
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 00:17:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 11:06:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

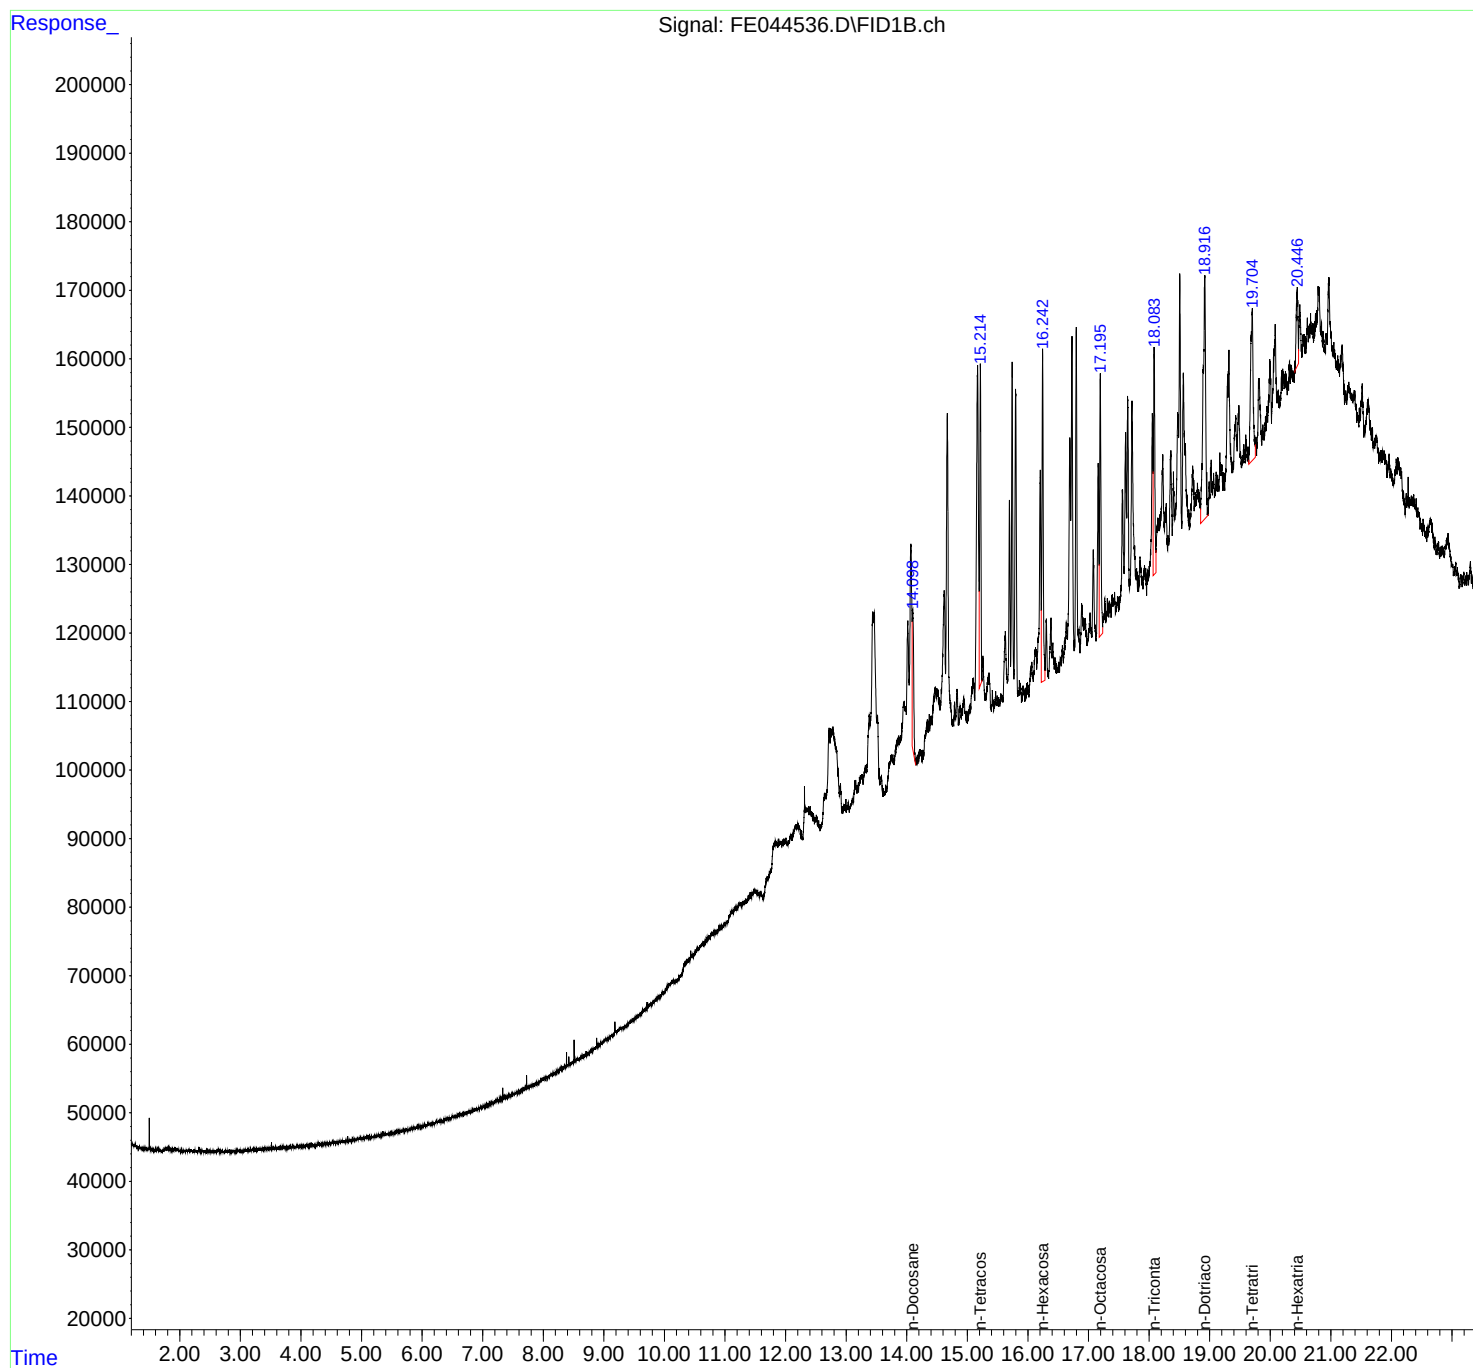


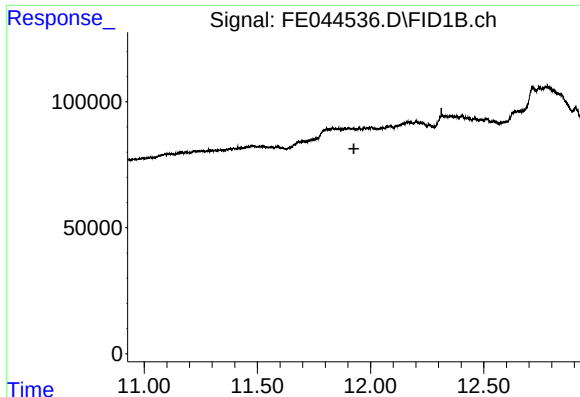

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.926 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

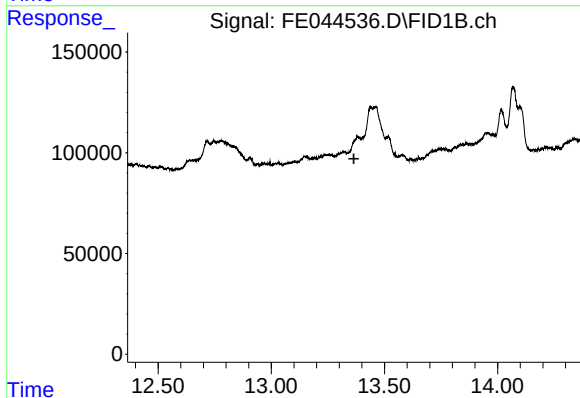


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.365 min
Response: 0
Conc: N.D.

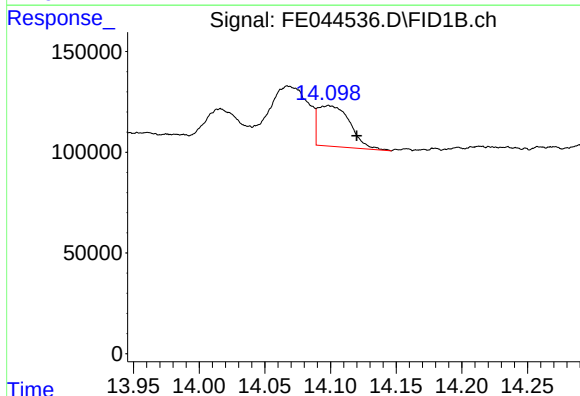


#13 n-Docosane (C22)

R.T.: 14.099 min
Delta R.T.: -0.021 min
Response: 345216
Conc: 2.24 ug/ml

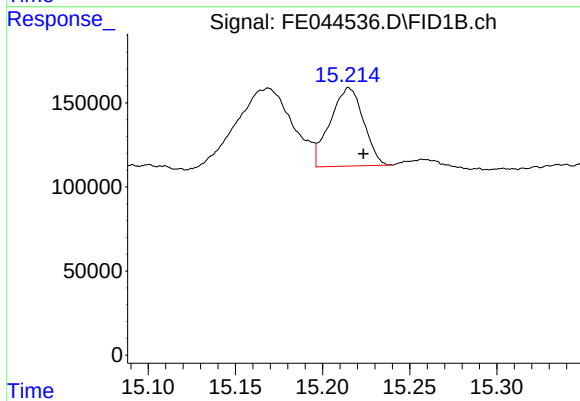

#14 n-Tetracosane (C24)


R.T.: 15.215 min
Delta R.T.: -0.008 min
Response: 622282
Conc: 4.12 ug/ml

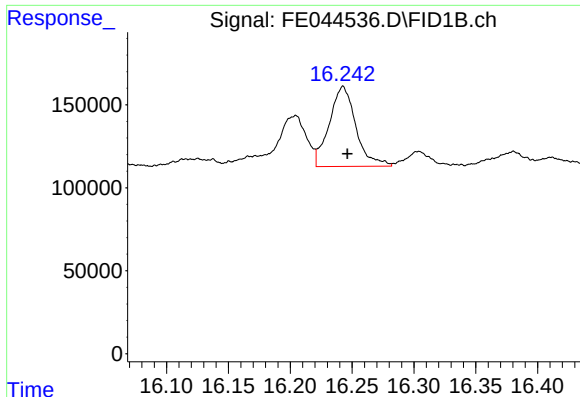

#15 n-Hexacosane (C26)


R.T.: 16.243 min
Delta R.T.: -0.004 min
Response: 722208
Conc: 4.91 ug/ml

Instrument :
FID_E
ClientSampleId :

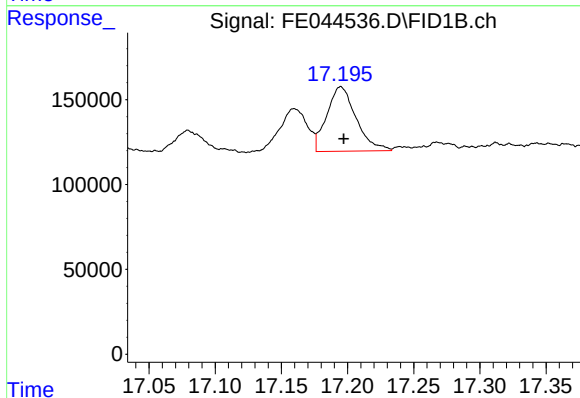


#16 n-Octacosane (C28)

R.T.: 17.195 min
Delta R.T.: -0.002 min
Response: 585412
Conc: 4.08 ug/ml

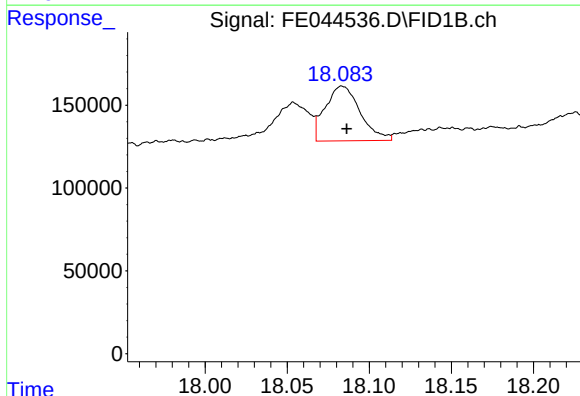


#17 n-Tricontane (C30)

R.T.: 18.084 min
Delta R.T.: -0.003 min
Response: 489681
Conc: 3.30 ug/ml

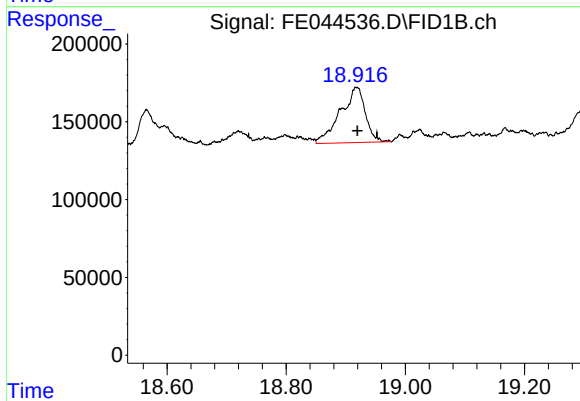

#18 n-Dotriacontane (C32)


R.T.: 18.918 min
Delta R.T.: -0.002 min
Response: 1034256
Conc: 6.99 ug/ml

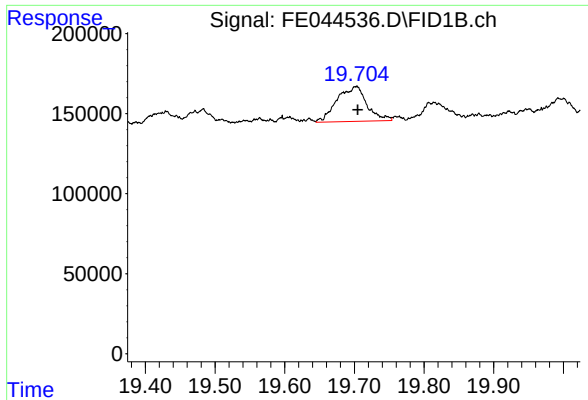

#19 n-Tetratriacontane (C34)

R.T.: 19.703 min
Delta R.T.: -0.002 min
Response: 652890
Conc: 4.47 ug/ml

Instrument :
FID_E
ClientSampleId :

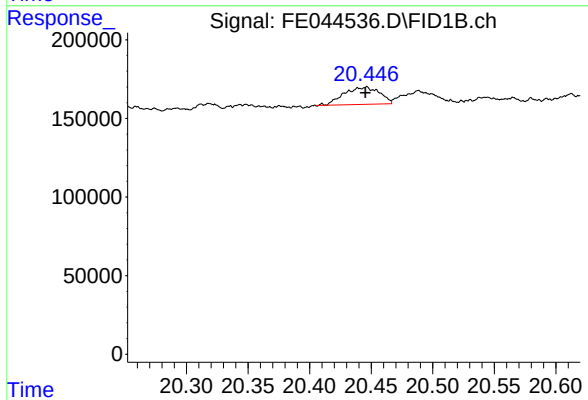

#20 n-Hexatriacontane (C36)

R.T.: 20.446 min
Delta R.T.: 0.000 min
Response: 220602
Conc: 1.52 ug/ml