

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100223AL\
 Data File : FE044557.D
 Signal(s) : FID1B.ch
 Acq On : 02 Oct 2023 19:20
 Operator : YP\AJ
 Sample : 04687-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 03 00:42:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092523.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 25 11:06:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.923	7500897	39.954 ug/ml
Spiked Amount 50.000		Recovery =	79.91%
12) S 1-chlorooctadecane (S...	13.362	5733090	42.142 ug/ml
Spiked Amount 50.000		Recovery =	84.28%
Target Compounds			
10) T n-Eicosane (C20)	12.970f	359527	2.235 ug/ml
13) T n-Docosane (C22)	14.136	189870	1.231 ug/ml
14) T n-Tetracosane (C24)	15.190	343645	2.273 ug/ml
16) T n-Octacosane (C28)	17.190	118560	0.827 ug/ml
17) T n-Tricontane (C30)	18.080	282358	1.905 ug/ml
18) T n-Dotriacontane (C32)	18.914	207440	1.401 ug/ml
19) T n-Tetratriacontane (C34)	19.697	57819	0.396 ug/ml
20) T n-Hexatriacontane (C36)	20.441	135716	0.936 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100223AL\
Data File : FE044557.D
Signal(s) : FID1B.ch
Acq On : 02 Oct 2023 19:20
Operator : YP\AJ
Sample : 04687-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 00:42:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 11:06:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

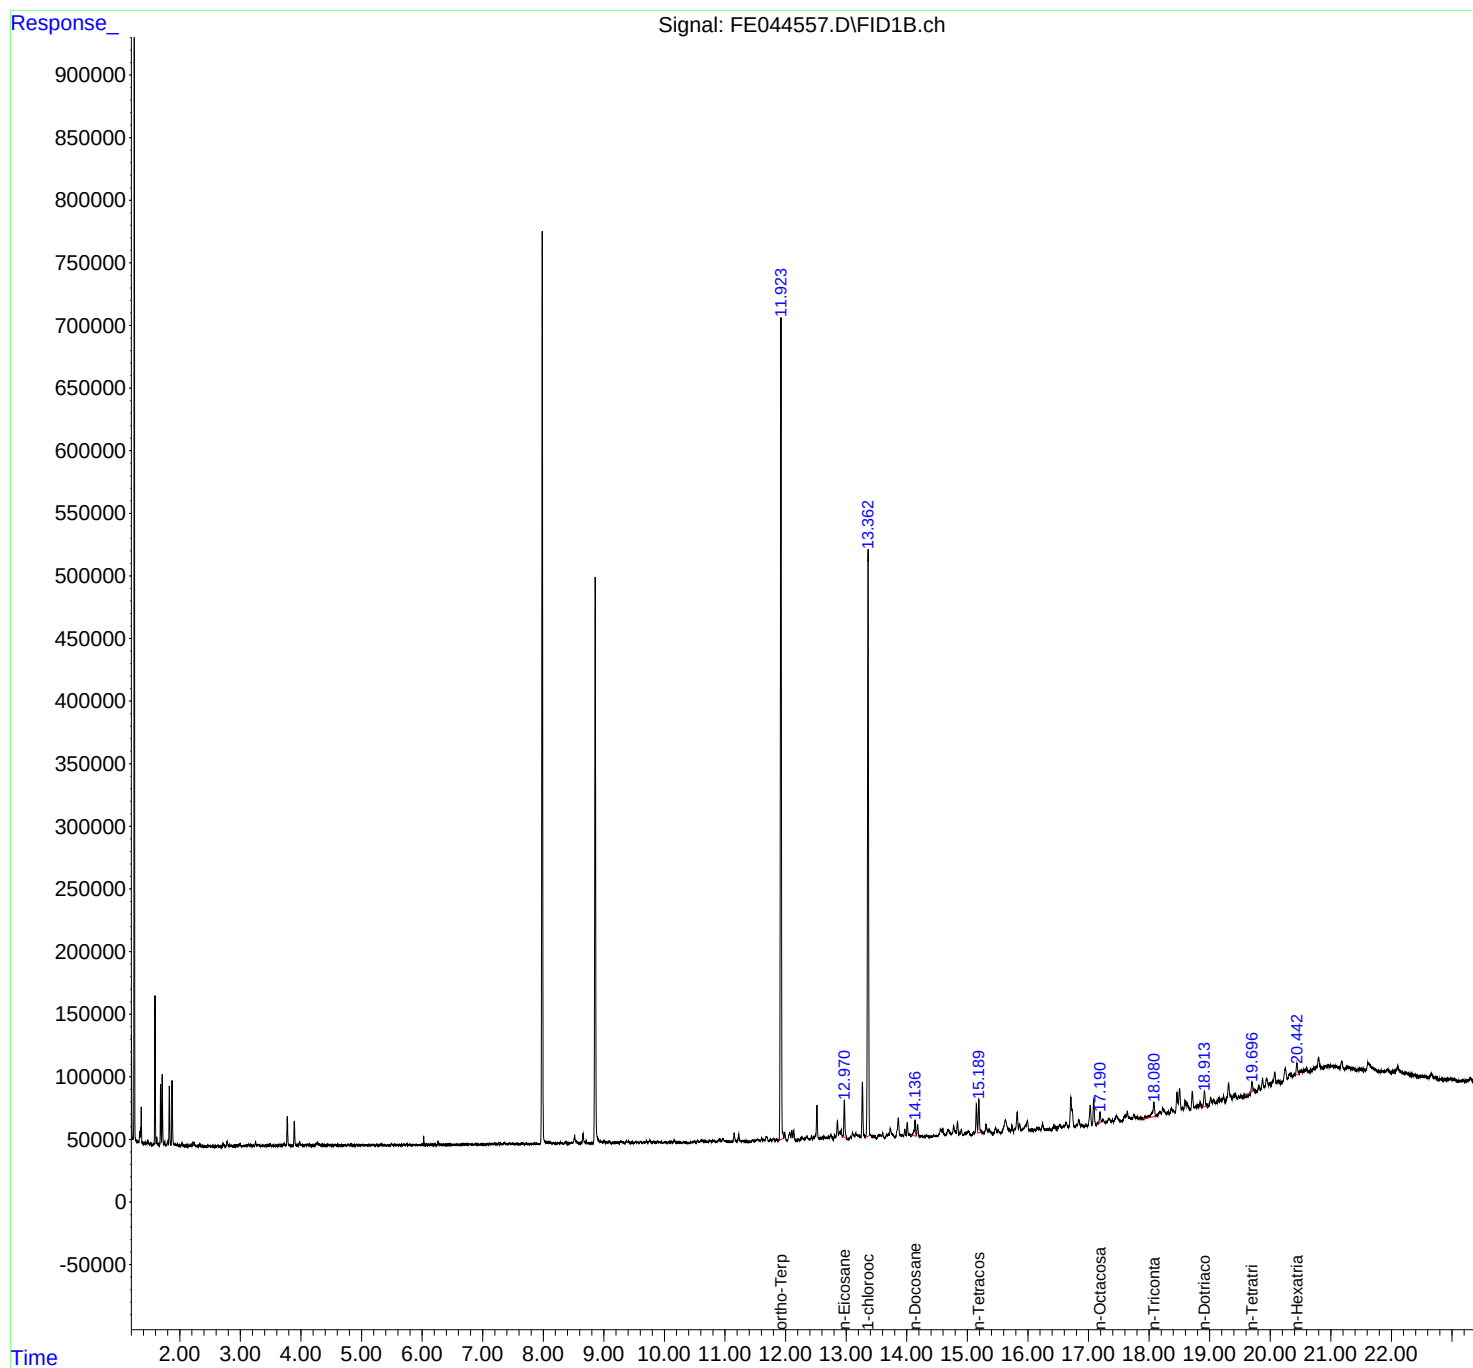


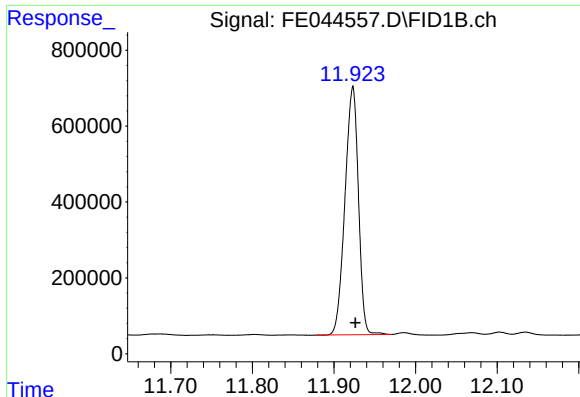

#9 ortho-Terphenyl (SURR)


R.T.: 11.923 min
Delta R.T.: -0.003 min
Response: 7500897
Conc: 39.95 ug/ml

Instrument :
FID_E
ClientSampleId :

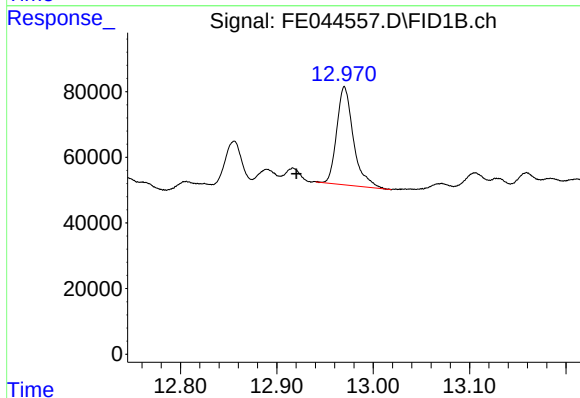


#10 n-Eicosane (C20)

R.T.: 12.970 min
Delta R.T.: 0.050 min
Response: 359527
Conc: 2.23 ug/ml

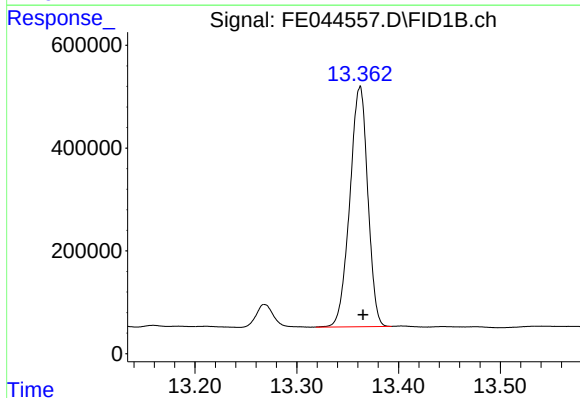


#12 1-chlorooctadecane (SURR)

R.T.: 13.362 min
Delta R.T.: -0.003 min
Response: 5733090
Conc: 42.14 ug/ml

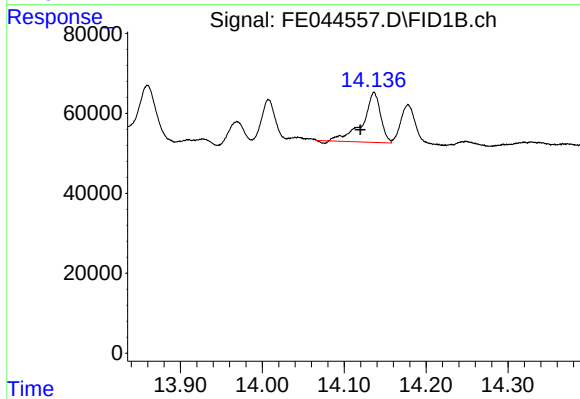

#13 n-Docosane (C22)


R.T.: 14.136 min
Delta R.T.: 0.017 min
Response: 189870
Conc: 1.23 ug/ml

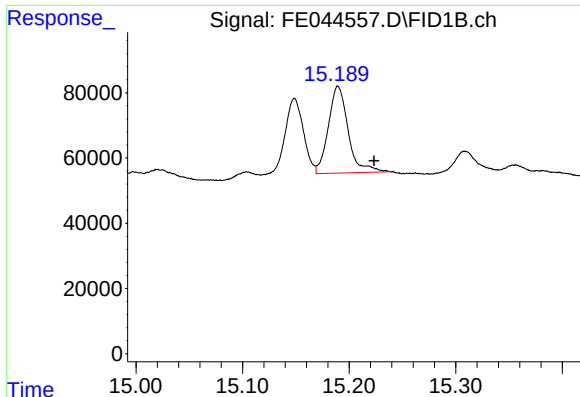

#14 n-Tetracosane (C24)


R.T.: 15.190 min
Delta R.T.: -0.034 min
Response: 343645
Conc: 2.27 ug/ml

Instrument :
FID_E
ClientSampleId :

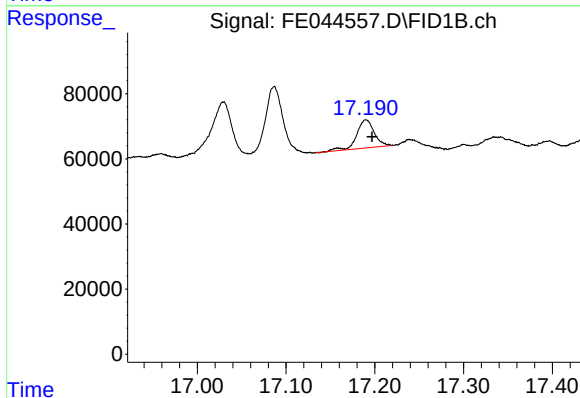


#16 n-Octacosane (C28)

R.T.: 17.190 min
Delta R.T.: -0.007 min
Response: 118560
Conc: 0.83 ug/ml

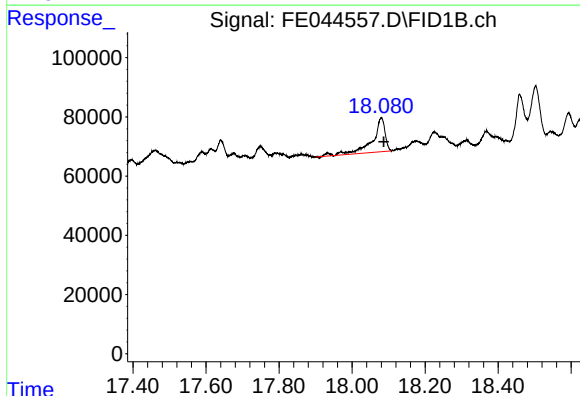


#17 n-Tricontane (C30)

R.T.: 18.080 min
Delta R.T.: -0.006 min
Response: 282358
Conc: 1.90 ug/ml

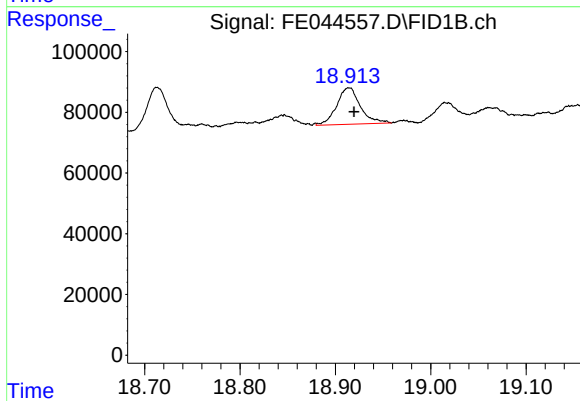

#18 n-Dotriacontane (C32)


R.T.: 18.914 min
Delta R.T.: -0.005 min
Response: 207440
Conc: 1.40 ug/ml

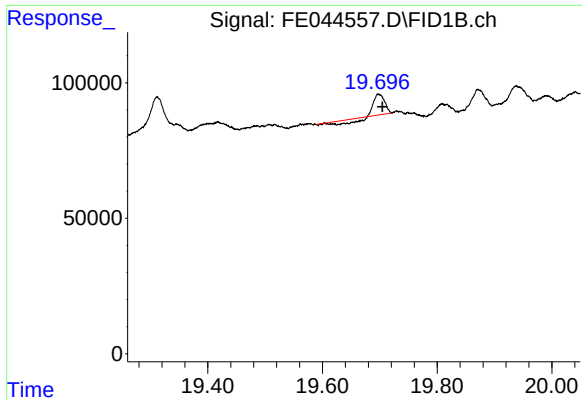

#19 n-Tetratriacontane (C34)

R.T.: 19.697 min
Delta R.T.: -0.008 min
Response: 57819
Conc: 0.40 ug/ml

Instrument :
FID_E
ClientSampleId :

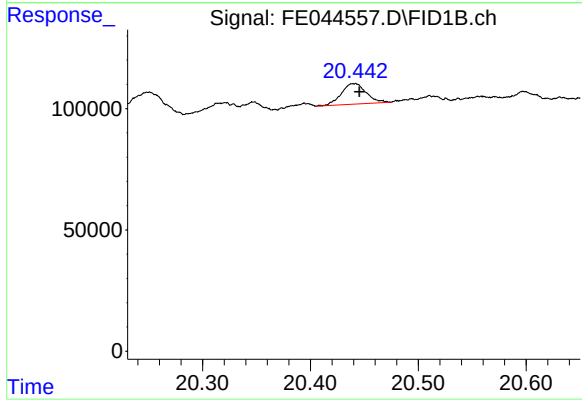

#20 n-Hexatriacontane (C36)

R.T.: 20.441 min
Delta R.T.: -0.005 min
Response: 135716
Conc: 0.94 ug/ml