

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100319\  
 Data File : FE030647.D  
 Signal(s) : FID1B.CH  
 Acq On : 03 Oct 2019 13:44  
 Operator : DD\AJ  
 Sample : K4660-01  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Oct 04 01:56:19 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE092419.M  
 Quant Title :  
 QLast Update : Wed Sep 25 02:50:34 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.675	4941250	15.938 ug/ml
Target Compounds			
4) N-TETRADECANE	8.276f	1965984	5.229 ug/ml
10) N-TETRACOSANE	14.876	294335	0.828 ug/ml
11) N-HEXACOSANE	15.899	594036	1.695 ug/ml
12) N-OCTACOSANE	16.852	677479	1.969 ug/ml
13) N-TRIACONTANE	17.740	981889	2.930 ug/ml
14) N-DOTRIACONTANE	18.573	879967	2.727 ug/ml
15) N-TETRATRIACONTANE	19.364	377157	1.208 ug/ml
16) N-HEXATRIACONTANE	20.110	783313	2.760 ug/ml
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100319\  
 Data File : FE030647.D  
 Signal(s) : FID1B.CH  
 Acq On : 03 Oct 2019 13:44  
 Operator : DD\AJ  
 Sample : K4660-01  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampled :

Integration File: autoint1.e  
 Quant Time: Oct 04 01:56:19 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE092419.M  
 Quant Title :  
 QLast Update : Wed Sep 25 02:50:34 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

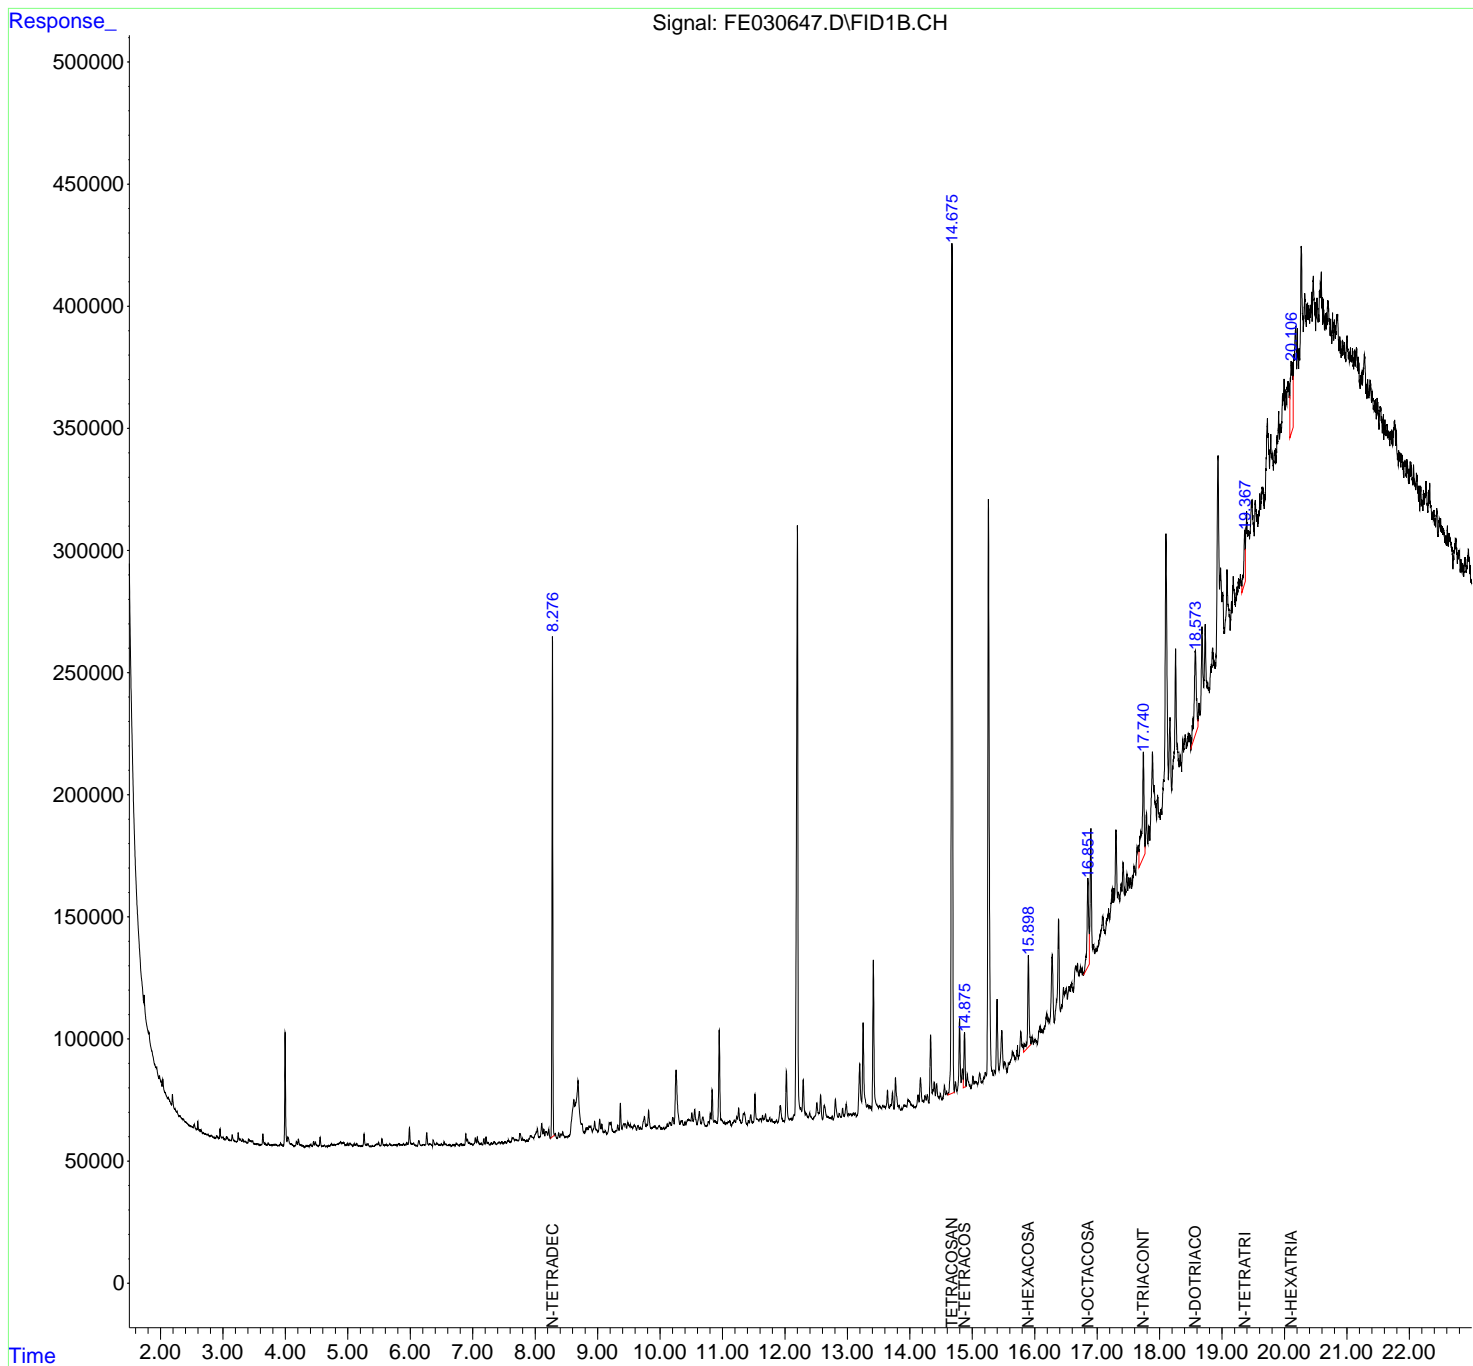

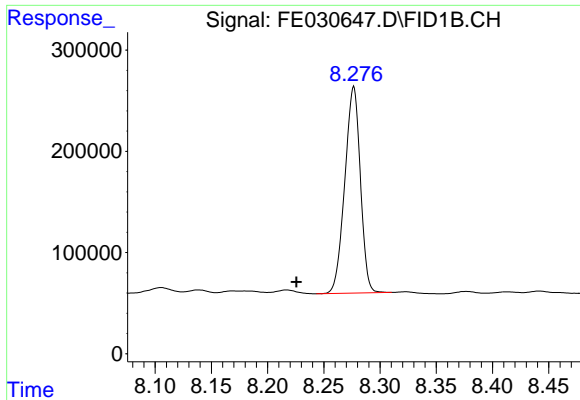


#4 N-TETRADECANE  
 R.T.: 8.276 min  
 Delta R.T.: 0.051 min  
 Response: 1965984  
 Conc: 5.23 ug/ml


Instrument :  
 FID\_E  
 ClientSampled :

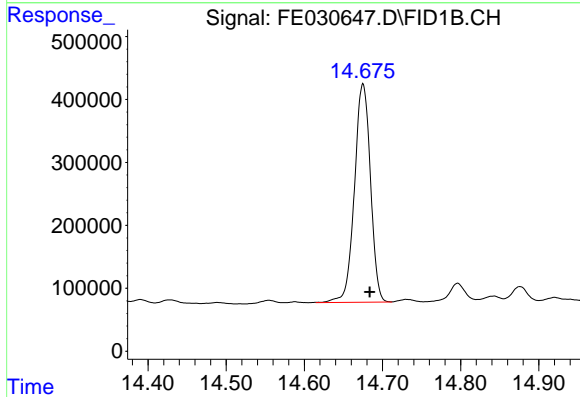


#9 TETRACOSANE-d50 (SURROGATE)  
 R.T.: 14.675 min  
 Delta R.T.: -0.009 min  
 Response: 4941250  
 Conc: 15.94 ug/ml

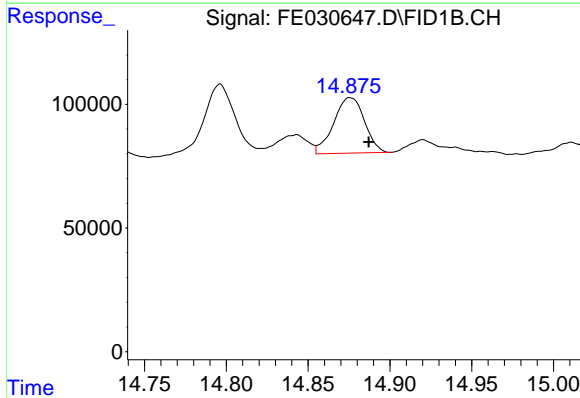

#10 N-TETRACOSANE  
 R.T.: 14.876 min  
 Delta R.T.: -0.011 min  
 Response: 294335  
 Conc: 0.83 ug/ml

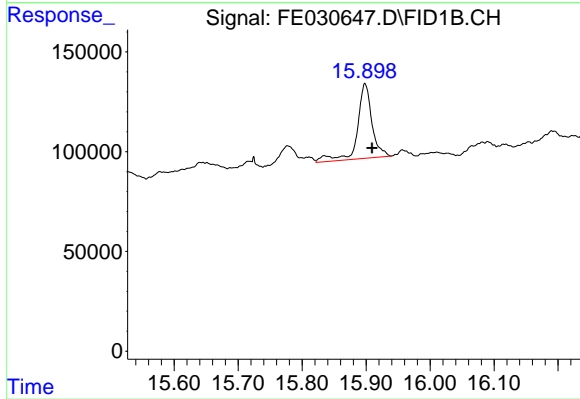


#11 N-HEXACOSANE  
 R.T.: 15.899 min  
 Delta R.T.: -0.011 min  
 Response: 594036  
 Conc: 1.70 ug/ml

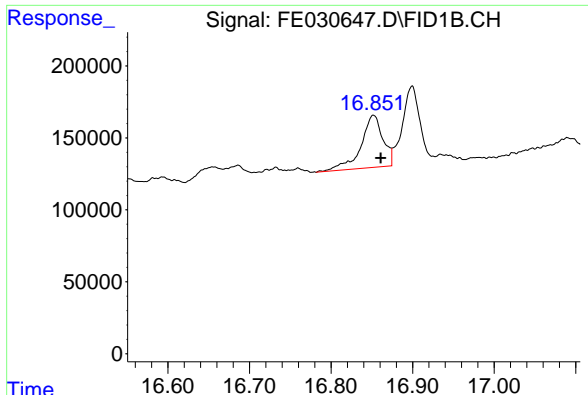

#12 N-OCTACOSANE


R.T.: 16.852 min  
 Delta R.T.: -0.009 min  
 Response: 677479  
 Conc: 1.97 ug/ml

Instrument :  
 FID\_E  
 ClientSampleId :

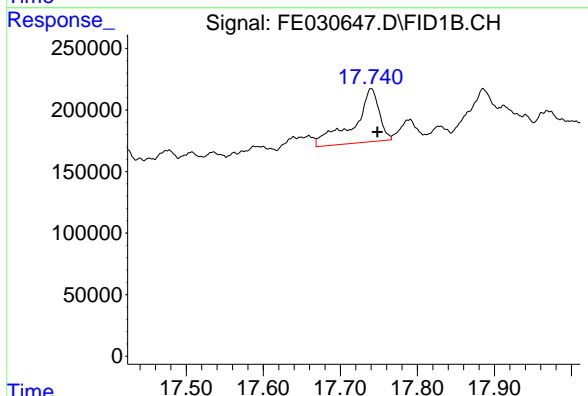


#13 N-TRIACONTANE

R.T.: 17.740 min  
 Delta R.T.: -0.008 min  
 Response: 981889  
 Conc: 2.93 ug/ml

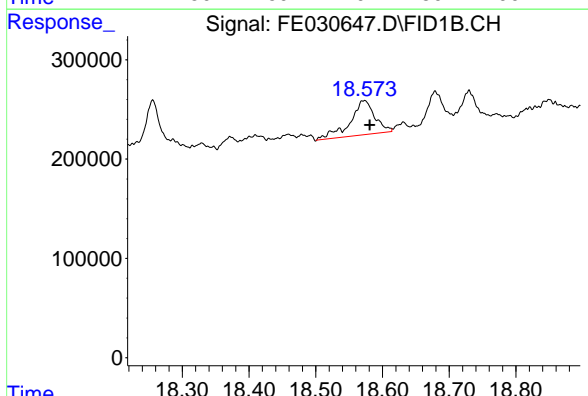


#14 N-DOTRIACONTANE

R.T.: 18.573 min  
 Delta R.T.: -0.008 min  
 Response: 879967  
 Conc: 2.73 ug/ml

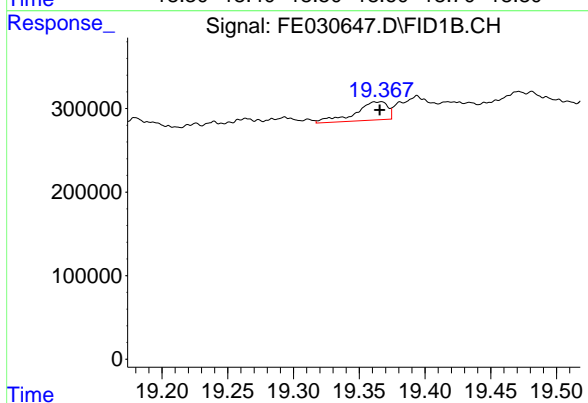

#15 N-TETRATRIACONTANE

R.T.: 19.364 min  
 Delta R.T.: -0.001 min  
 Response: 377157  
 Conc: 1.21 ug/ml

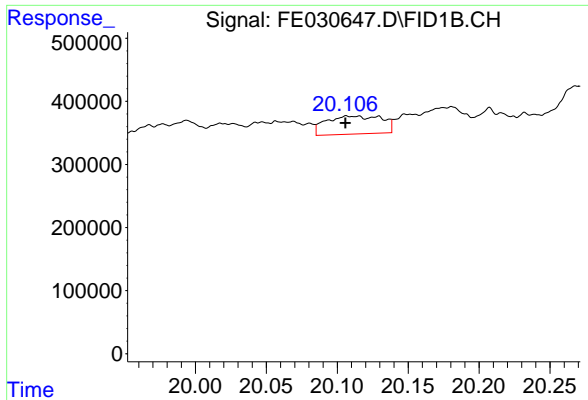

#16 N-HEXATRIACONTANE

R.T.: 20.110 min  
Delta R.T.: 0.004 min  
Response: 783313  
Conc: 2.76 ug/ml

Instrument :  
FID\_E  
ClientSampleId :