

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100319\
Data File : FE030648.D
Signal(s) : FID1B.CH
Acq On : 03 Oct 2019 14:17
Operator : DD\AJ
Sample : K4660-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TP-1

Integration File: autoint1.e
Quant Time: Oct 04 01:56:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
Quant Title :
QLast Update : Wed Sep 25 02:50:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.676	4141786	13.360 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100319\
Data File : FE030648.D
Signal(s) : FID1B.CH
Acq On : 03 Oct 2019 14:17
Operator : DD\AJ
Sample : K4660-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TP-1

Integration File: autoint1.e
Quant Time: Oct 04 01:56:31 2019
Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
Quant Title :
QLast Update : Wed Sep 25 02:50:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

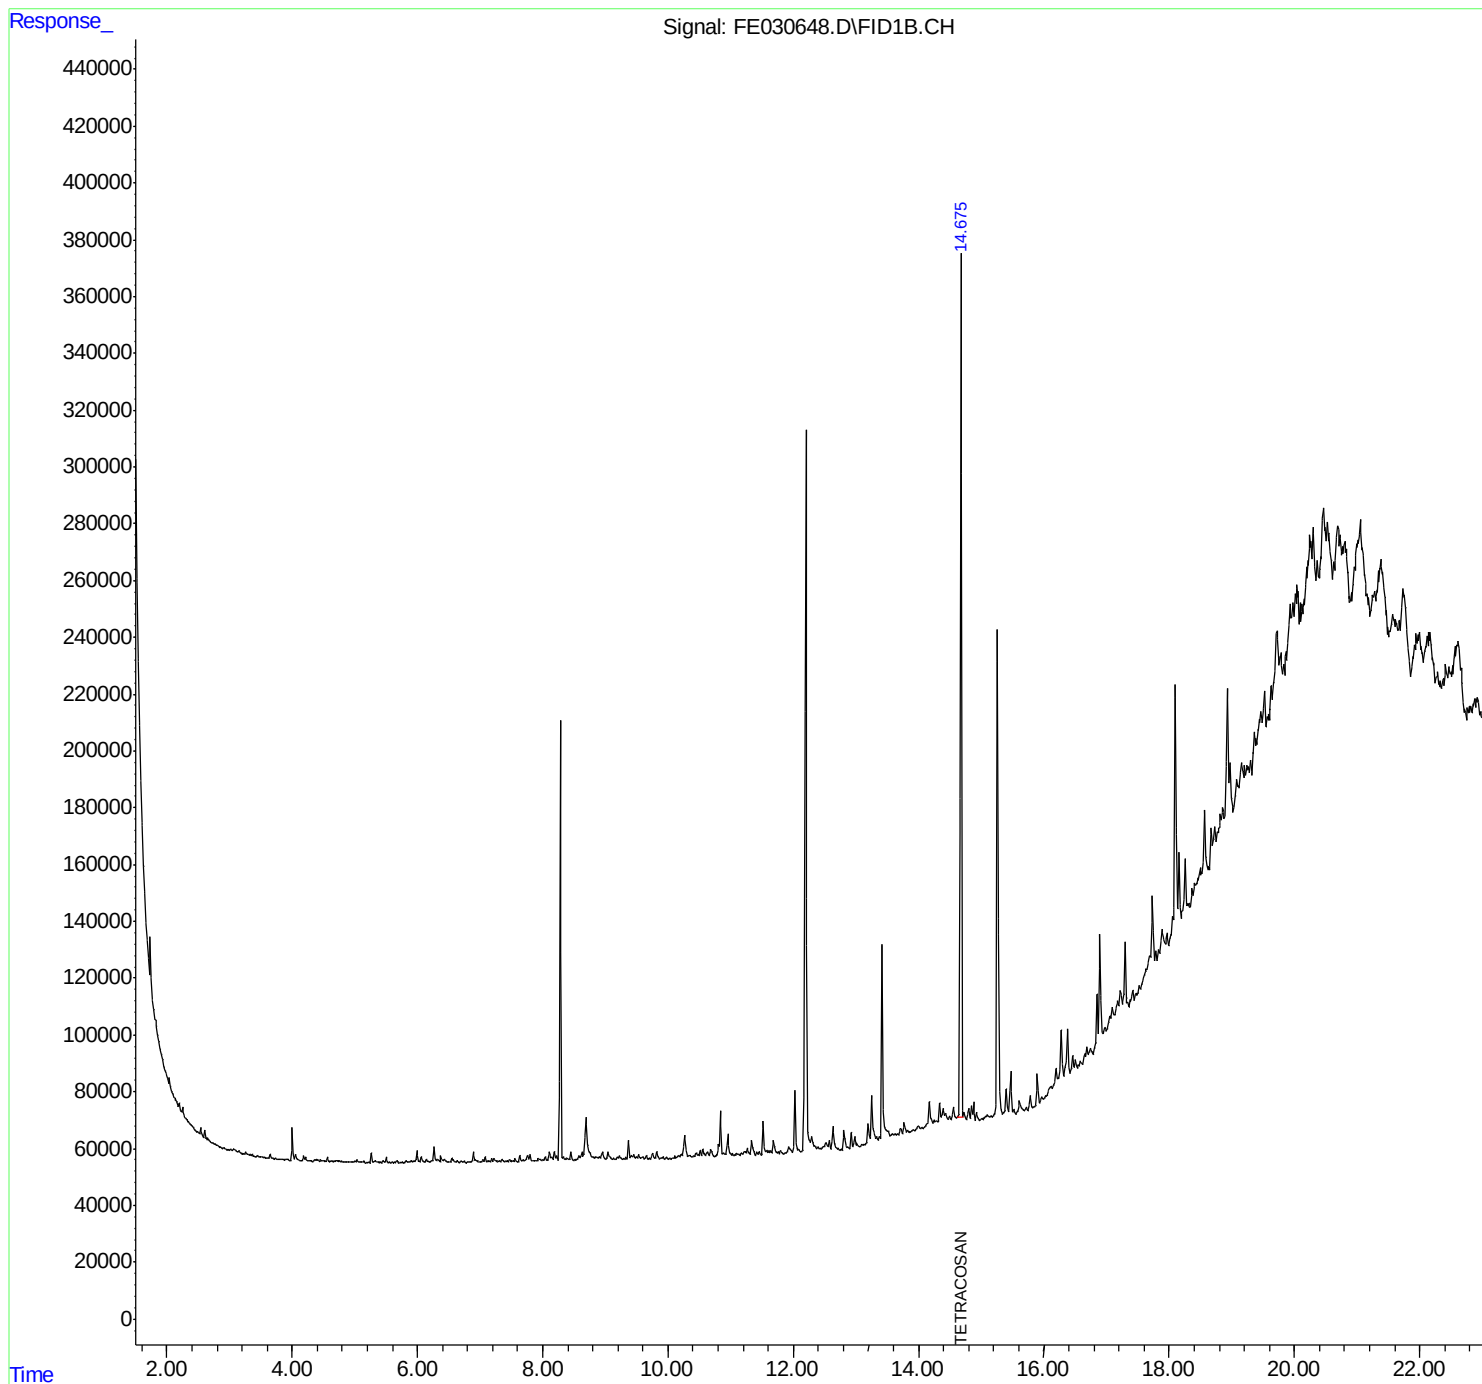

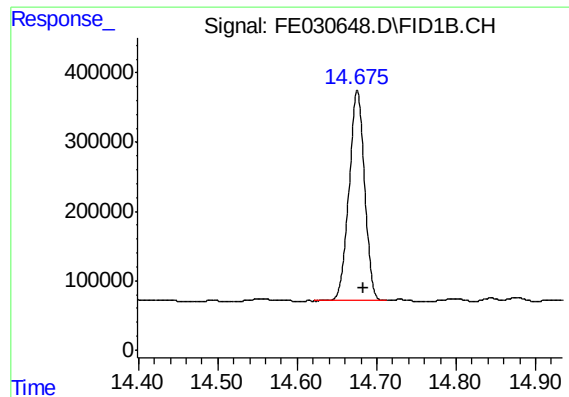

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.676 min
Delta R.T.: -0.008 min
Response: 4141786
Conc: 13.36 ug/ml

Instrument :
FID_E
ClientSampleId :
TP-1