

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100319\
 Data File : FE030657.D
 Signal(s) : FID1B.CH
 Acq On : 03 Oct 2019 19:17
 Operator : DD\AJ
 Sample : PB123592BS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 PB123592BS

Integration File: autoint1.e
 Quant Time: Oct 04 01:58:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
 Quant Title :
 QLast Update : Wed Sep 25 02:50:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.683	8627308	27.828 ug/ml
Target Compounds			
2) N-DECANE	4.415	9640116	25.256 ug/ml
3) N-DODECANE	6.430	9901302	25.870 ug/ml
4) N-TETRADECANE	8.227	9772198	25.990 ug/ml
5) N-HEXADECANE	9.829	9808476	26.272 ug/ml
6) N-OCTADECANE	11.272	9467644	25.834 ug/ml
7) N-EICOSANE	12.583	9265370	25.395 ug/ml
8) N-DOCOSANE	13.783	9202078	25.639 ug/ml
10) N-TETRACOSANE	14.887	9642744	27.121 ug/ml
11) N-HEXACOSANE	15.909	8917240	25.448 ug/ml
12) N-OCTACOSANE	16.860	8925522	25.936 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100319\
Data File : FE030657.D
Signal(s) : FID1B.CH
Acq On : 03 Oct 2019 19:17
Operator : DD\AJ
Sample : PB123592BS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB123592BS

Integration File: autoint1.e
Quant Time: Oct 04 01:58:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
Quant Title :
QLast Update : Wed Sep 25 02:50:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

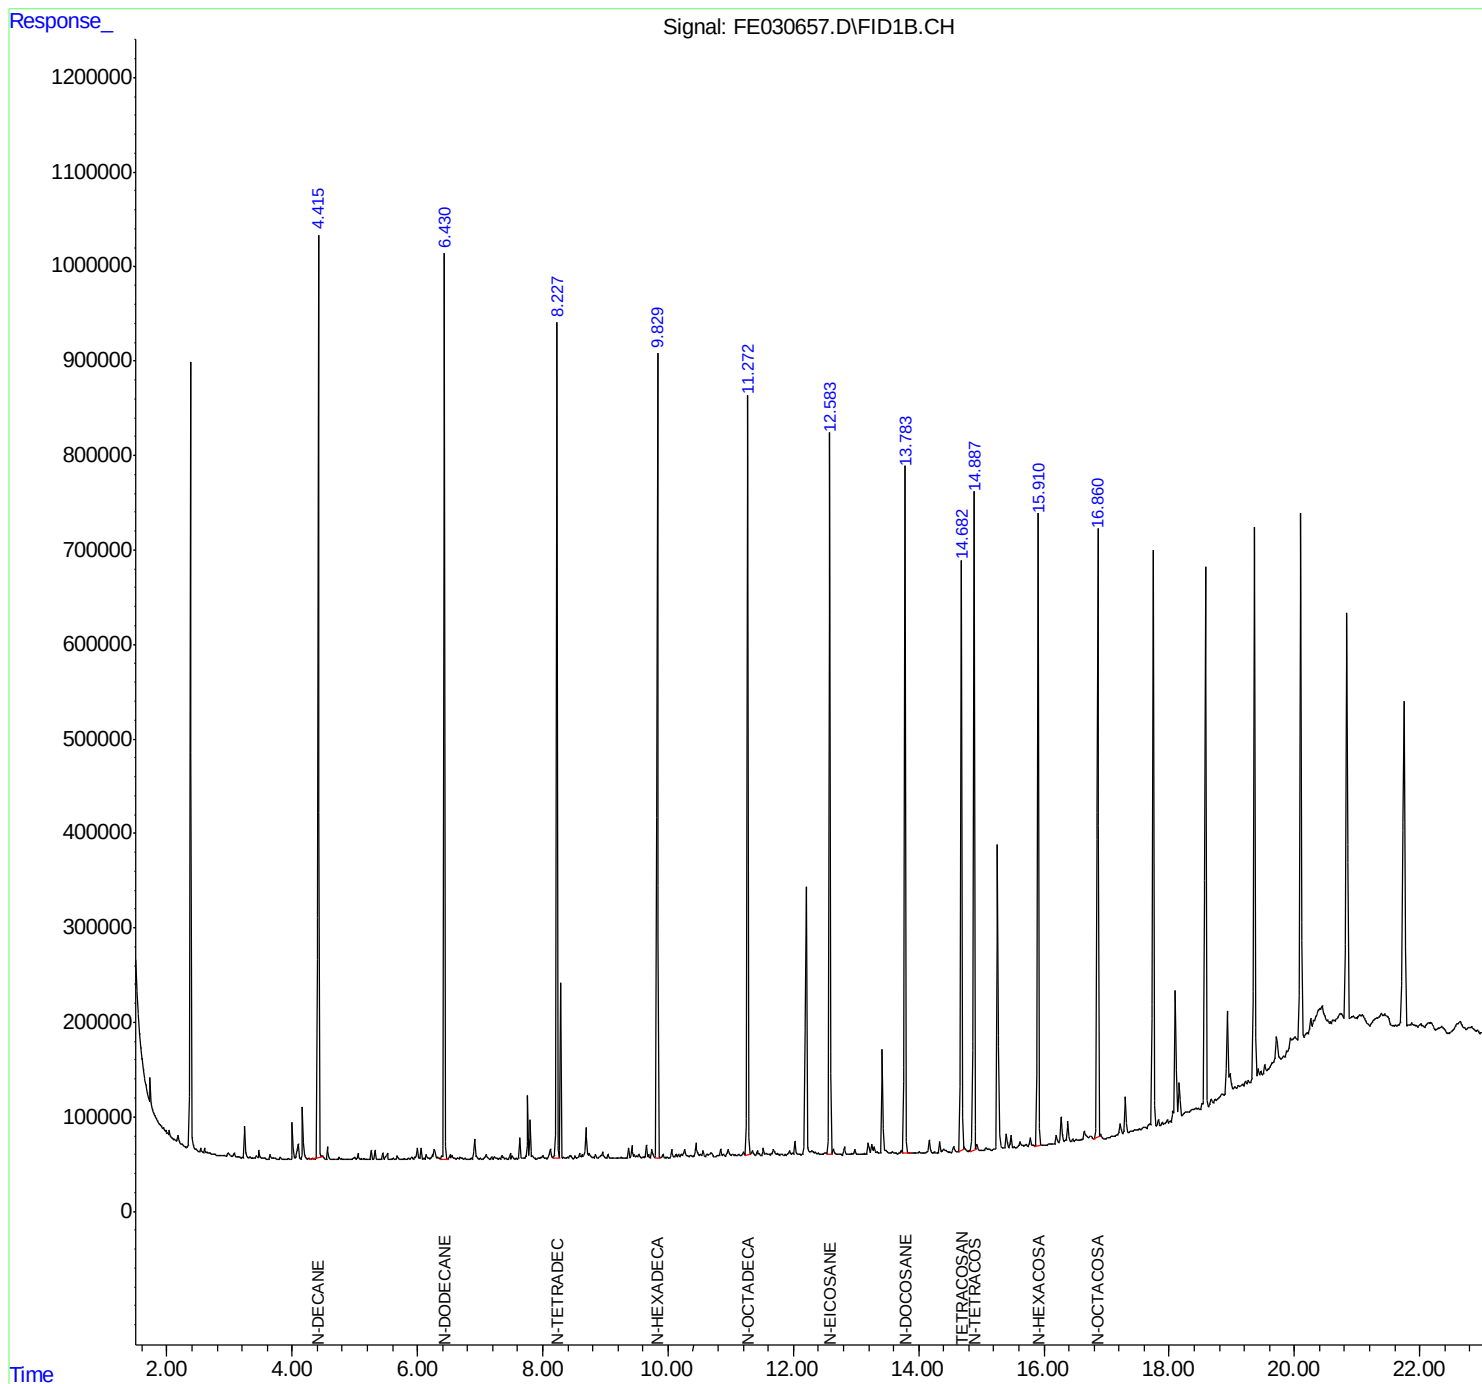


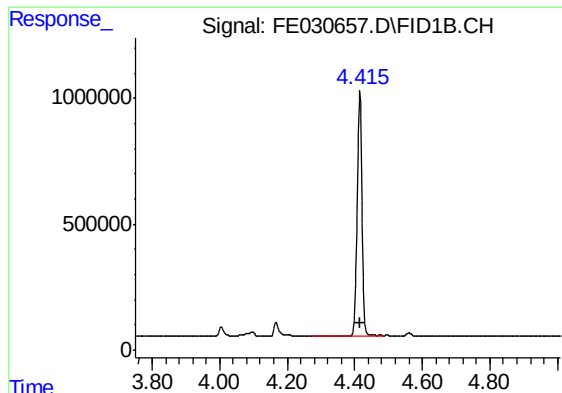

#2 N-DECANE


R.T.: 4.415 min
Delta R.T.: -0.002 min
Response: 9640116
Conc: 25.26 ug/ml

Instrument :
FID_E
ClientSampleId :
PB123592BS

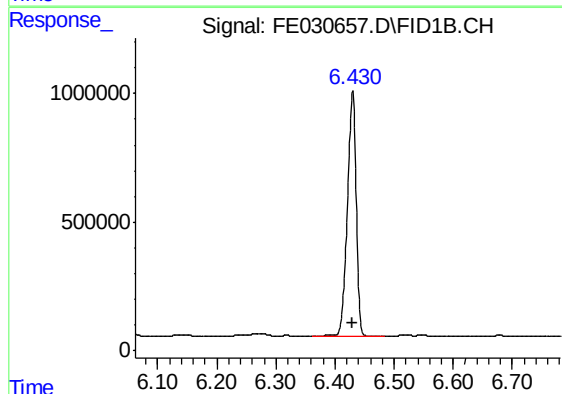


#3 N-DODECANE

R.T.: 6.430 min
Delta R.T.: 0.000 min
Response: 9901302
Conc: 25.87 ug/ml

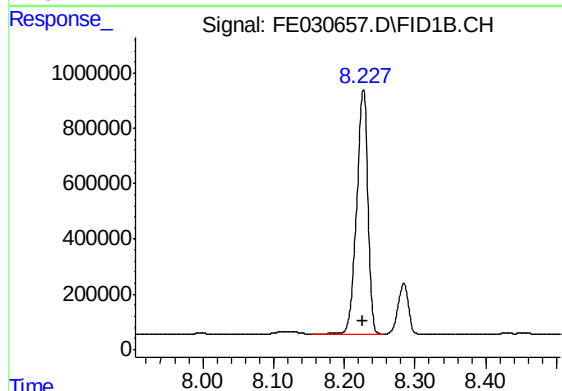


#4 N-TETRADECANE

R.T.: 8.227 min
Delta R.T.: 0.001 min
Response: 9772198
Conc: 25.99 ug/ml

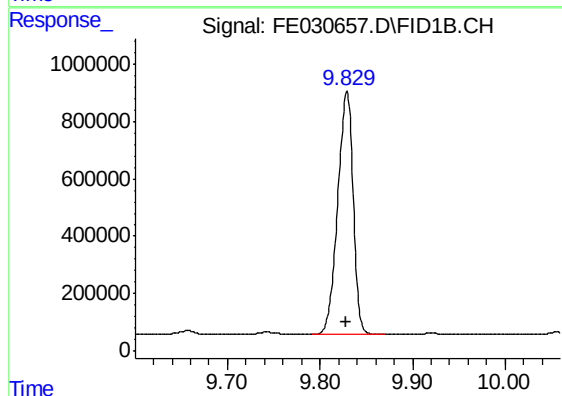

#5 N-HEXADECANE


R.T.: 9.829 min
Delta R.T.: 0.000 min
Response: 9808476
Conc: 26.27 ug/ml

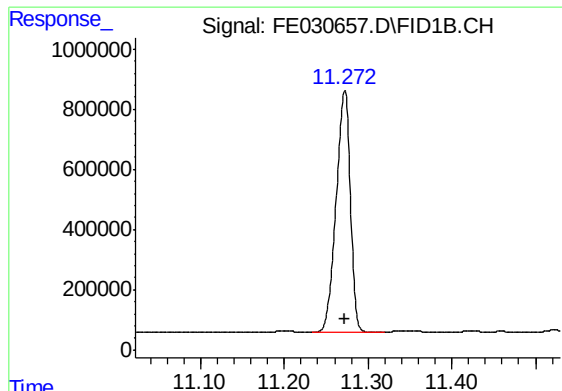

#6 N-OCTADECANE


R.T.: 11.272 min
Delta R.T.: 0.000 min
Response: 9467644
Conc: 25.83 ug/ml

Instrument :
FID_E
ClientSampleId :
PB123592BS

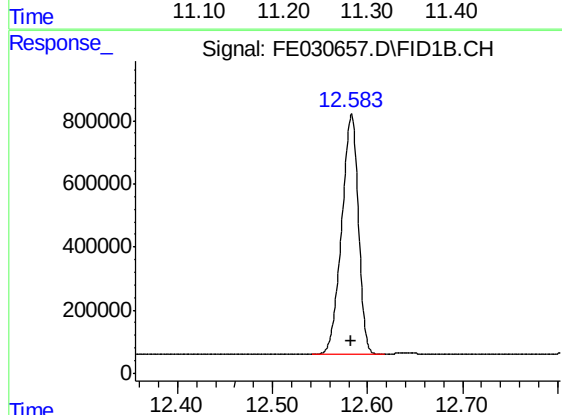


#7 N-EICOSANE

R.T.: 12.583 min
Delta R.T.: 0.000 min
Response: 9265370
Conc: 25.39 ug/ml

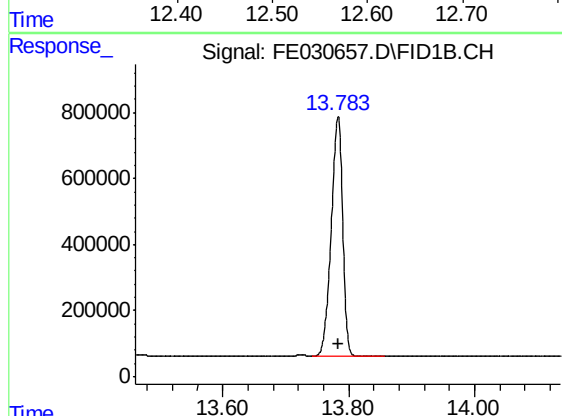


#8 N-DOCOSANE

R.T.: 13.783 min
Delta R.T.: 0.000 min
Response: 9202078
Conc: 25.64 ug/ml

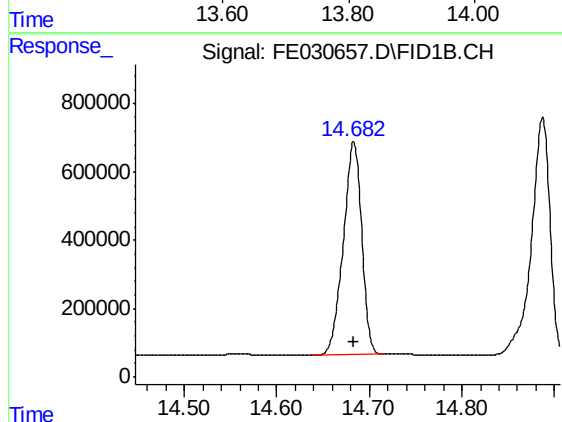

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.683 min
Delta R.T.: 0.000 min
Response: 8627308
Conc: 27.83 ug/ml

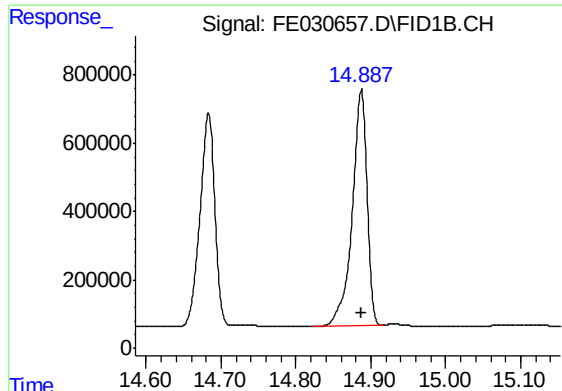

#10 N-TETRACOSANE


R.T.: 14.887 min
Delta R.T.: 0.000 min
Response: 9642744
Conc: 27.12 ug/ml

Instrument :
FID_E
ClientSampleId :
PB123592BS

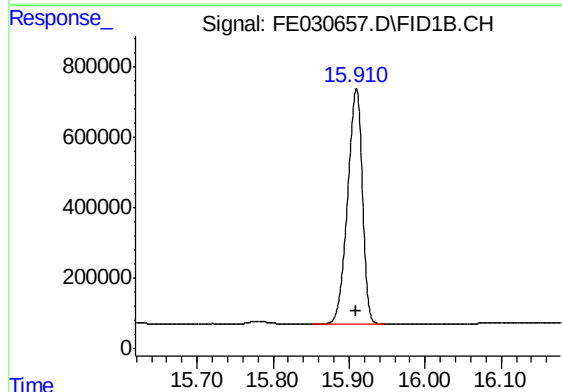

#11 N-HEXACOSANE

R.T.: 15.909 min
Delta R.T.: 0.000 min
Response: 8917240
Conc: 25.45 ug/ml

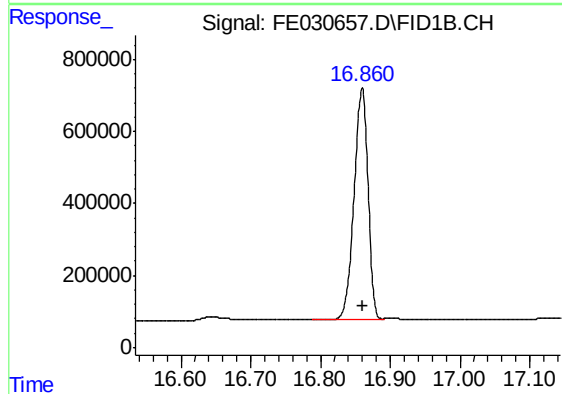

#12 N-OCTACOSANE

R.T.: 16.860 min
Delta R.T.: -0.001 min
Response: 8925522
Conc: 25.94 ug/ml