

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100323\
Data File : FE044568.D
Signal(s) : FID1B.ch
Acq On : 03 Oct 2023 09:59
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 03 13:25:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100323.M
Quant Title :
QLast Update : Tue Oct 03 12:58:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.015	2420038	16.495 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100323\
Data File : FE044568.D
Signal(s) : FID1B.ch
Acq On : 03 Oct 2023 09:59
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 03 13:25:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100323.M
Quant Title :
QLast Update : Tue Oct 03 12:58:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

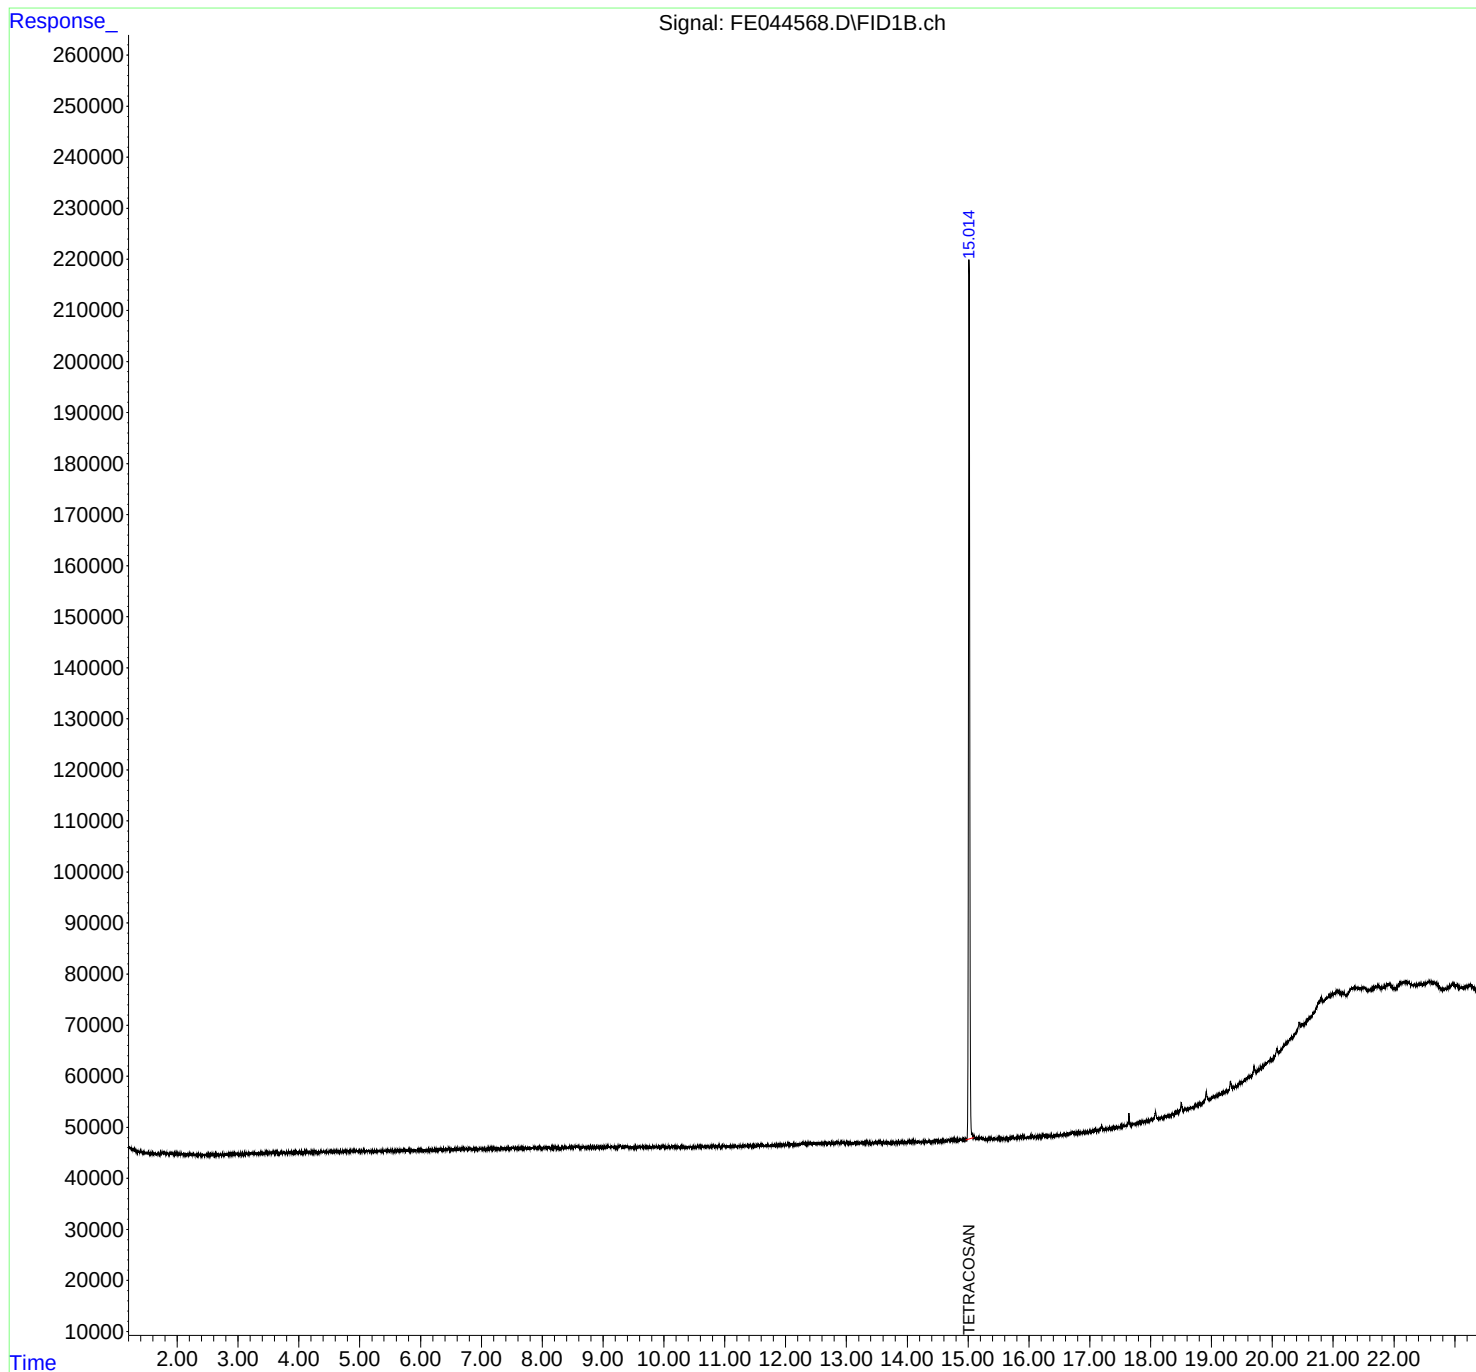

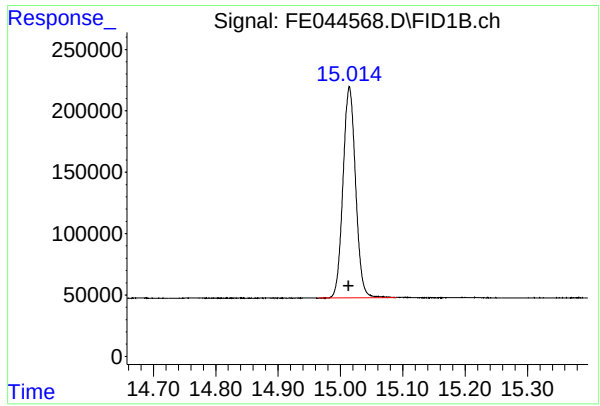

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.015 min

Delta R.T.: 0.001 min

Response: 2420038

Conc: 16.50 ug/ml

Instrument :

FID_E

ClientSampleId :

I.BLK