

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100425AL\
 Data File : FC069932.D
 Signal(s) : FID1A.ch
 Acq On : 03 Oct 2025 17:57
 Operator : YP/AJ
 Sample : Q3263-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 06 01:27:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092325.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 23 14:56:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.083	6396836	40.507 ug/ml
Spiked Amount 50.000		Recovery =	81.01%
Target Compounds			
6) T n-Tetradecane (C14)	8.275	65965	0.445 ug/ml
8) T n-Octadecane (C18)	11.320	39241	0.220 ug/ml
10) T n-Eicosane (C20)	12.631	45043	0.250 ug/ml
13) T n-Docosane (C22)	13.830	41111	0.226 ug/ml
14) T n-Tetracosane (C24)	14.934	50160	0.273 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100425AL\
Data File : FC069932.D
Signal(s) : FID1A.ch
Acq On : 03 Oct 2025 17:57
Operator : YP/AJ
Sample : Q3263-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 06 01:27:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092325.M
Quant Title : GC Extractables
QLast Update : Tue Sep 23 14:56:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

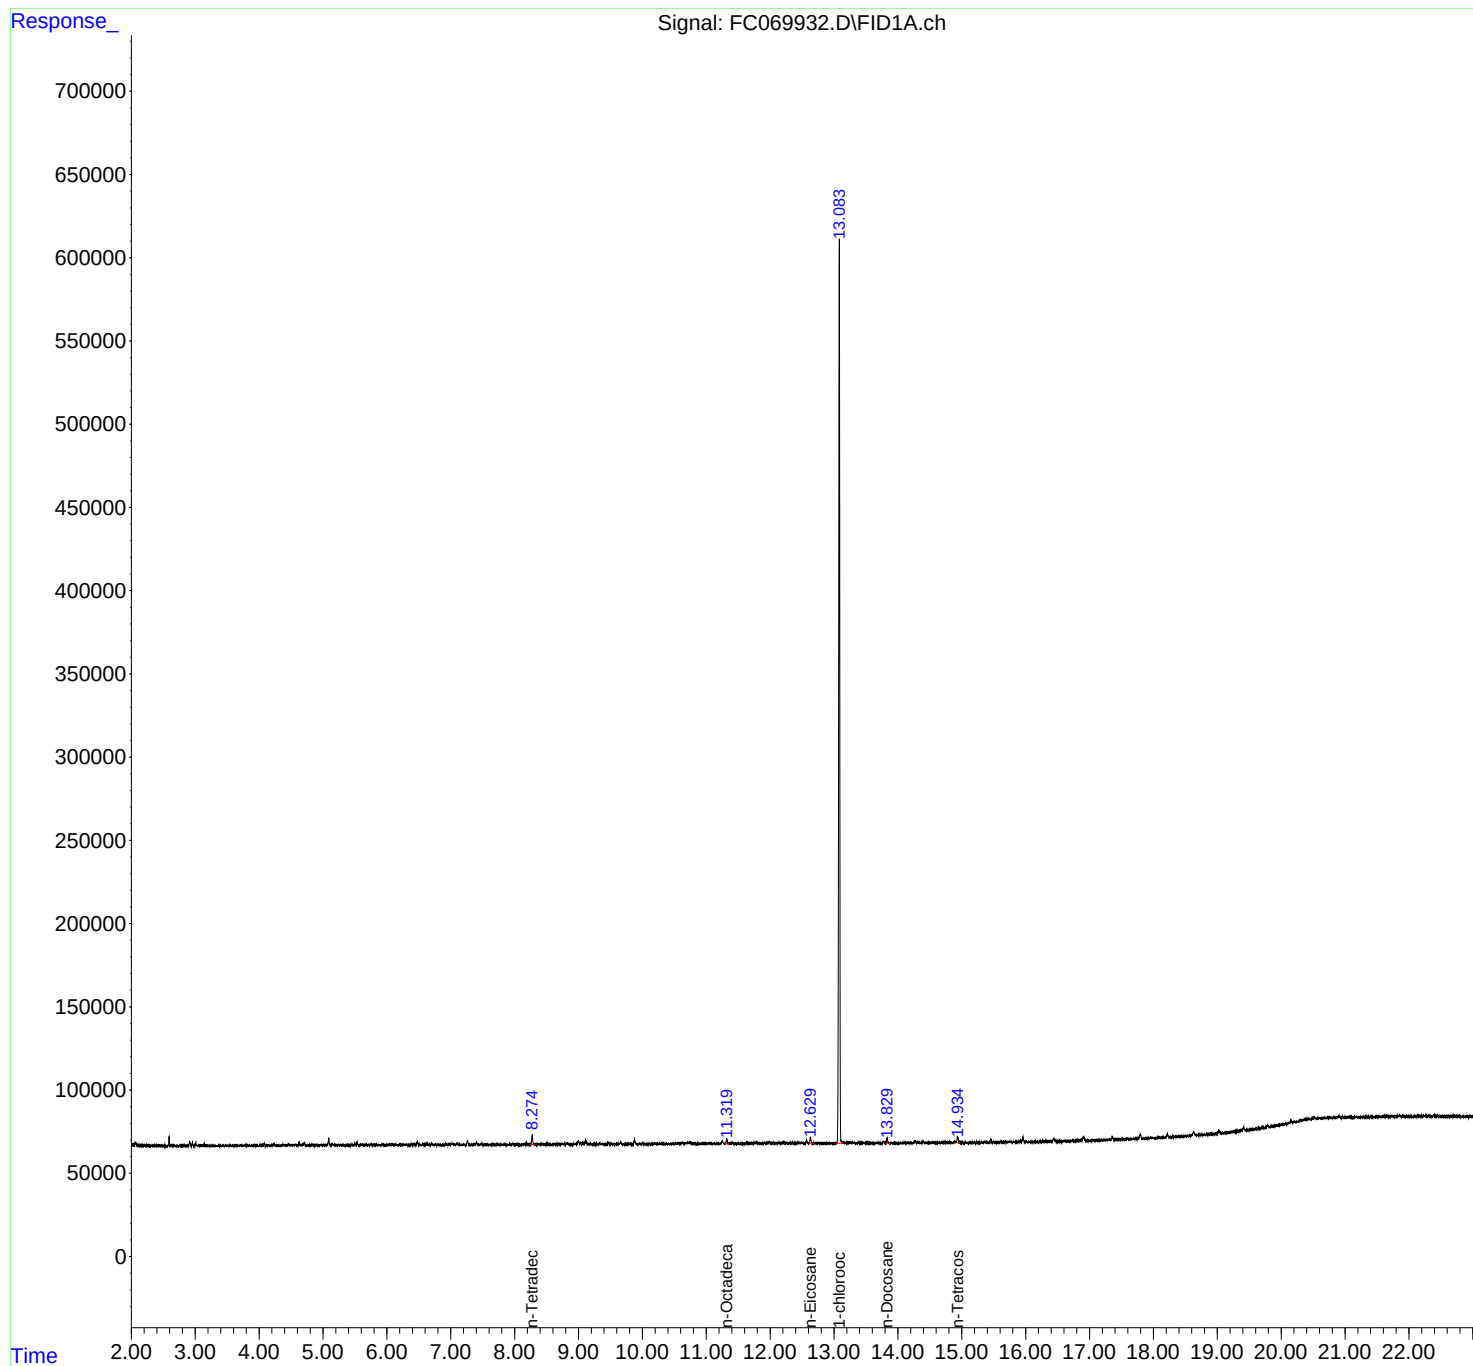


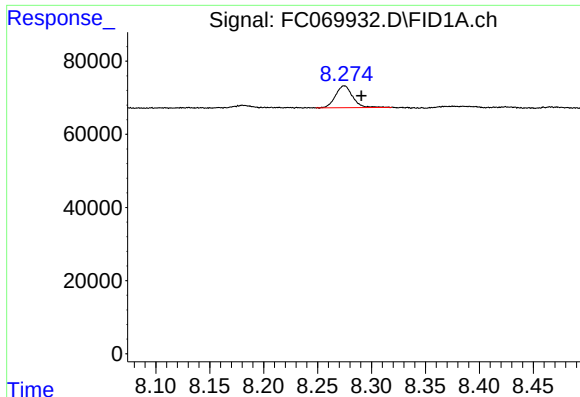

#6 n-Tetradecane (C14)


R.T.: 8.275 min
Delta R.T.: -0.016 min
Response: 65965
Conc: 0.44 ug/ml

Instrument :
FID_E
ClientSampleId :

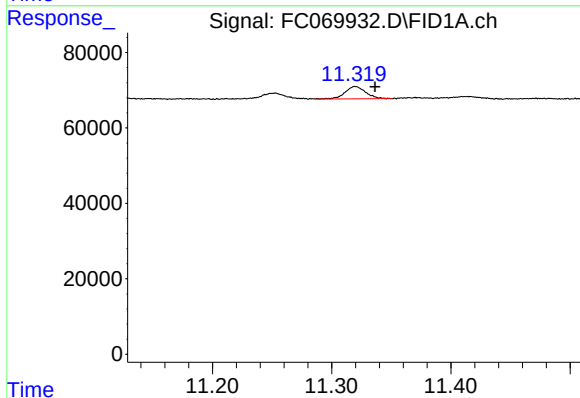


#8 n-Octadecane (C18)

R.T.: 11.320 min
Delta R.T.: -0.017 min
Response: 39241
Conc: 0.22 ug/ml

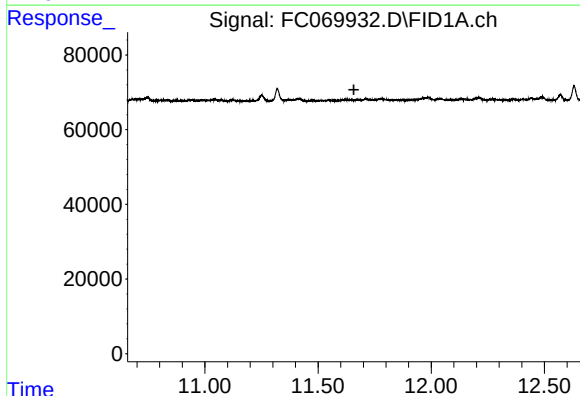


#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.658 min
Response: 0
Conc: N.D.

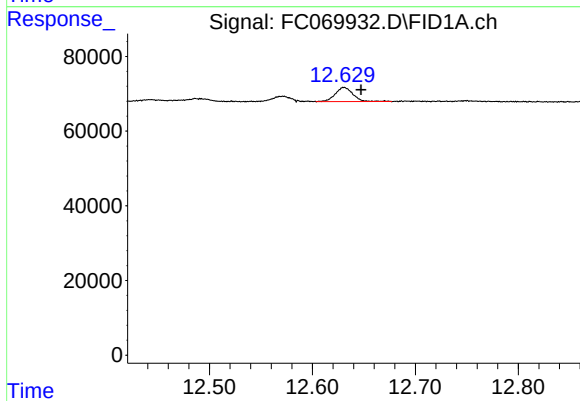

#10 n-Eicosane (C20)


R.T.: 12.631 min
Delta R.T.: -0.017 min
Response: 45043
Conc: 0.25 ug/ml

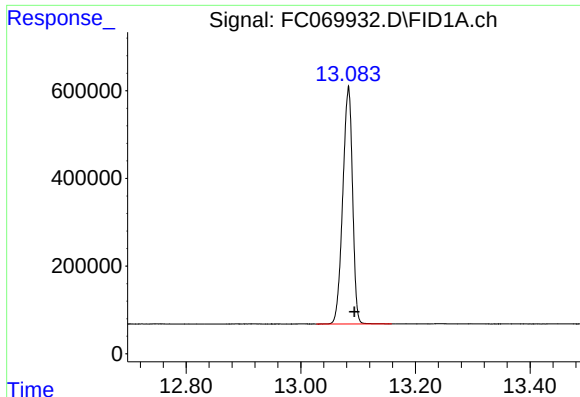

#12 1-chlorooctadecane (SURR)


R.T.: 13.083 min
Delta R.T.: -0.011 min
Response: 6396836
Conc: 40.51 ug/ml

Instrument :
FID_E
ClientSampleId :

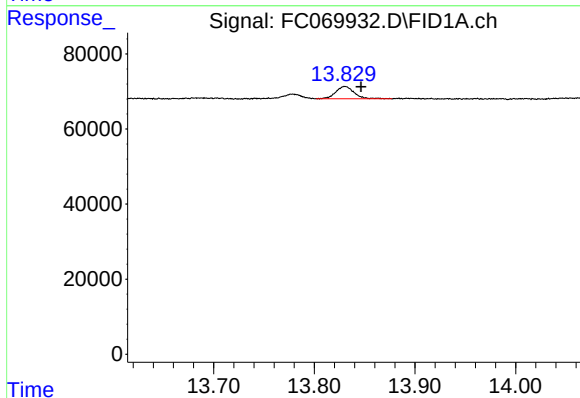

#13 n-Docosane (C22)

R.T.: 13.830 min
Delta R.T.: -0.016 min
Response: 41111
Conc: 0.23 ug/ml

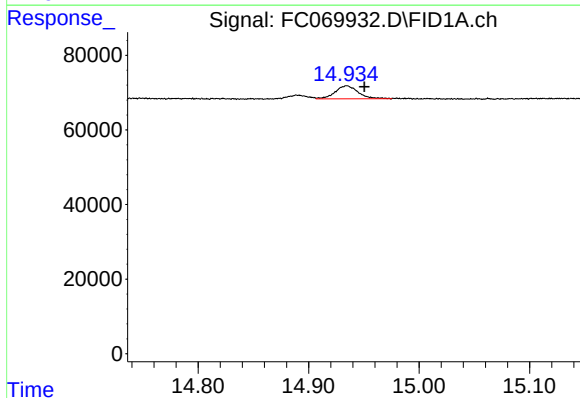

#14 n-Tetracosane (C24)

R.T.: 14.934 min
Delta R.T.: -0.016 min
Response: 50160
Conc: 0.27 ug/ml