

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100419\
 Data File : FE030664.D
 Signal(s) : FID1B.CH
 Acq On : 04 Oct 2019 10:56
 Operator : DD\AJ
 Sample : PB123592BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 04 21:54:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
 Quant Title :
 QLast Update : Wed Sep 25 02:50:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.679	6853473	22.106 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.739	252635	0.754 ug/ml
14) N-DOTRIACONTANE	18.571	254953	0.790 ug/ml
15) N-TETRATRIACONTANE	19.355	183570	0.588 ug/ml
16) N-HEXATRIACONTANE	20.095	161602	0.569 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100419\
Data File : FE030664.D
Signal(s) : FID1B.CH
Acq On : 04 Oct 2019 10:56
Operator : DD\AJ
Sample : PB123592BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 04 21:54:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
Quant Title :
QLast Update : Wed Sep 25 02:50:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

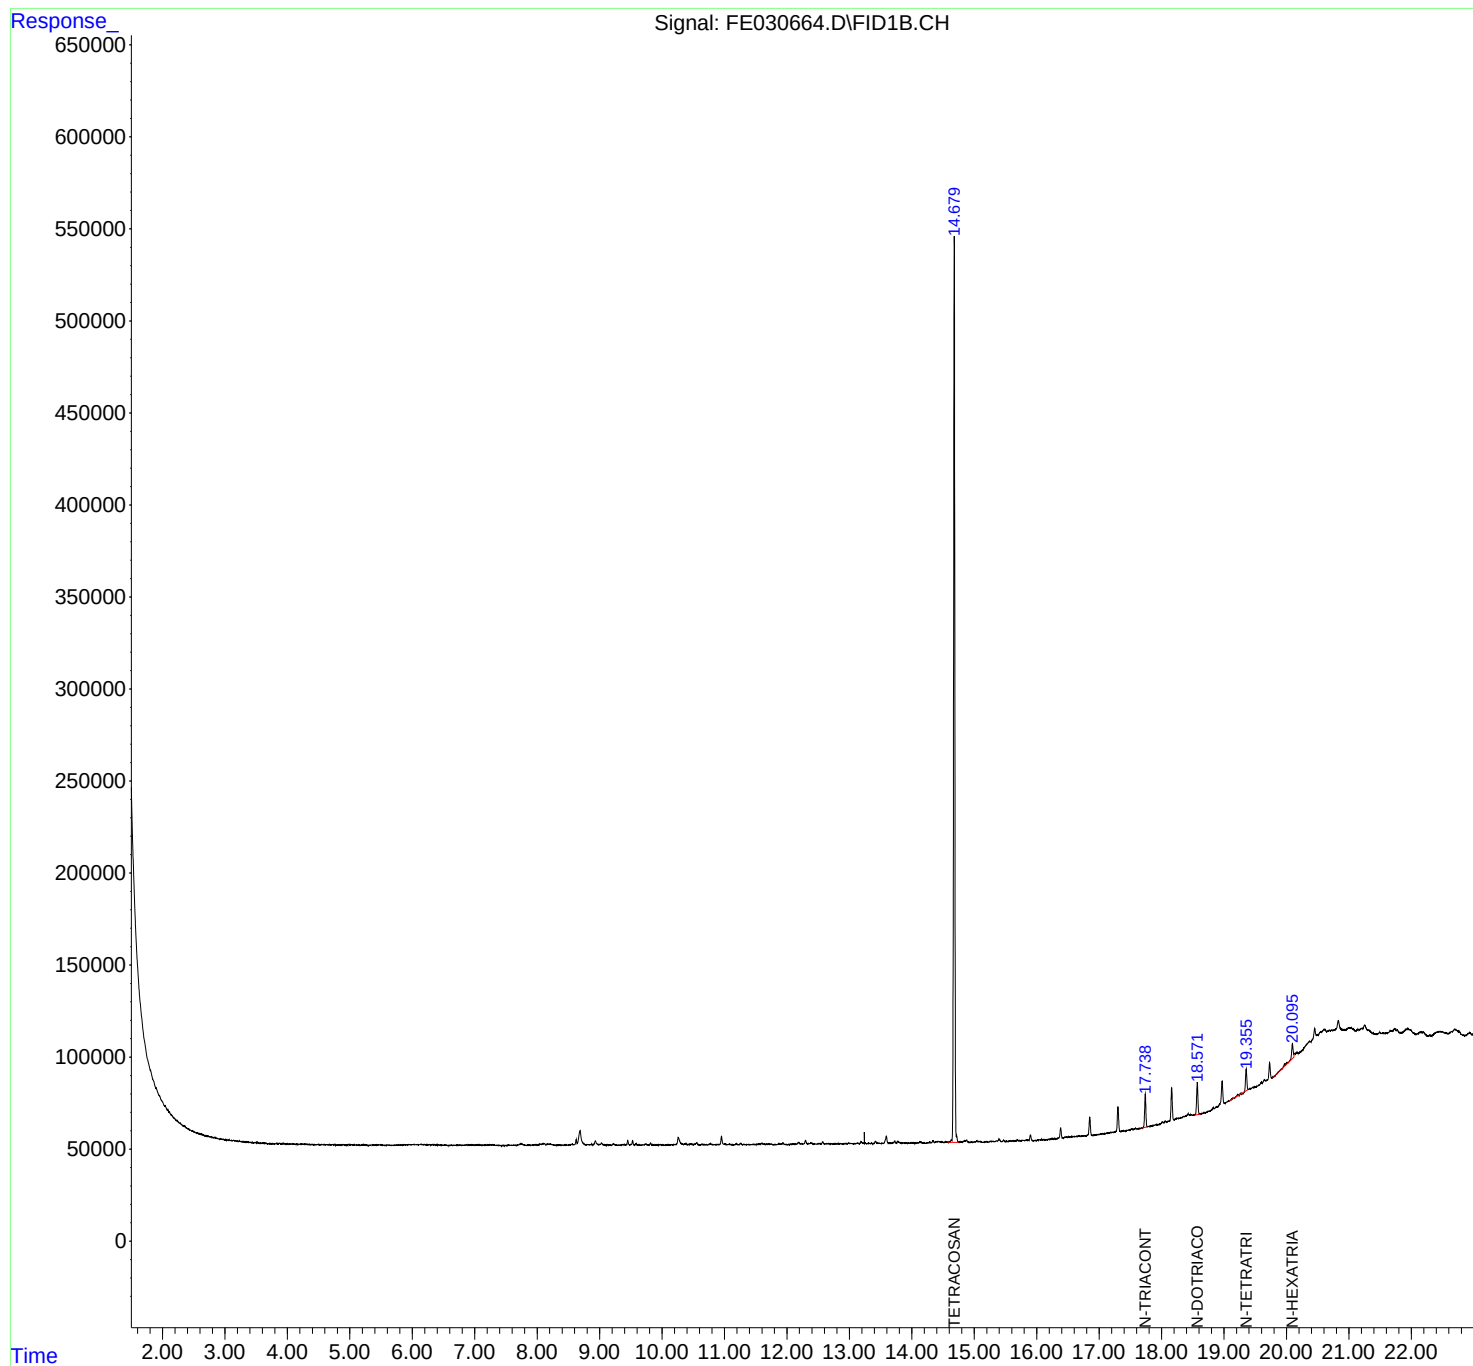


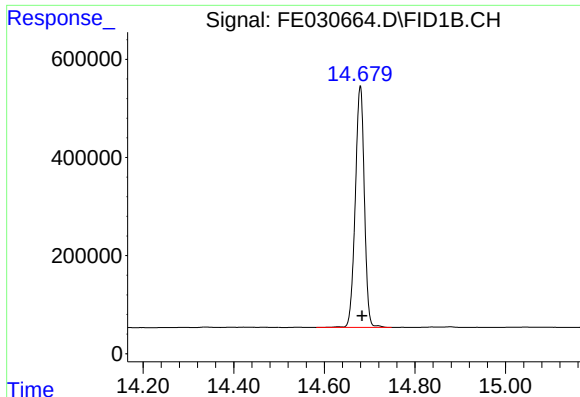

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.679 min
Delta R.T.: -0.004 min
Response: 6853473
Conc: 22.11 ug/ml

Instrument :
FID_E
ClientSampleId :

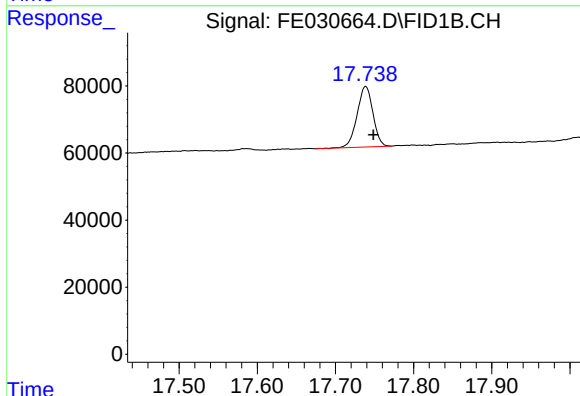


#13 N-TRIACONTANE

R.T.: 17.739 min
Delta R.T.: -0.010 min
Response: 252635
Conc: 0.75 ug/ml

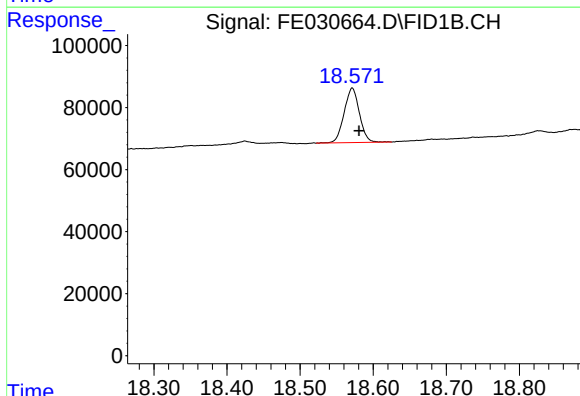


#14 N-DOTRIACONTANE

R.T.: 18.571 min
Delta R.T.: -0.009 min
Response: 254953
Conc: 0.79 ug/ml

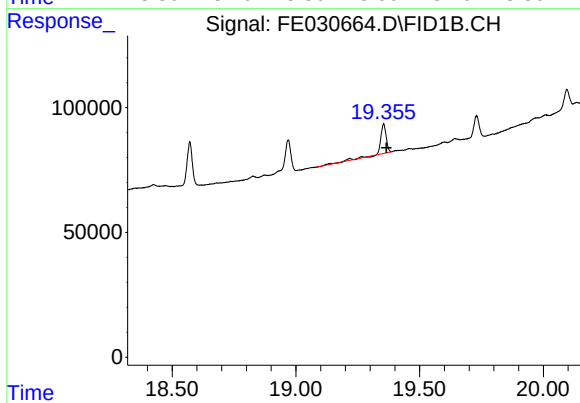

#15 N-TETRATRIACONTANE

R.T.: 19.355 min
Delta R.T.: -0.011 min
Response: 183570
Conc: 0.59 ug/ml

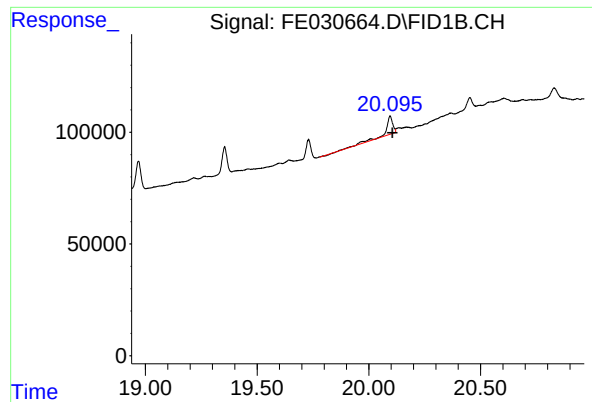

#16 N-HEXATRIACONTANE

R.T.: 20.095 min
Delta R.T.: -0.011 min
Response: 161602
Conc: 0.57 ug/ml

Instrument :
FID_E
ClientSampleId :