

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100422AL\  
 Data File : FE037940.D  
 Signal(s) : FID1B.ch  
 Acq On : 04 Oct 2022 20:09  
 Operator : YP\AJ  
 Sample : N4960-01DL 5X  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 PAT-01-100322DL

Integration File: autoint1.e  
 Quant Time: Oct 05 04:16:06 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 092822.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Sep 28 06:23:29 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units  |
|--------------------------------|--------|------------|-------------|
| -----                          |        |            |             |
| System Monitoring Compounds    |        |            |             |
| 9) S ortho-Terphenyl (SURR)    | 11.610 | 925569     | 5.351 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 10.70%      |
| 12) S 1-chlorooctadecane (S... | 13.031 | 806071     | 5.964 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 11.93%      |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100422AL\  
Data File : FE037940.D  
Signal(s) : FID1B.ch  
Acq On : 04 Oct 2022 20:09  
Operator : YP\AJ  
Sample : N4960-01DL 5X  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
PAT-01-100322DL

Integration File: autoint1.e  
Quant Time: Oct 05 04:16:06 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 092822.M  
Quant Title : GC Extractables  
QLast Update : Wed Sep 28 06:23:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

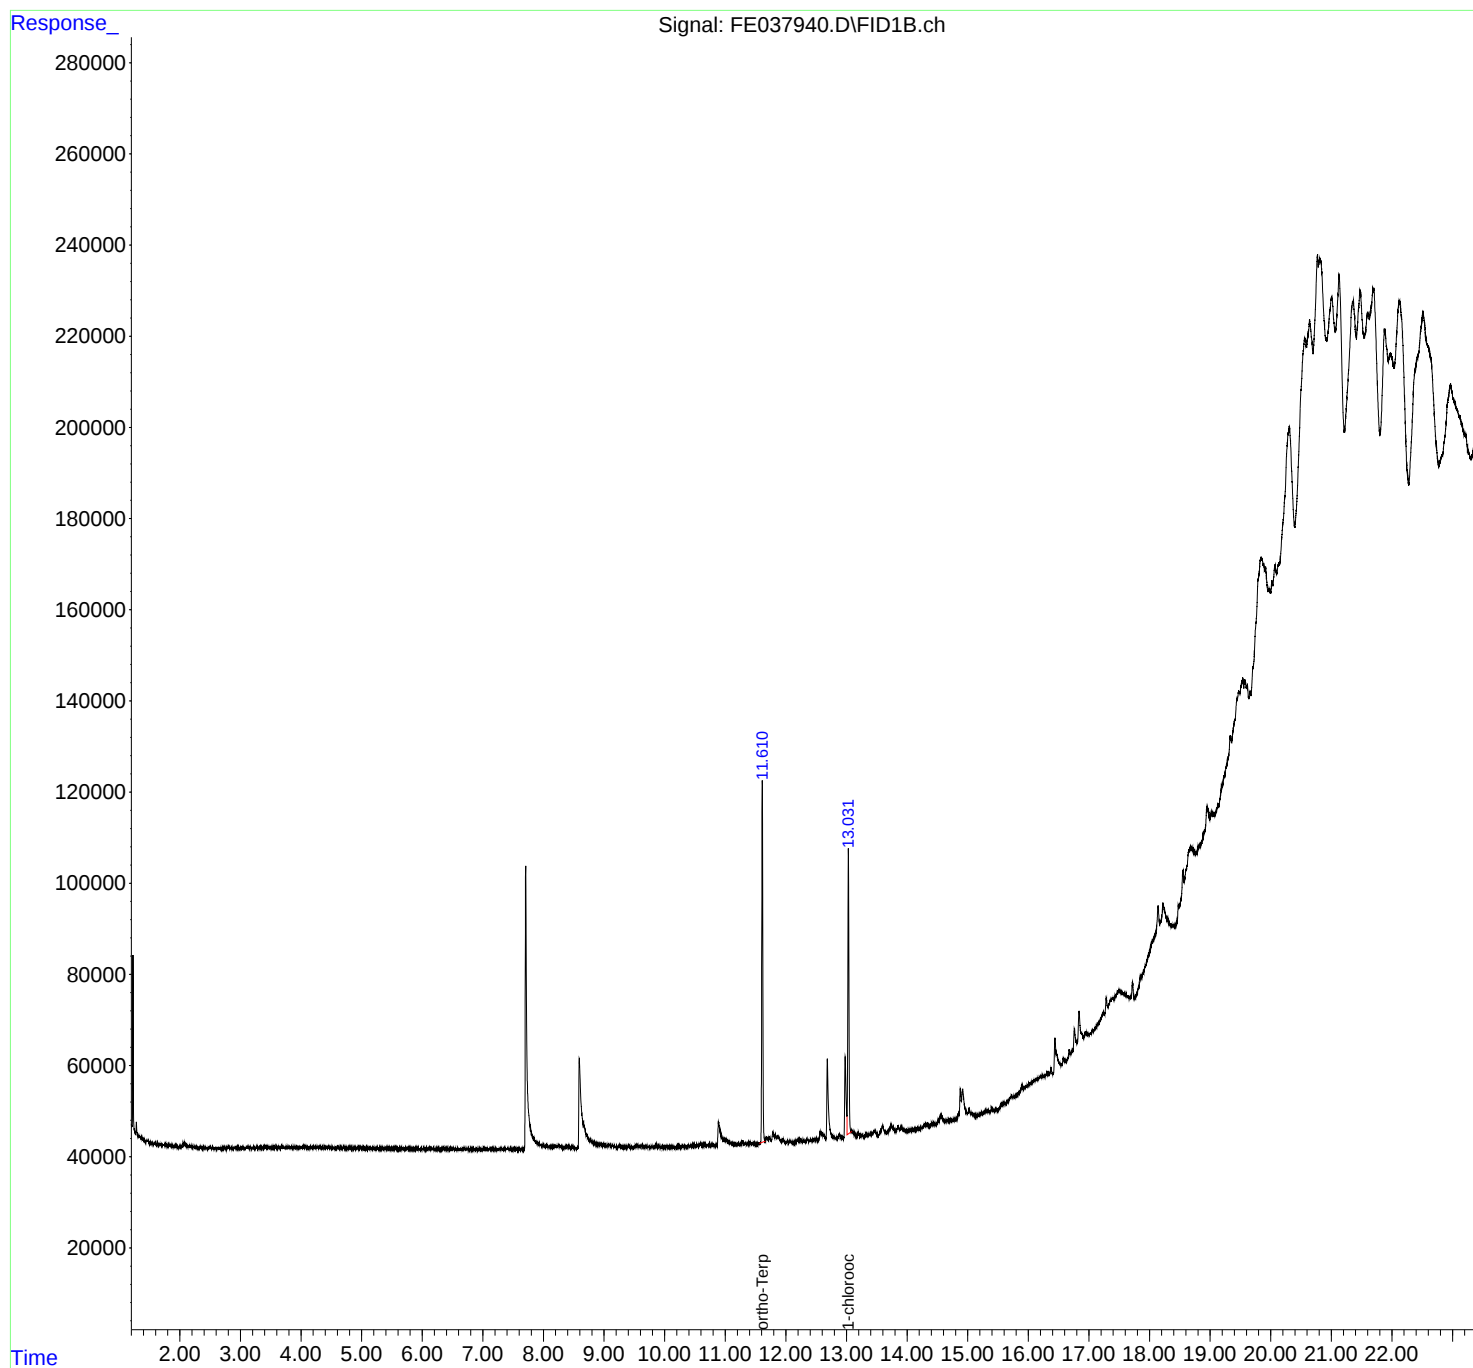


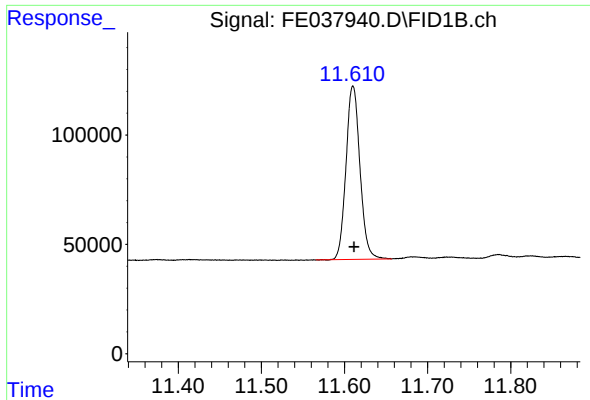

#9 ortho-Terphenyl (SURR)

R.T.: 11.610 min  
Delta R.T.: -0.001 min  
Response: 925569  
Conc: 5.35 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
PAT-01-100322DL

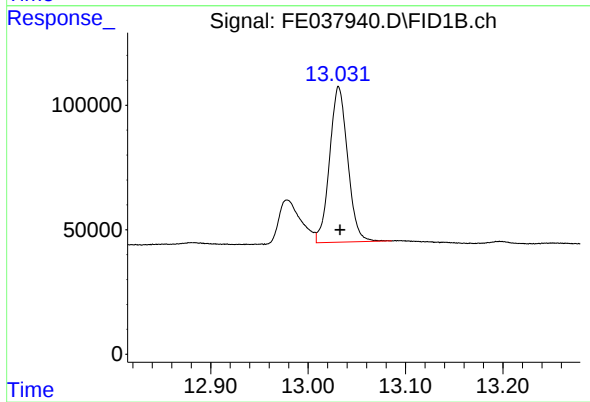

#12 1-chlorooctadecane (SURR)

R.T.: 13.031 min  
Delta R.T.: -0.001 min  
Response: 806071  
Conc: 5.96 ug/ml