

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100423AL\
 Data File : FE044575.D
 Signal(s) : FID1B.ch
 Acq On : 04 Oct 2023 08:35
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 05 00:16:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092523.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 25 11:06:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) T n-Docosane (C22)	14.104	288087	1.868 ug/ml
14) T n-Tetracosane (C24)	15.216	191490	1.267 ug/ml
15) T n-Hexacosane (C26)	16.240	197804	1.345 ug/ml
16) T n-Octacosane (C28)	17.191	145110	1.012 ug/ml
17) T n-Tricontane (C30)	18.081	129140	0.871 ug/ml
18) T n-Dotriacontane (C32)	18.914	293943	1.986 ug/ml
19) T n-Tetratriacontane (C34)	19.699	209732	1.435 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100423AL\
Data File : FE044575.D
Signal(s) : FID1B.ch
Acq On : 04 Oct 2023 08:35
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 05 00:16:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 11:06:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

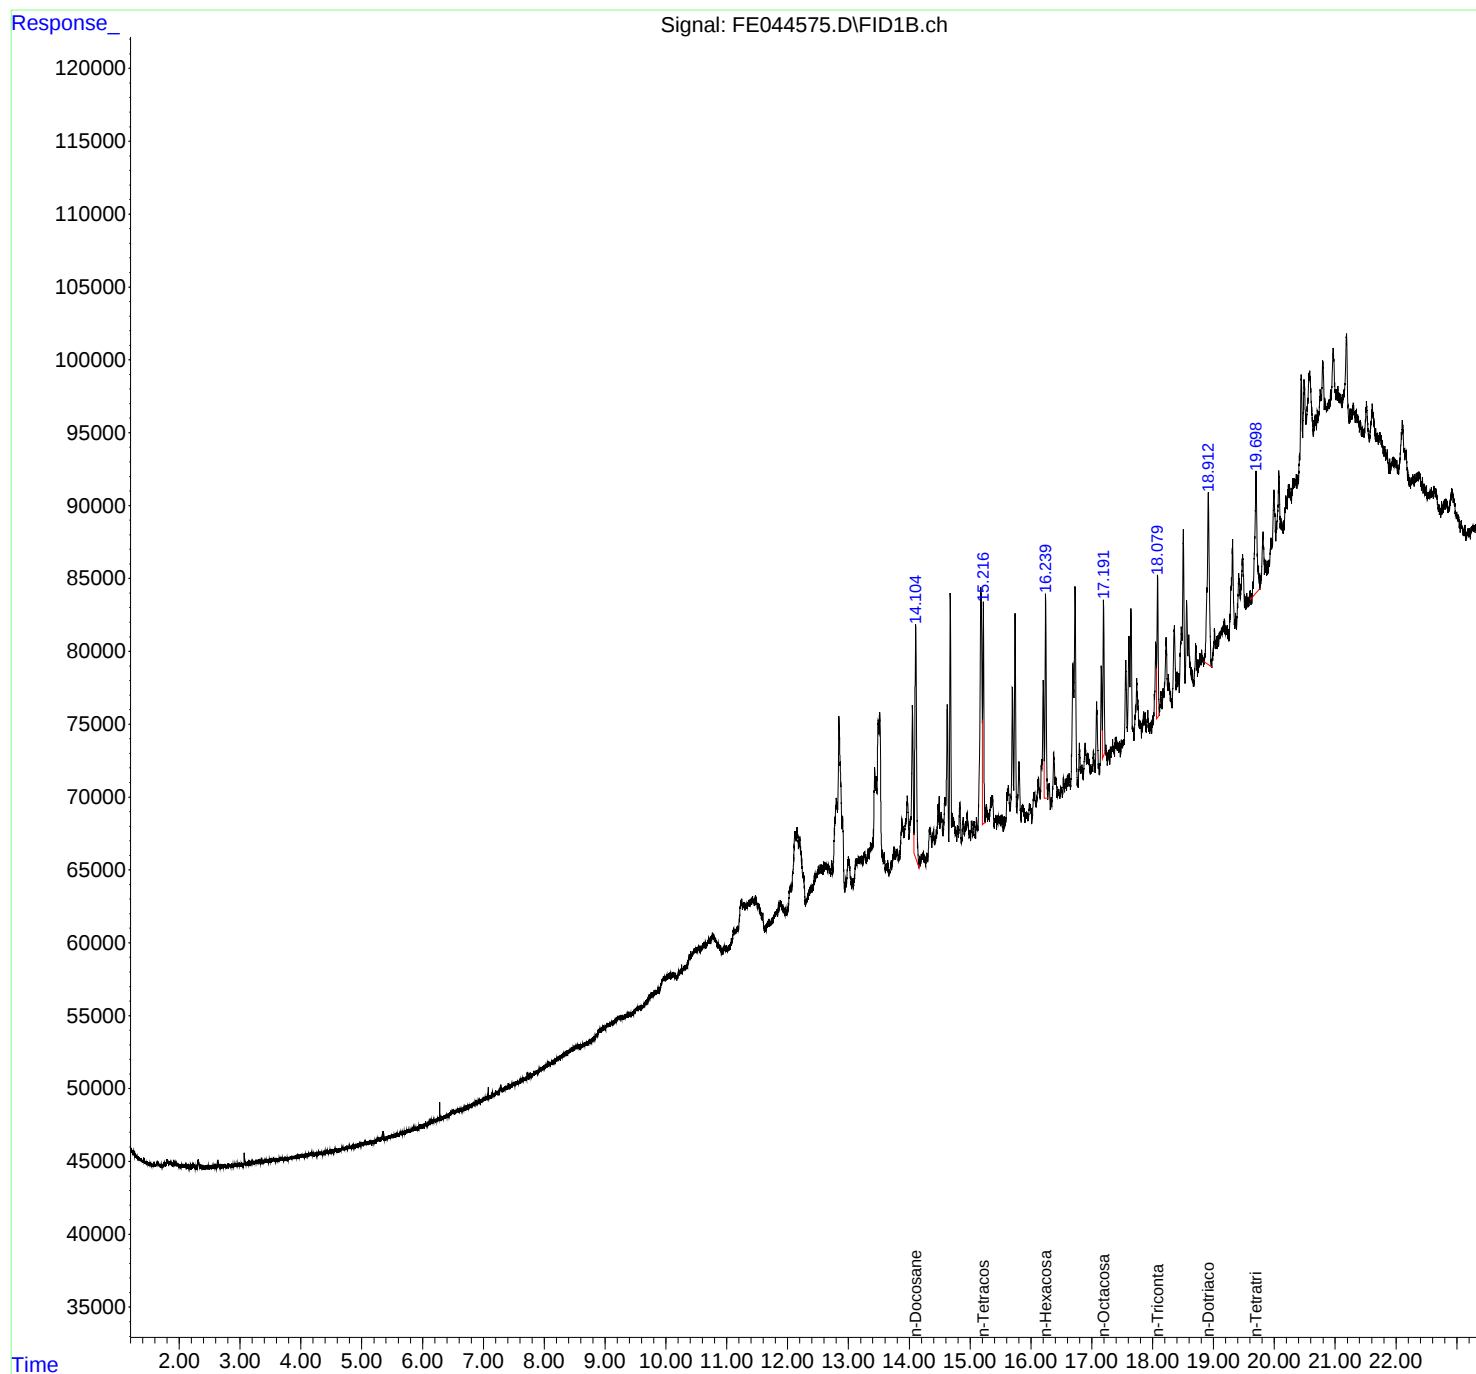


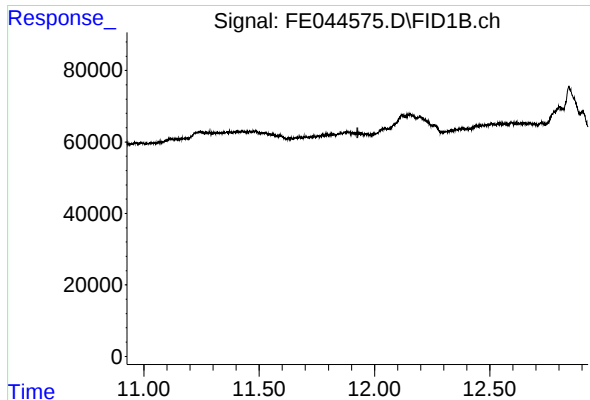

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.926 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

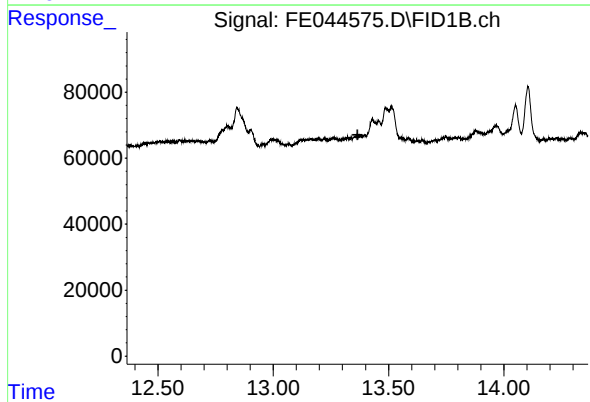


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.365 min
Response: 0
Conc: N.D.

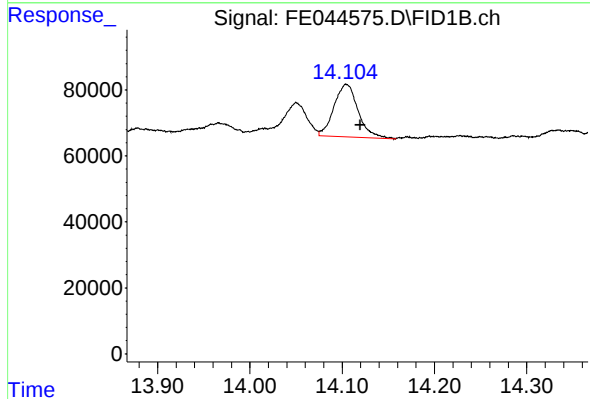


#13 n-Docosane (C22)

R.T.: 14.104 min
Delta R.T.: -0.015 min
Response: 288087
Conc: 1.87 ug/ml

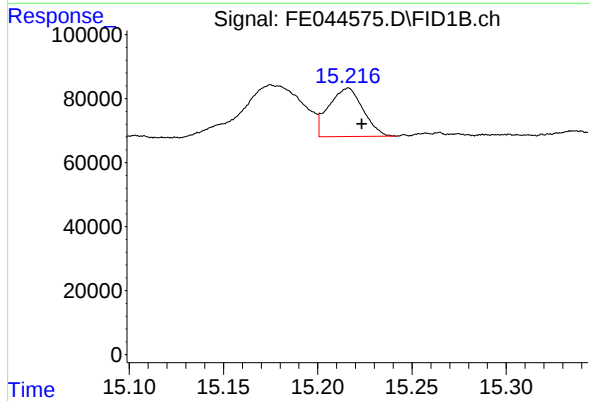

#14 n-Tetracosane (C24)


R.T.: 15.216 min
Delta R.T.: -0.007 min
Response: 191490
Conc: 1.27 ug/ml

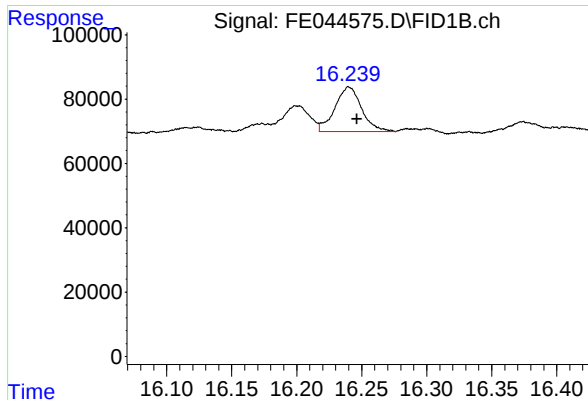

#15 n-Hexacosane (C26)


R.T.: 16.240 min
Delta R.T.: -0.006 min
Response: 197804
Conc: 1.34 ug/ml

Instrument :
FID_E
ClientSampleId :

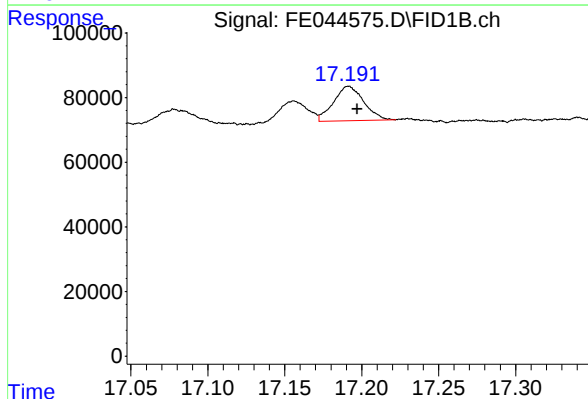


#16 n-Octacosane (C28)

R.T.: 17.191 min
Delta R.T.: -0.006 min
Response: 145110
Conc: 1.01 ug/ml

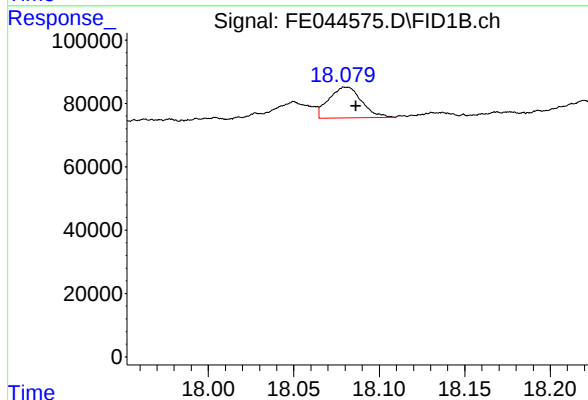


#17 n-Tricontane (C30)

R.T.: 18.081 min
Delta R.T.: -0.006 min
Response: 129140
Conc: 0.87 ug/ml

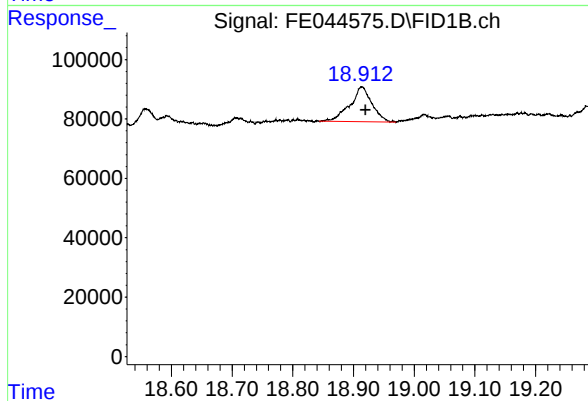

#18 n-Dotriacontane (C32)

R.T.: 18.914 min
Delta R.T.: -0.006 min
Response: 293943
Conc: 1.99 ug/ml

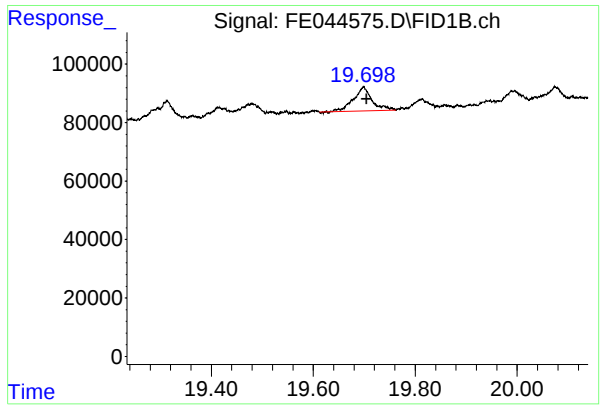

#19 n-Tetratriacontane (C34)

R.T.: 19.699 min

Delta R.T.: -0.006 min

Response: 209732

Conc: 1.44 ug/ml

Instrument :

FID_E

ClientSampleId :