

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100518\
Data File : FE028870.D
Signal(s) : FID1B.CH
Acq On : 05 Oct 2018 10:16
Operator : DD\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 06 04:10:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092218.M
Quant Title :
QLast Update : Fri Sep 21 08:15:58 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	15.125	223051	0.911 ug/ml
14)	N-DOTRIACONTANE	18.848	631855	3.329 ug/ml
16)	N-HEXATRIACONTANE	20.401	560626	2.944 ug/ml
18)	N-TETRACONTANE	22.197	470854	2.723 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100518\
Data File : FE028870.D
Signal(s) : FID1B.CH
Acq On : 05 Oct 2018 10:16
Operator : DD\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 06 04:10:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092218.M
Quant Title :
QLast Update : Fri Sep 21 08:15:58 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

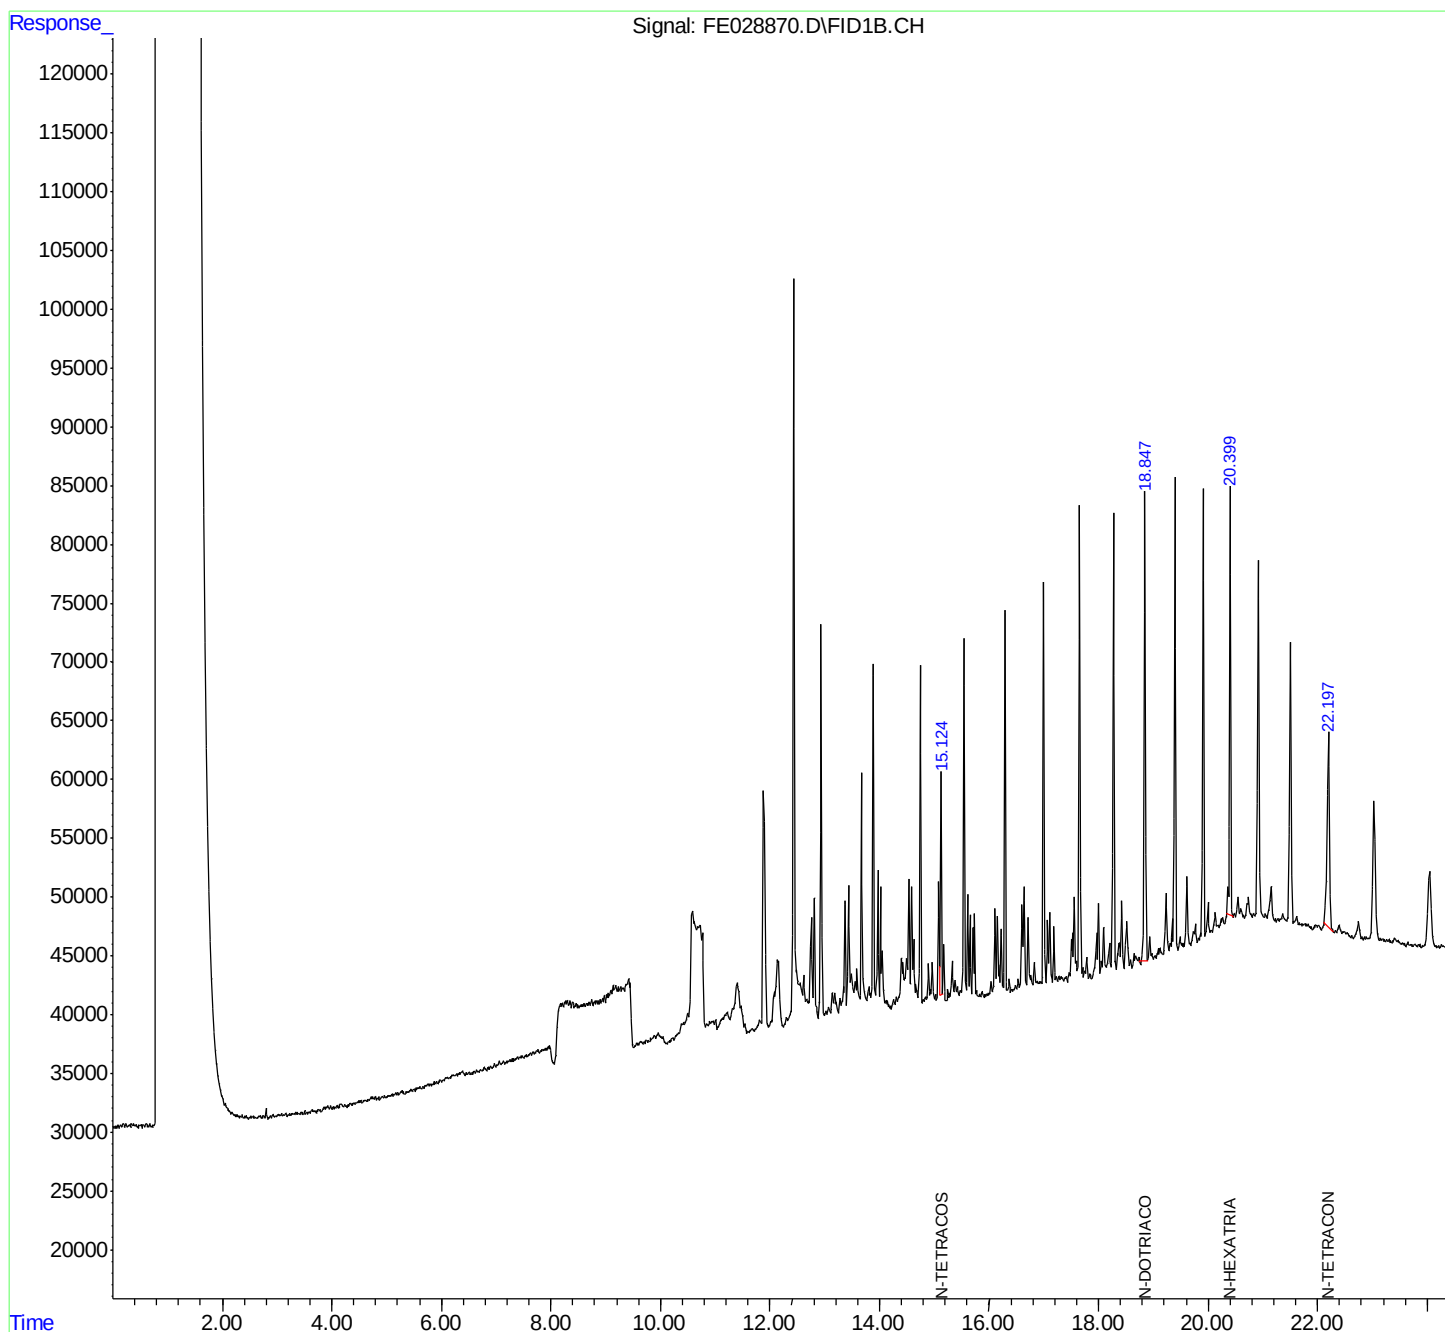

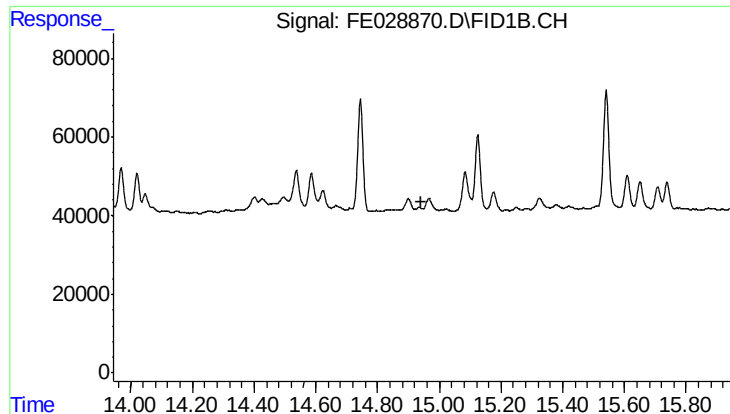


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.944 min
Response: 0
Conc: N.D.

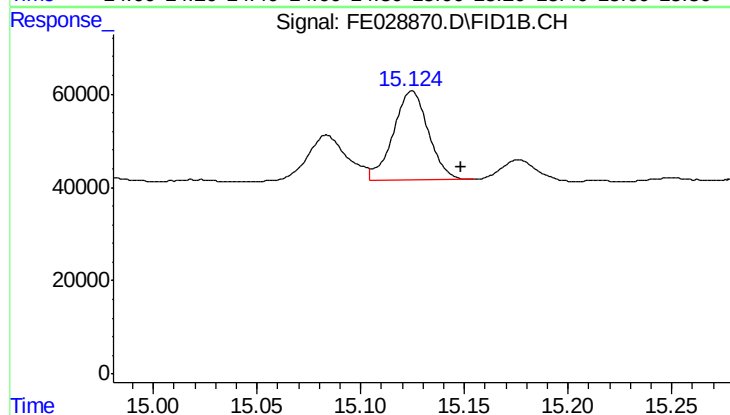


#10 N-TETRACOSANE

R.T.: 15.125 min
Delta R.T.: -0.024 min
Response: 223051
Conc: 0.91 ug/ml

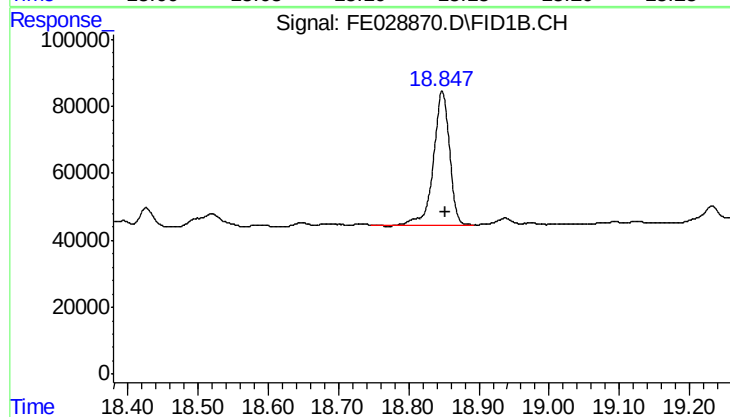


#14 N-DOTRIACONTANE

R.T.: 18.848 min
Delta R.T.: -0.005 min
Response: 631855
Conc: 3.33 ug/ml

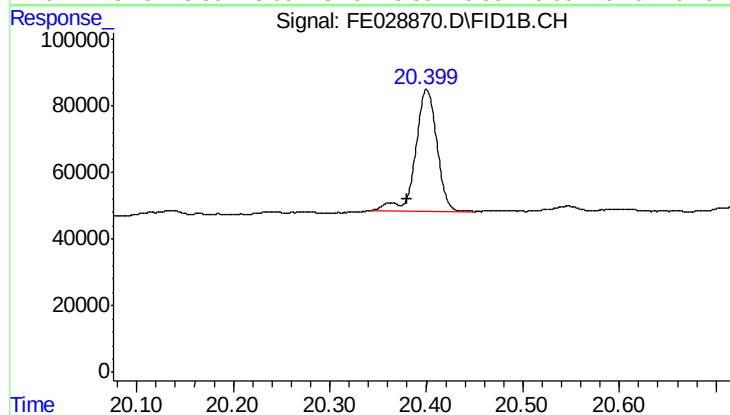

#16 N-HEXATRIACONTANE

R.T.: 20.401 min
Delta R.T.: 0.020 min
Response: 560626
Conc: 2.94 ug/ml

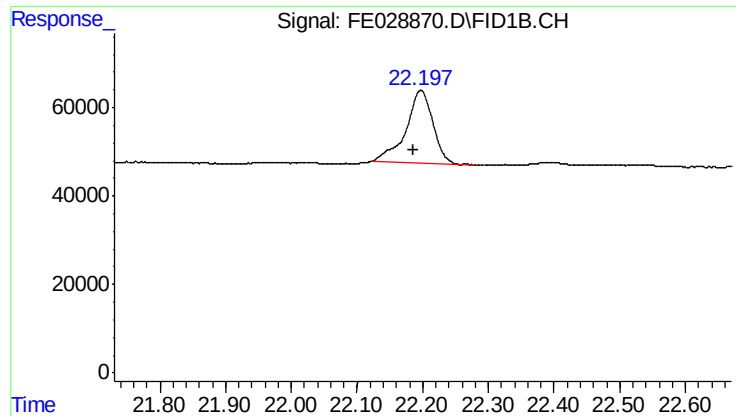

#18 N-TETRACONTANE

R.T.: 22.197 min
Delta R.T.: 0.011 min
Response: 470854
Conc: 2.72 ug/ml