

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100520\
 Data File : FE032920.D
 Signal(s) : FID1B.CH
 Acq On : 05 Oct 2020 21:54
 Operator : DD\AJ
 Sample : PB132086BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 06 00:56:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
 Quant Title :
 QLast Update : Tue Sep 15 03:21:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.666	4537221	14.482 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.849	228216	0.649 ug/ml
13) N-TRIACONTANE	17.724	61476	0.178 ug/ml
14) N-DOTRIACONTANE	18.554	234000	0.703 ug/ml
15) N-TETRATRIACONTANE	19.343	35687	0.112 ug/ml
16) N-HEXATRIACONTANE	20.103	367870	1.246 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100520\
Data File : FE032920.D
Signal(s) : FID1B.CH
Acq On : 05 Oct 2020 21:54
Operator : DD\AJ
Sample : PB132086BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 06 00:56:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE091420.M
Quant Title :
QLast Update : Tue Sep 15 03:21:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

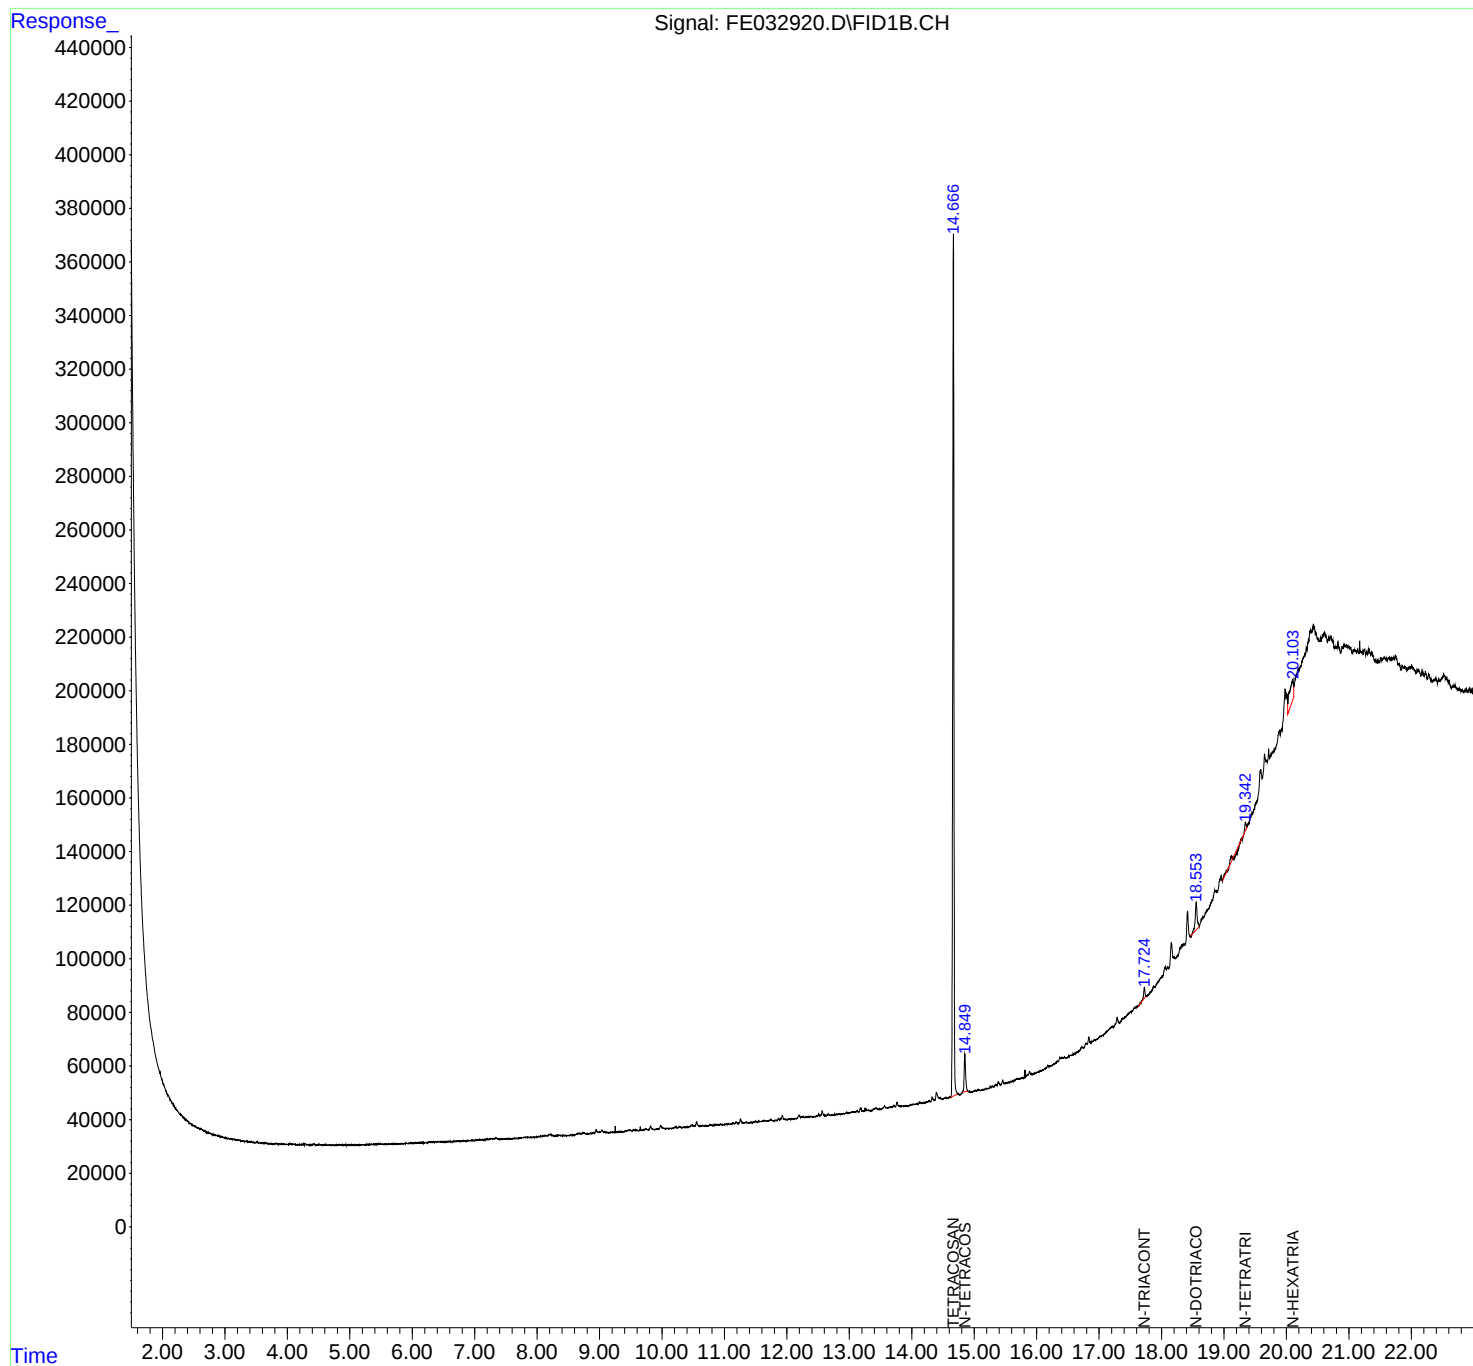


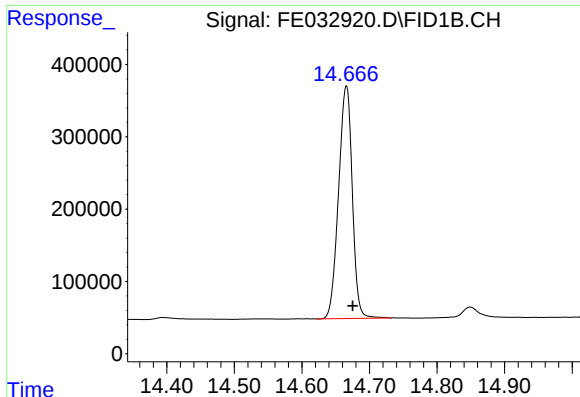

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.666 min
Delta R.T.: -0.009 min
Response: 4537221
Conc: 14.48 ug/ml

Instrument :
FID_E
ClientSampleId :

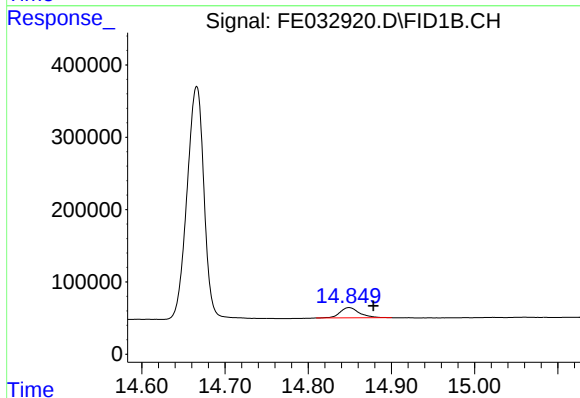


#10 N-TETRACOSANE

R.T.: 14.849 min
Delta R.T.: -0.029 min
Response: 228216
Conc: 0.65 ug/ml

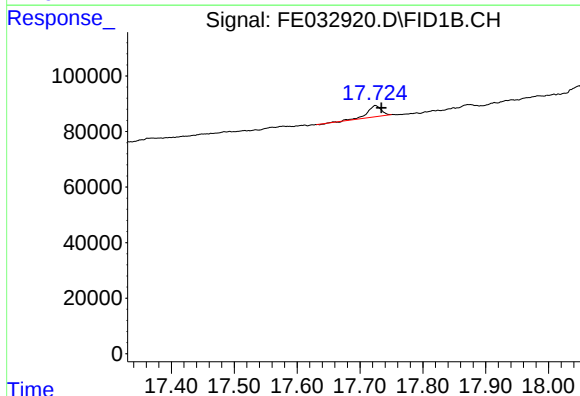


#13 N-TRIACONTANE

R.T.: 17.724 min
Delta R.T.: -0.010 min
Response: 61476
Conc: 0.18 ug/ml

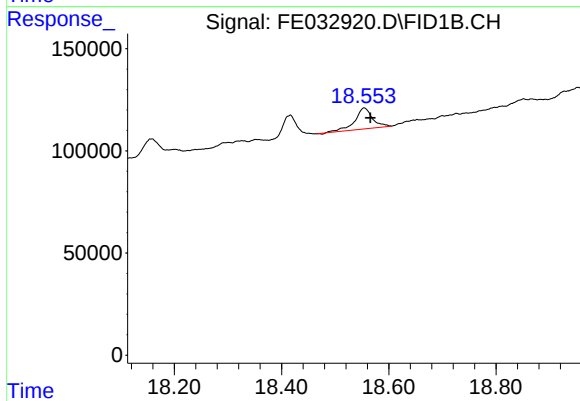

#14 N-DOTRIACONTANE

R.T.: 18.554 min
Delta R.T.: -0.012 min
Response: 234000
Conc: 0.70 ug/ml

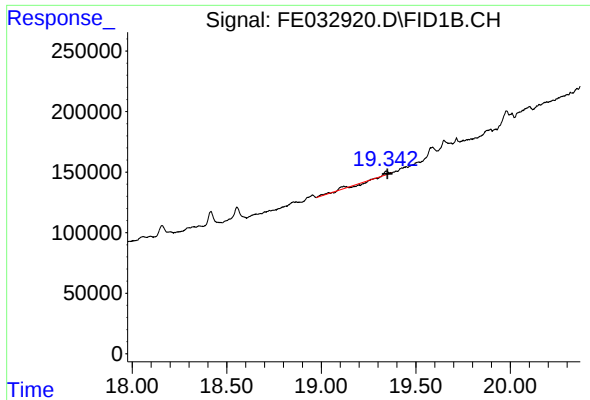

#15 N-TETRATRIACONTANE


R.T.: 19.343 min

Delta R.T.: -0.006 min

Response: 35687

Conc: 0.11 ug/ml

Instrument :
FID_E
ClientSampleId :

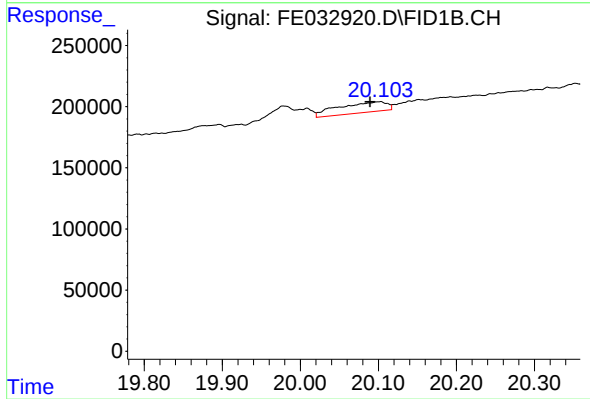

#16 N-HEXATRIACONTANE

R.T.: 20.103 min

Delta R.T.: 0.014 min

Response: 367870

Conc: 1.25 ug/ml