

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100520\  
 Data File : FE032919.D  
 Signal(s) : FID1B.CH  
 Acq On : 05 Oct 2020 21:21  
 Operator : DD\AJ  
 Sample : L4260-11 5X  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 PAV-B23-100220-0-10

Manual Integrations  
 APPROVED

Ankita  
 10/6/2020 12:15:39 PM

Integration File: autoint1.e  
 Quant Time: Oct 06 00:56:18 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE091420.M  
 Quant Title :  
 QLast Update : Tue Sep 15 03:21:18 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.666 | 918014   | 2.930 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100520\  
Data File : FE032919.D  
Signal(s) : FID1B.CH  
Acq On : 05 Oct 2020 21:21  
Operator : DD\AJ  
Sample : L4260-11 5X  
Misc :  
ALS Vial : 20 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
PAV-B23-100220-0-10


Manual Integrations  
APPROVED

Ankita  
10/6/2020 12:15:39 PM

Integration File: autoint1.e  
Quant Time: Oct 06 00:56:18 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE091420.M  
Quant Title :  
QLast Update : Tue Sep 15 03:21:18 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

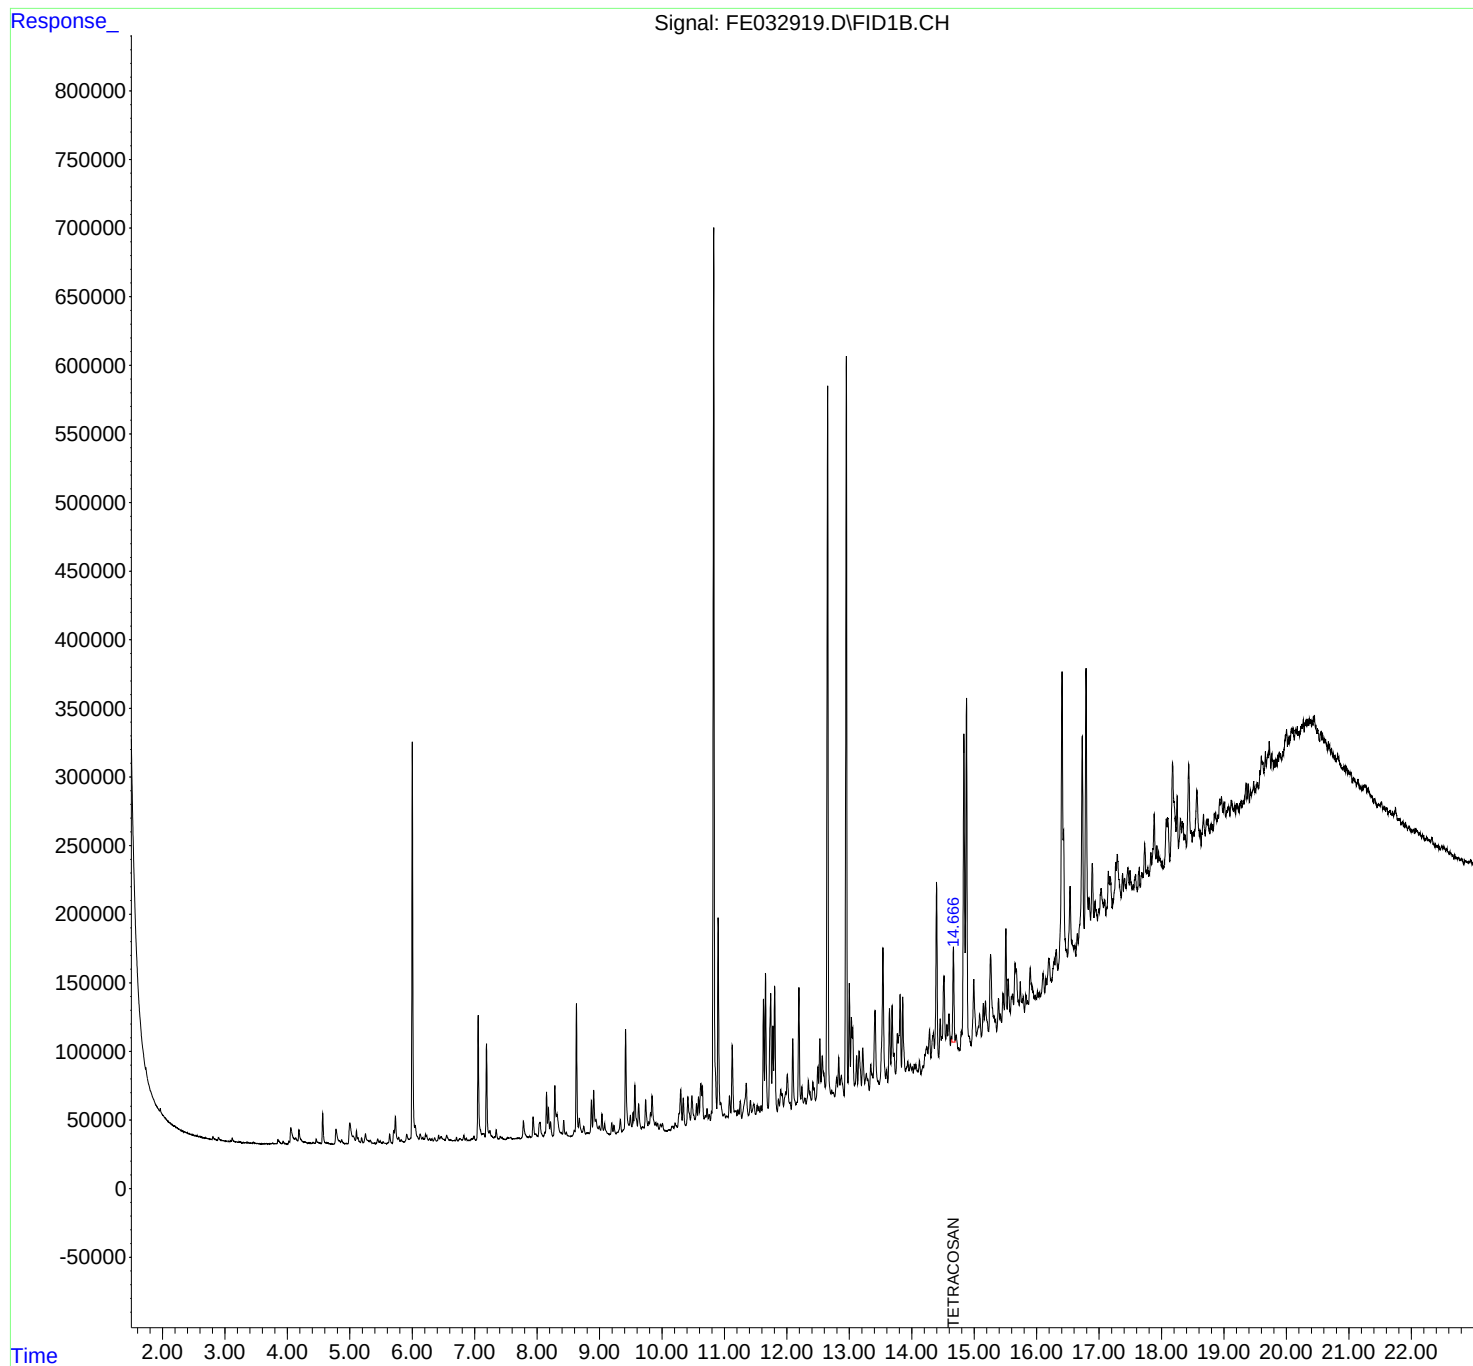

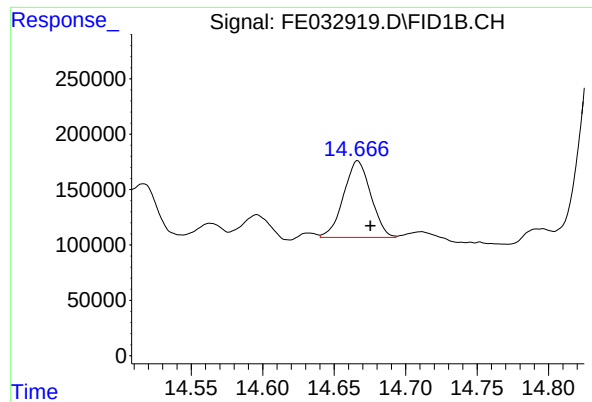

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.666 min  
Delta R.T.: -0.009 min  
Response: 918014  
Conc: 2.93 ug/ml m

Instrument :  
FID\_E  
ClientSampleId :  
PAV-B23-100220-0-10

Manual Integrations  
APPROVED

Ankita  
10/6/2020 12:15:39 PM