

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100523AL\
Data File : FE044634.D
Signal(s) : FID1B.ch
Acq On : 06 Oct 2023 01:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 06 03:36:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 11:06:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.721	74617	0.511 ug/ml
20) T	n-Hexatriacontane (C36)	20.399	41502	0.286 ug/ml
21) T	n-Octatriacontane (C38)	21.123f	274586	1.833 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100523AL\
Data File : FE044634.D
Signal(s) : FID1B.ch
Acq On : 06 Oct 2023 01:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 06 03:36:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 11:06:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

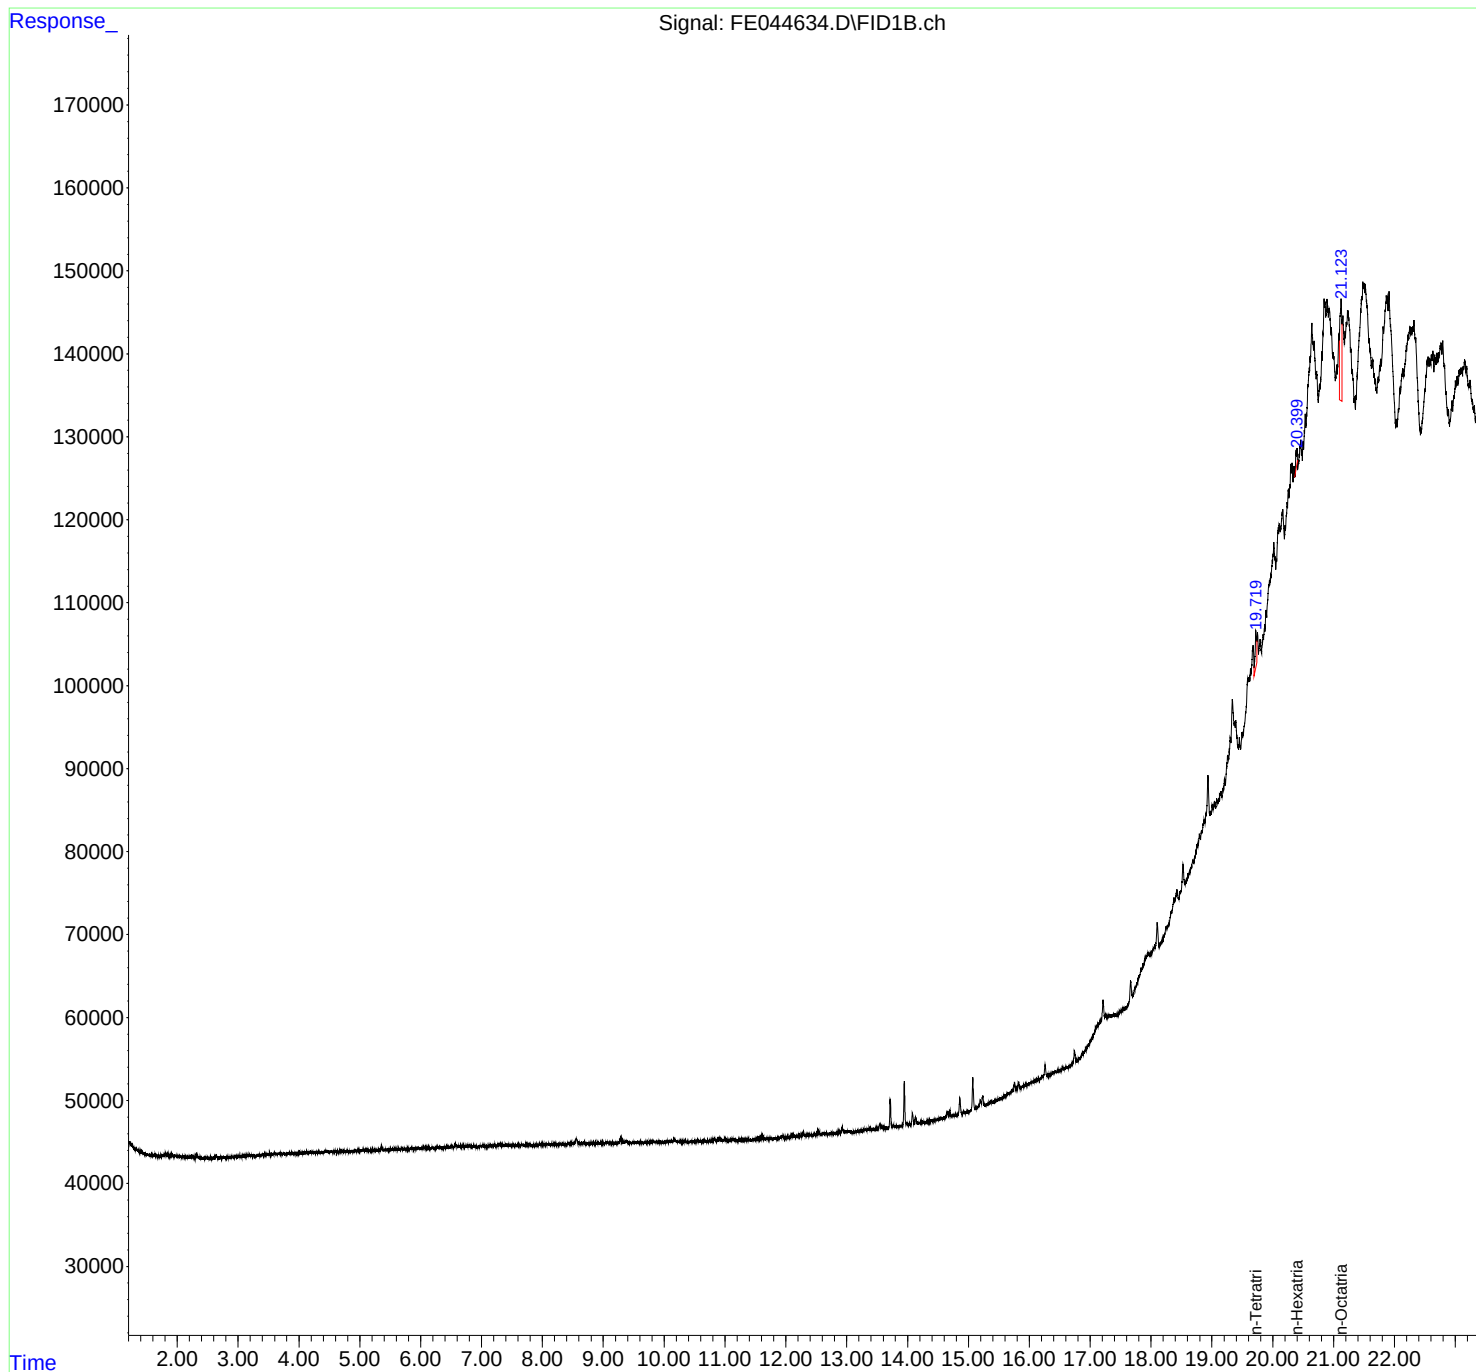


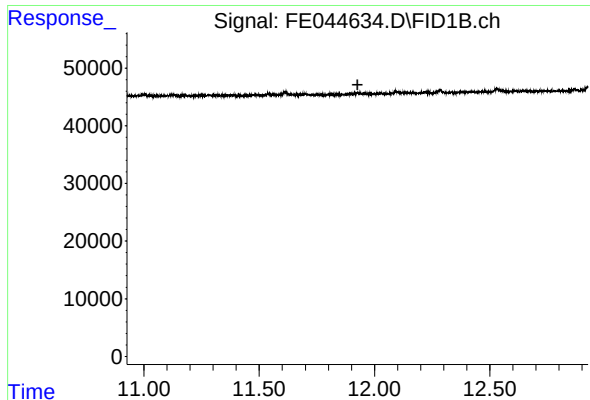

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.926 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

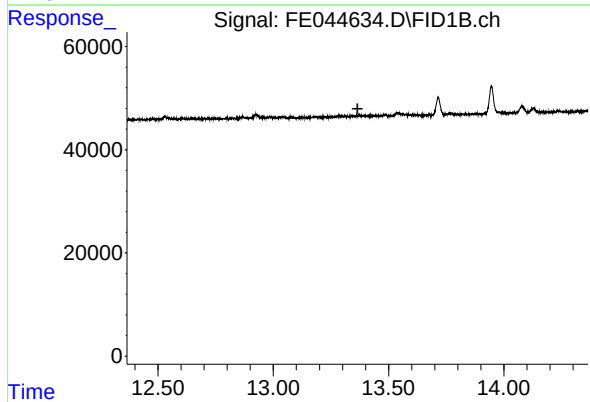


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.365 min
Response: 0
Conc: N.D.

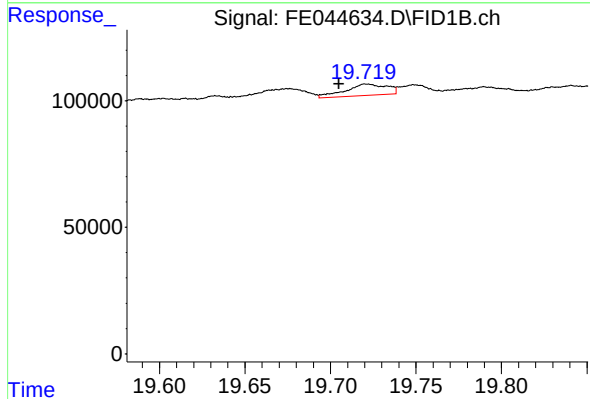


#19 n-Tetratriacontane (C34)

R.T.: 19.721 min
Delta R.T.: 0.016 min
Response: 74617
Conc: 0.51 ug/ml

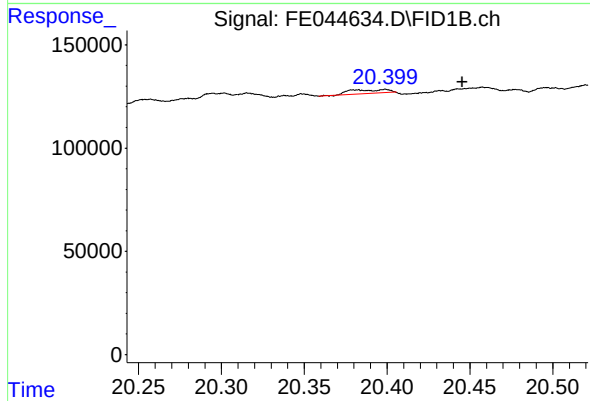

#20 n-Hexatriacontane (C36)

R.T.: 20.399 min
Delta R.T.: -0.047 min
Response: 41502
Conc: 0.29 ug/ml

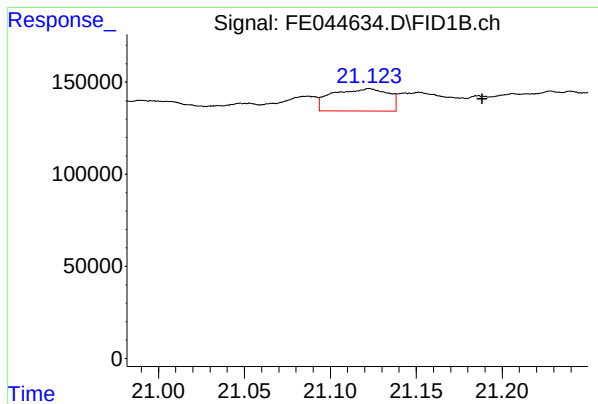

#21 n-Octatriacontane (C38)

R.T.: 21.123 min
Delta R.T.: -0.065 min
Response: 274586
Conc: 1.83 ug/ml

Instrument :

FID_E

ClientSampleId :