

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100622\
Data File : FE037987.D
Signal(s) : FID1B.ch
Acq On : 06 Oct 2022 16:59
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 07 04:51:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100522.M
Quant Title :
QLast Update : Wed Oct 05 16:55:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.429	2533110	18.120 ug/ml
12) N-OCTACOSANE	16.827	2679424	19.042 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100622\
Data File : FE037987.D
Signal(s) : FID1B.ch
Acq On : 06 Oct 2022 16:59
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 07 04:51:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100522.M
Quant Title :
QLast Update : Wed Oct 05 16:55:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

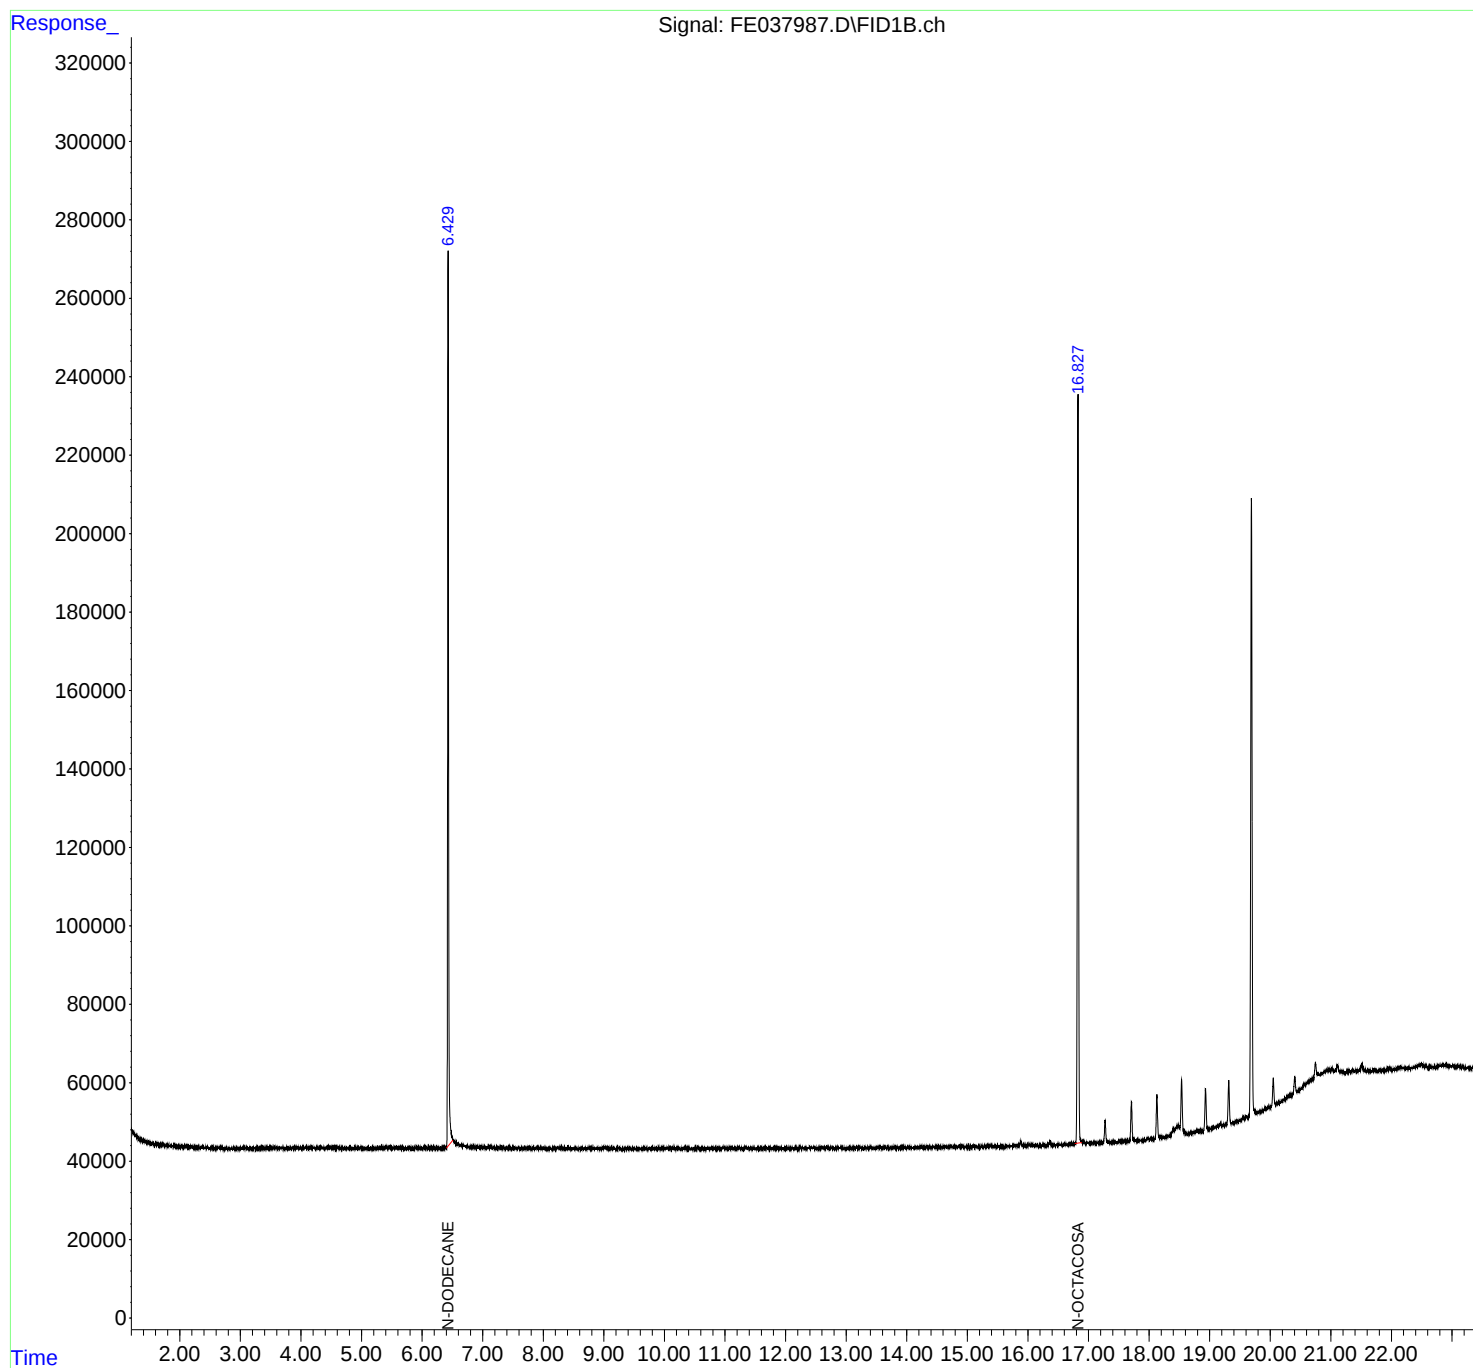


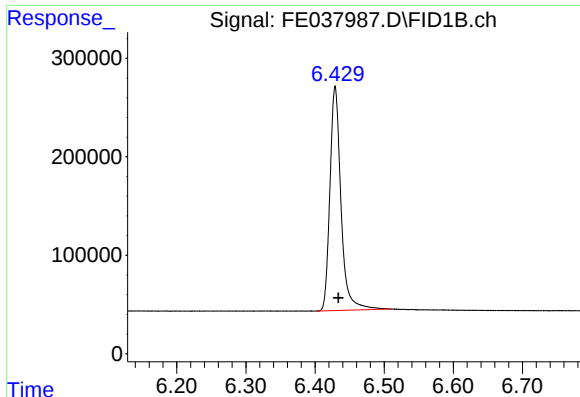

#3 N-DODECANE


R.T.: 6.429 min
Delta R.T.: -0.005 min
Response: 2533110
Conc: 18.12 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

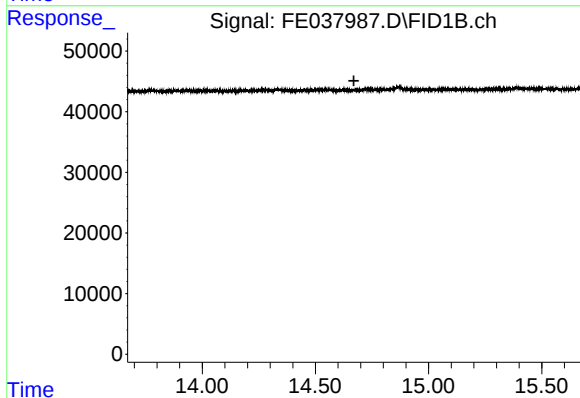

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.670 min
Response: 0
Conc: N.D.

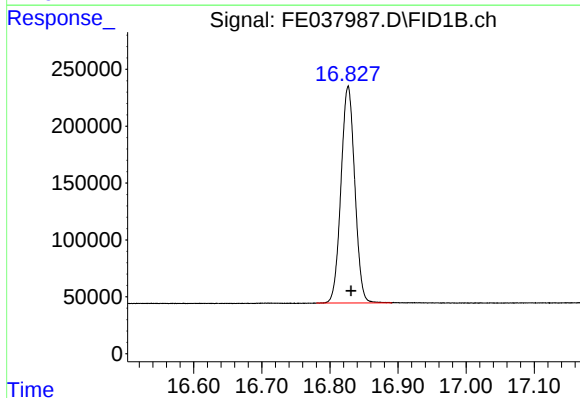

#12 N-OCTACOSANE

R.T.: 16.827 min
Delta R.T.: -0.004 min
Response: 2679424
Conc: 19.04 ug/ml