

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100625AL\
 Data File : FE056217.D
 Signal(s) : FID1B.ch
 Acq On : 07 Oct 2025 00:38
 Operator : YP\AJ
 Sample : Q3262-05DL2 500X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 MOO-25-0281-82DL2

Integration File: autoint1.e
 Quant Time: Oct 07 01:35:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092425.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 24 12:55:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.506	195187	1.399 ug/ml
Spiked Amount 50.000		Recovery =	2.80%
Target Compounds			
10) T n-Eicosane (C20)	13.054	69622	0.420 ug/ml
11) T n-Heneicosane (C21)	13.696	572184	3.521 ug/ml
13) T n-Docosane (C22)	14.275	638947	3.999 ug/ml
14) T n-Tetracosane (C24)	15.367	336765	2.210 ug/ml
15) T n-Hexacosane (C26)	16.430	312599	2.192 ug/ml
18) T n-Dotriacontane (C32)	19.063	271711	1.821 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100625AL\
Data File : FE056217.D
Signal(s) : FID1B.ch
Acq On : 07 Oct 2025 00:38
Operator : YP\AJ
Sample : Q3262-05DL2 500X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MOO-25-0281-82DL2

Integration File: autoint1.e
Quant Time: Oct 07 01:35:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092425.M
Quant Title : GC Extractables
QLast Update : Wed Sep 24 12:55:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

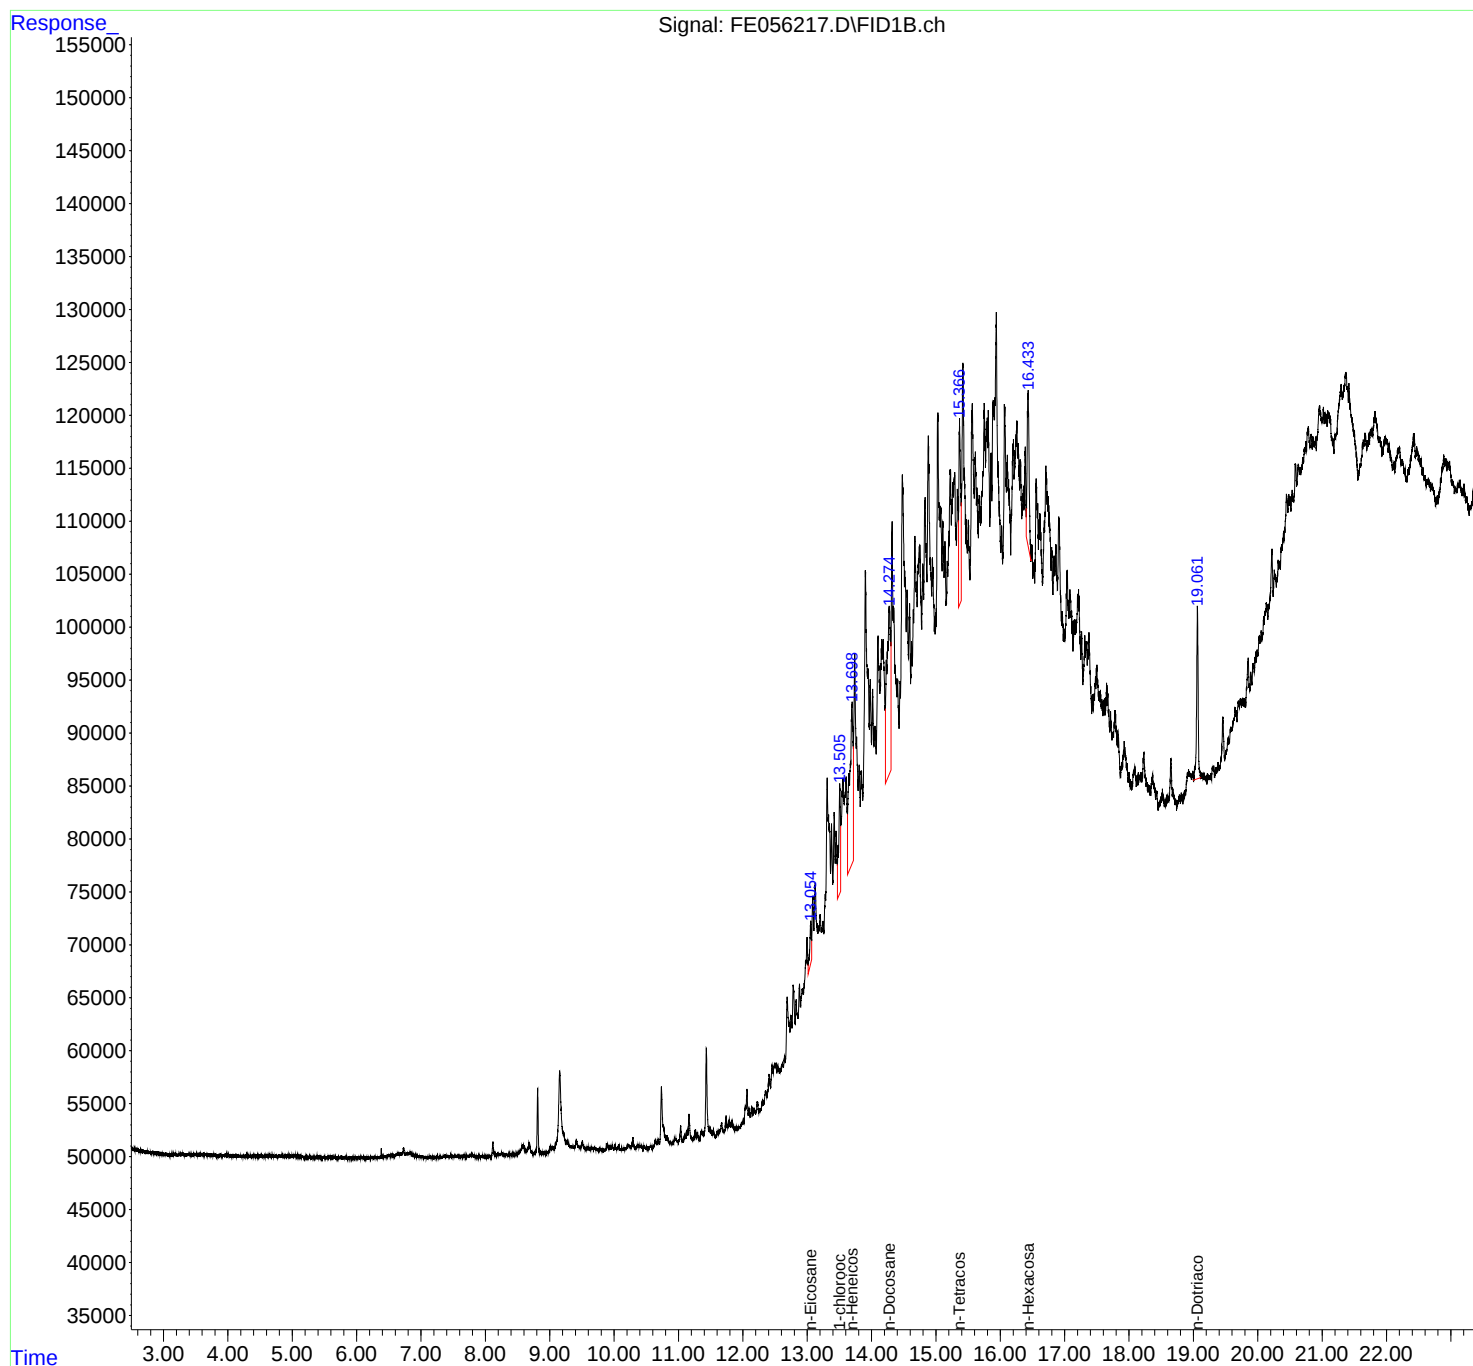


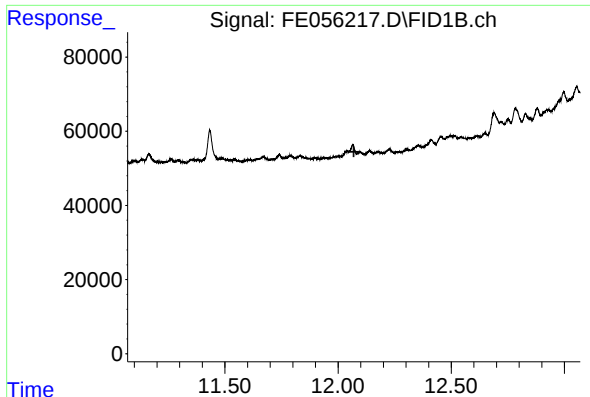

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 12.070 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MOO-25-0281-82DL2

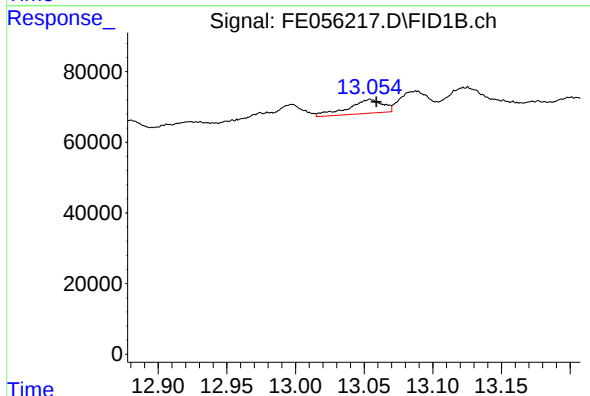


#10 n-Eicosane (C20)

R.T.: 13.054 min
Delta R.T.: -0.005 min
Response: 69622
Conc: 0.42 ug/ml

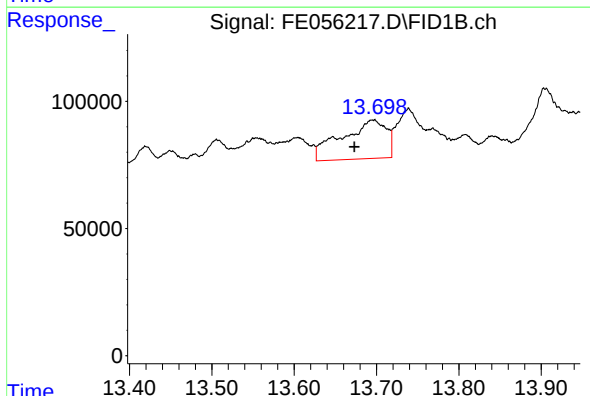


#11 n-Heneicosane (C21)

R.T.: 13.696 min
Delta R.T.: 0.023 min
Response: 572184
Conc: 3.52 ug/ml

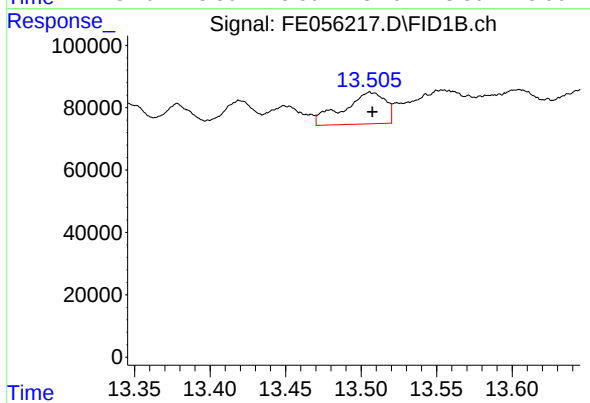

#12 1-chlorooctadecane (SURR)


R.T.: 13.506 min
Delta R.T.: 0.000 min
Response: 195187
Conc: 1.40 ug/ml

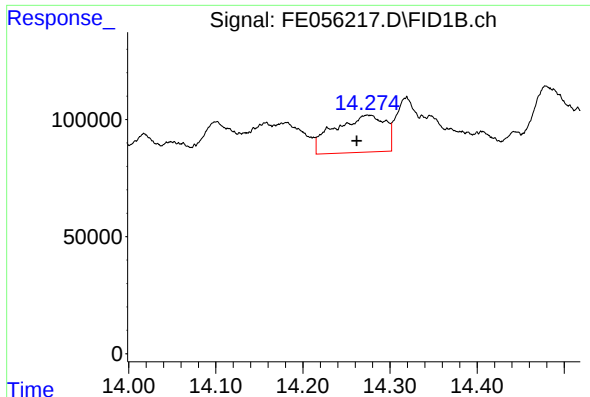

#13 n-Docosane (C22)


R.T.: 14.275 min
Delta R.T.: 0.014 min
Response: 638947
Conc: 4.00 ug/ml

Instrument :
FID_E
ClientSampleId :
MOO-25-0281-82DL2

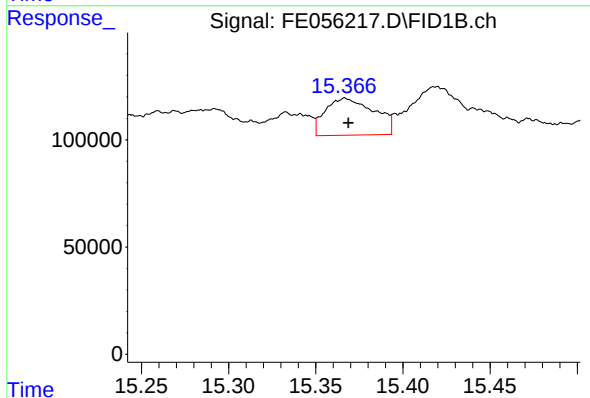


#14 n-Tetracosane (C24)

R.T.: 15.367 min
Delta R.T.: -0.002 min
Response: 336765
Conc: 2.21 ug/ml

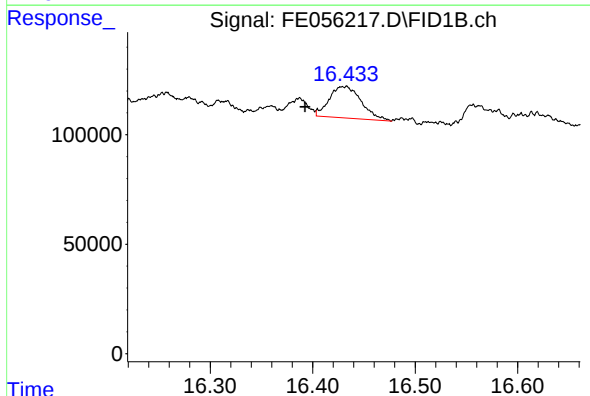

#15 n-Hexacosane (C26)

R.T.: 16.430 min
Delta R.T.: 0.038 min
Response: 312599
Conc: 2.19 ug/ml

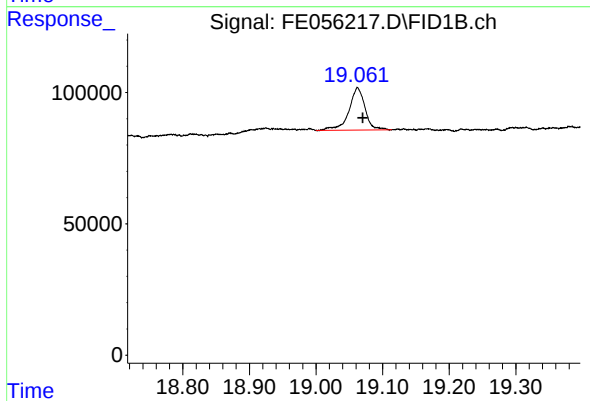

#18 n-Dotriacontane (C32)

R.T.: 19.063 min
Delta R.T.: -0.008 min
Response: 271711
Conc: 1.82 ug/ml