

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100625AL\
Data File : FE056219.D
Signal(s) : FID1B.ch
Acq On : 07 Oct 2025 02:09
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 07 04:02:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092425.M
Quant Title : GC Extractables
QLast Update : Wed Sep 24 12:55:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	19.062	148376	0.994 ug/ml
19) T	n-Tetratriacontane (C34)	19.847	125295	0.886 ug/ml
20) T	n-Hexatriacontane (C36)	20.588	83940	0.654 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100625AL\
Data File : FE056219.D
Signal(s) : FID1B.ch
Acq On : 07 Oct 2025 02:09
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 07 04:02:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092425.M
Quant Title : GC Extractables
QLast Update : Wed Sep 24 12:55:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

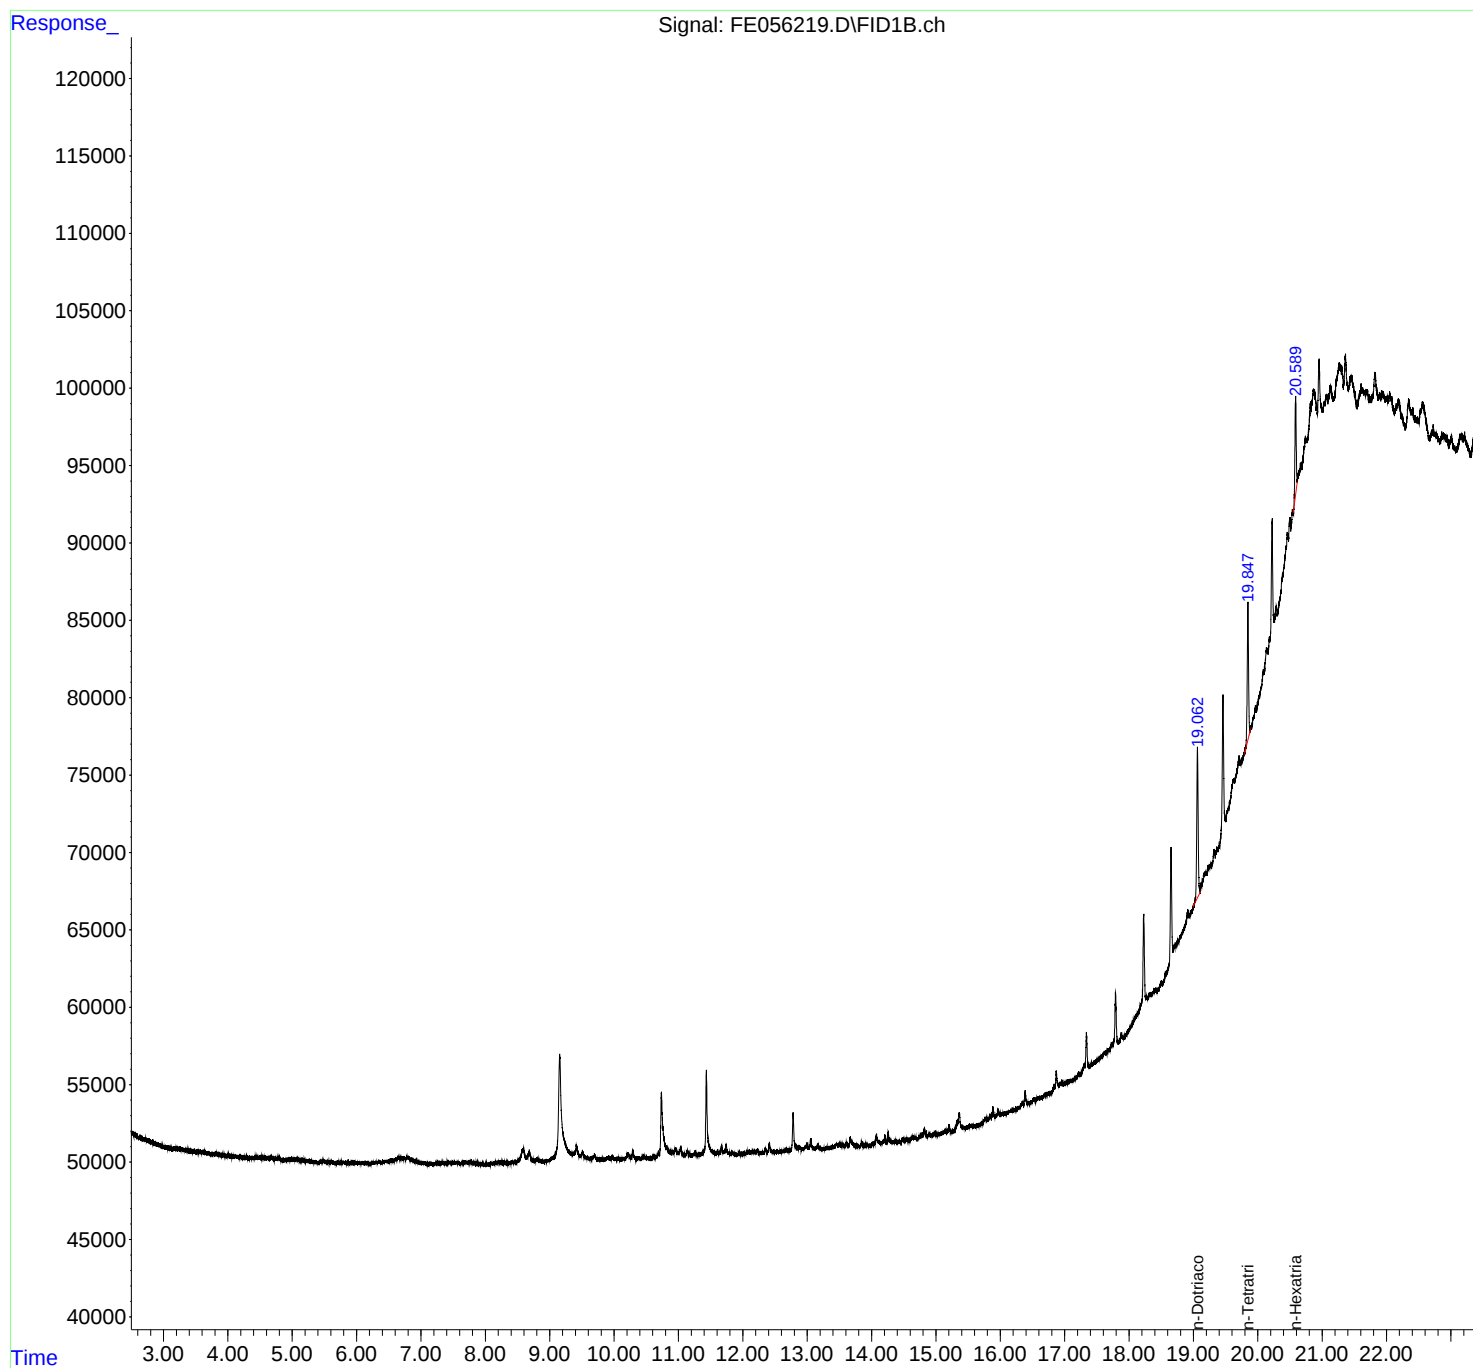


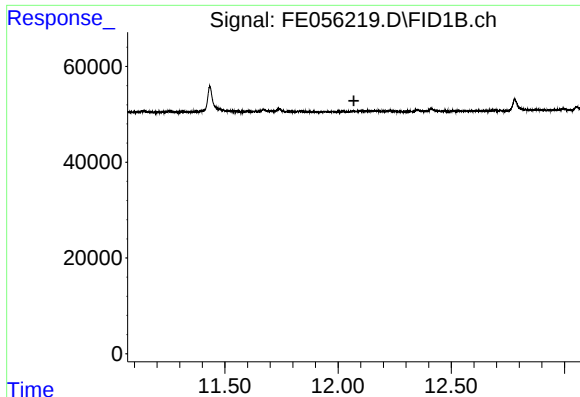

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 12.070 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
I.BLK

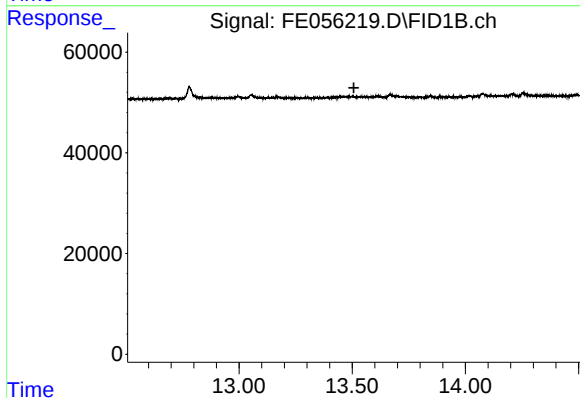


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.507 min
Response: 0
Conc: N.D.

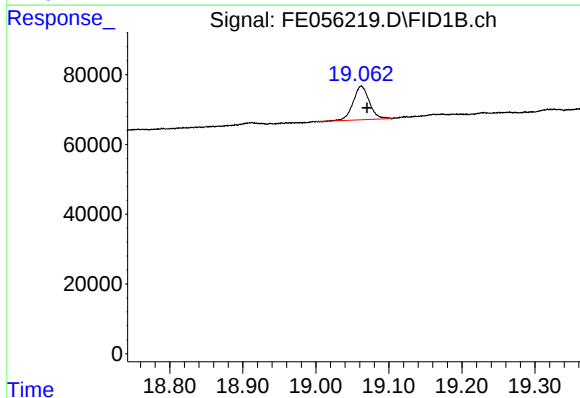


#18 n-Dotriacontane (C32)

R.T.: 19.062 min
Delta R.T.: -0.008 min
Response: 148376
Conc: 0.99 ug/ml

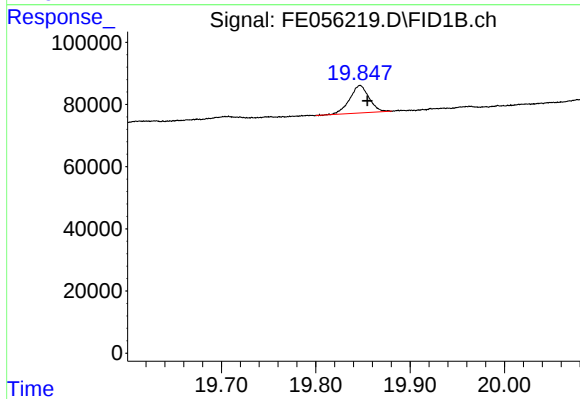

#19 n-Tetratriacontane (C34)

R.T.: 19.847 min
Delta R.T.: -0.008 min
Response: 125295
Conc: 0.89 ug/ml

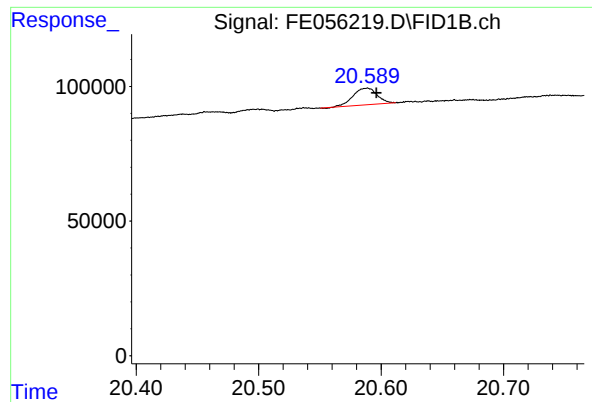

#20 n-Hexatriacontane (C36)

R.T.: 20.588 min
Delta R.T.: -0.008 min
Response: 83940
Conc: 0.65 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK