

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100722\
Data File : FE037997.D
Signal(s) : FID1B.ch
Acq On : 07 Oct 2022 11:37
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 08 20:48:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100522.M
Quant Title :
QLast Update : Wed Oct 05 16:55:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.430	2392042	17.110 ug/ml
12) N-OCTACOSANE	16.828	2310665	16.422 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100722\
Data File : FE037997.D
Signal(s) : FID1B.ch
Acq On : 07 Oct 2022 11:37
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 08 20:48:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100522.M
Quant Title :
QLast Update : Wed Oct 05 16:55:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

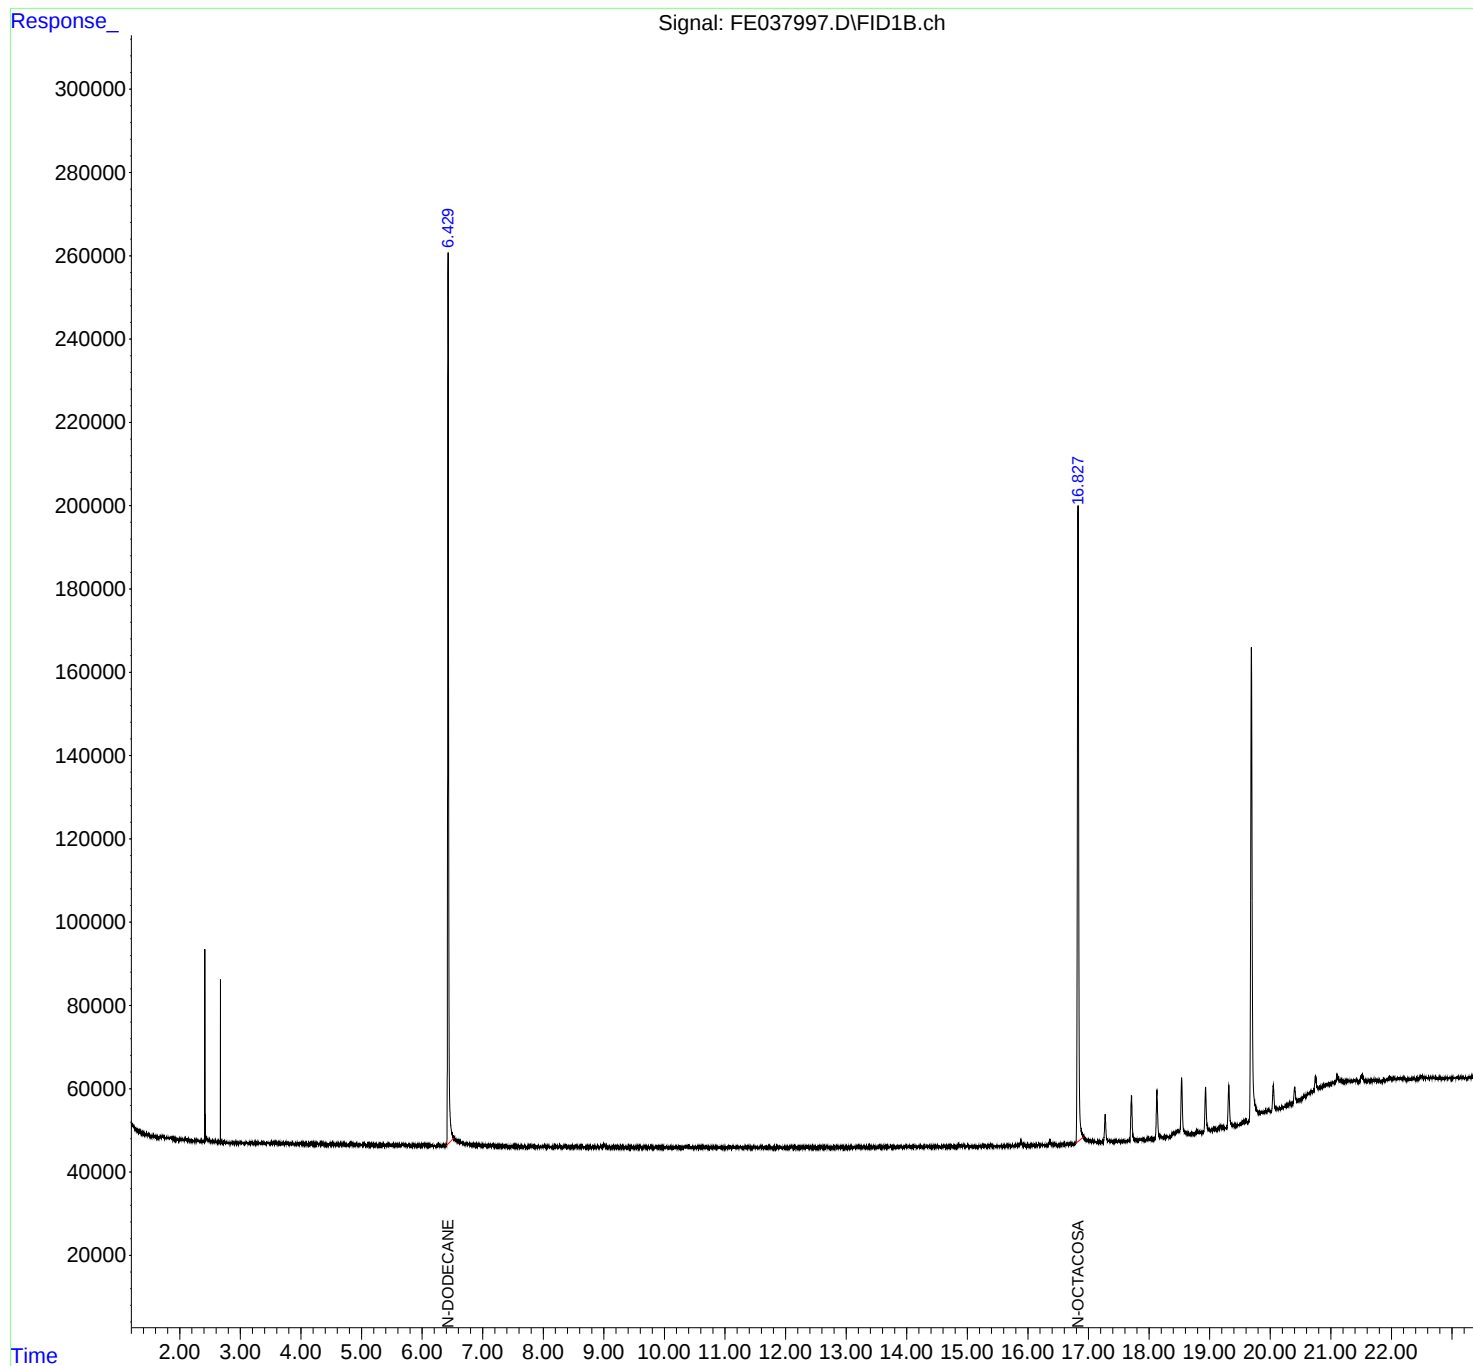


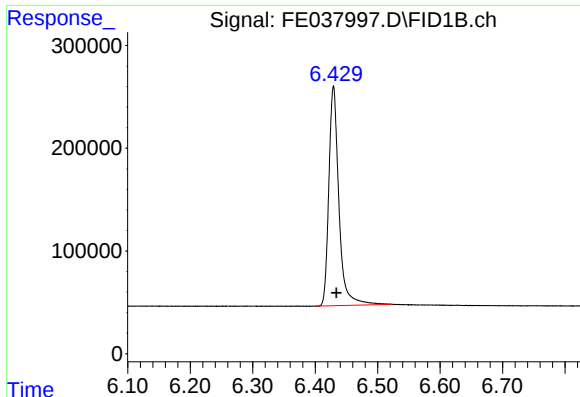

#3 N-DODECANE


R.T.: 6.430 min
Delta R.T.: -0.004 min
Response: 2392042
Conc: 17.11 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

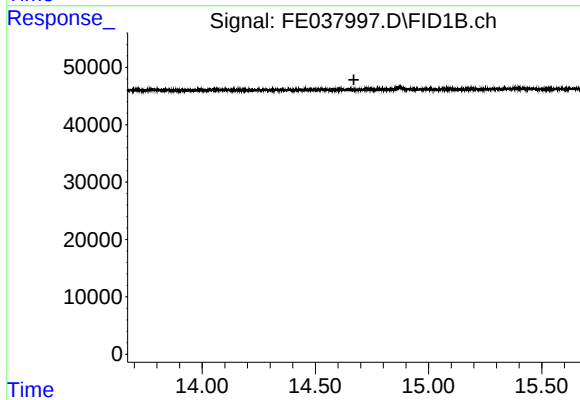

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.670 min
Response: 0
Conc: N.D.

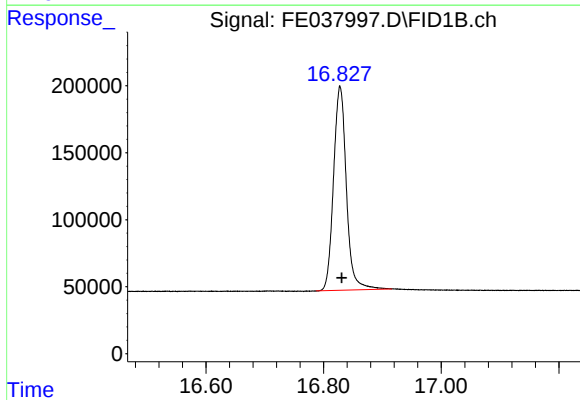

#12 N-OCTACOSANE

R.T.: 16.828 min
Delta R.T.: -0.003 min
Response: 2310665
Conc: 16.42 ug/ml